

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056903.D
 Acq On : 9 Mar 2023 6:52
 Operator : CG/JU
 Sample : PB151235BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.691	20	26	30	rBV3	3561	5969	0.93%	0.102%
2	3.903	61	62	67	rBV2	739	1070	0.17%	0.018%
3	4.067	86	90	91	rBV	644	868	0.14%	0.015%
4	4.126	97	100	110	rBV	55334	95505	14.91%	1.624%
5	4.220	114	116	121	rVB2	612	855	0.13%	0.015%
6	4.490	159	162	164	rVB2	1184	1375	0.21%	0.023%
7	5.166	273	277	279	rBV	618	858	0.13%	0.015%
8	7.540	674	681	688	rBV	70647	119140	18.60%	2.026%
9	7.716	706	711	720	rVB	49824	81631	12.75%	1.388%
10	7.939	741	749	756	rBB	63147	107074	16.72%	1.821%
11	8.415	824	830	837	rVB	58319	97200	15.18%	1.653%
12	9.102	941	947	956	rBB	80812	139237	21.74%	2.368%
13	9.590	1022	1030	1038	rBB2	67376	118102	18.44%	2.009%
14	10.325	1148	1155	1162	rVB2	56889	101656	15.87%	1.729%
15	10.859	1238	1246	1254	rBV	85130	147807	23.08%	2.514%
16	11.259	1306	1314	1322	rBB	82320	147159	22.98%	2.503%
17	11.382	1328	1335	1343	rVB	84054	150522	23.50%	2.560%
18	12.810	1573	1578	1584	rVB2	923	1443	0.23%	0.025%
19	13.903	1758	1764	1769	rVB2	1044	1322	0.21%	0.022%
20	14.414	1845	1851	1857	rBV	200429	283023	44.19%	4.814%
21	14.731	1898	1905	1913	rVB2	196755	303496	47.39%	5.162%
22	15.031	1949	1956	1963	rBV	164446	248256	38.76%	4.223%
23	15.189	1977	1983	1994	rBV	98306	158096	24.69%	2.689%
24	16.012	2116	2123	2131	rVB	265005	405006	63.24%	6.889%
25	16.118	2134	2141	2148	rBV	97859	146132	22.82%	2.486%
26	17.769	2416	2422	2430	rVB	243458	373262	58.28%	6.349%
27	17.869	2432	2439	2447	rVV	346778	507602	79.26%	8.634%
28	19.702	2747	2751	2754	rBV	4571	5305	0.83%	0.090%
29	19.772	2758	2763	2767	rVB	4009	5555	0.87%	0.094%
30	20.007	2798	2803	2806	rBV3	1320	2600	0.41%	0.044%
31	20.137	2818	2825	2831	rVB	447628	640417	100.00%	10.893%
32	20.260	2844	2846	2848	rVB2	955	895	0.14%	0.015%
33	20.953	2962	2964	2970	rBV3	1333	2620	0.41%	0.045%
34	21.000	2970	2972	2974	rBV2	1034	985	0.15%	0.017%
35	21.182	3001	3003	3006	rBV3	1288	1469	0.23%	0.025%
36	21.235	3010	3012	3013	rBV2	1493	1074	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056903.D
 Acq On : 9 Mar 2023 6:52
 Operator : CG/JU
 Sample : PB151235BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	21.823	3111	3112	3115	rVB2	2450	1474	0.23%	0.025%
38	22.093	3151	3158	3169	rVB2	251247	433880	67.75%	7.380%
39	24.326	3536	3538	3540	rBV3	1363	1123	0.18%	0.019%
40	24.567	3575	3579	3585	rBV5	4039	7692	1.20%	0.131%
41	25.154	3677	3679	3683	rBV3	2639	3006	0.47%	0.051%
42	25.395	3709	3720	3733	rVB2	203114	601193	93.88%	10.226%
43	25.648	3752	3763	3775	rVB2	139392	416405	65.02%	7.083%
44	28.397	4229	4231	4233	rBV3	2678	2213	0.35%	0.038%
45	28.679	4277	4279	4281	rBV3	1555	1440	0.22%	0.024%
46	30.219	4539	4541	4542	rBV	2477	1715	0.27%	0.029%
47	30.613	4606	4608	4610	rBV2	1766	1420	0.22%	0.024%
48	30.877	4651	4653	4654	rBV	1677	1069	0.17%	0.018%
49	31.212	4708	4710	4712	rBV3	1500	1066	0.17%	0.018%
50	31.852	4817	4819	4820	rBV2	1578	986	0.15%	0.017%




Sum of corrected areas: 5879268

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056903.D
Acq On : 9 Mar 2023 6:52
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

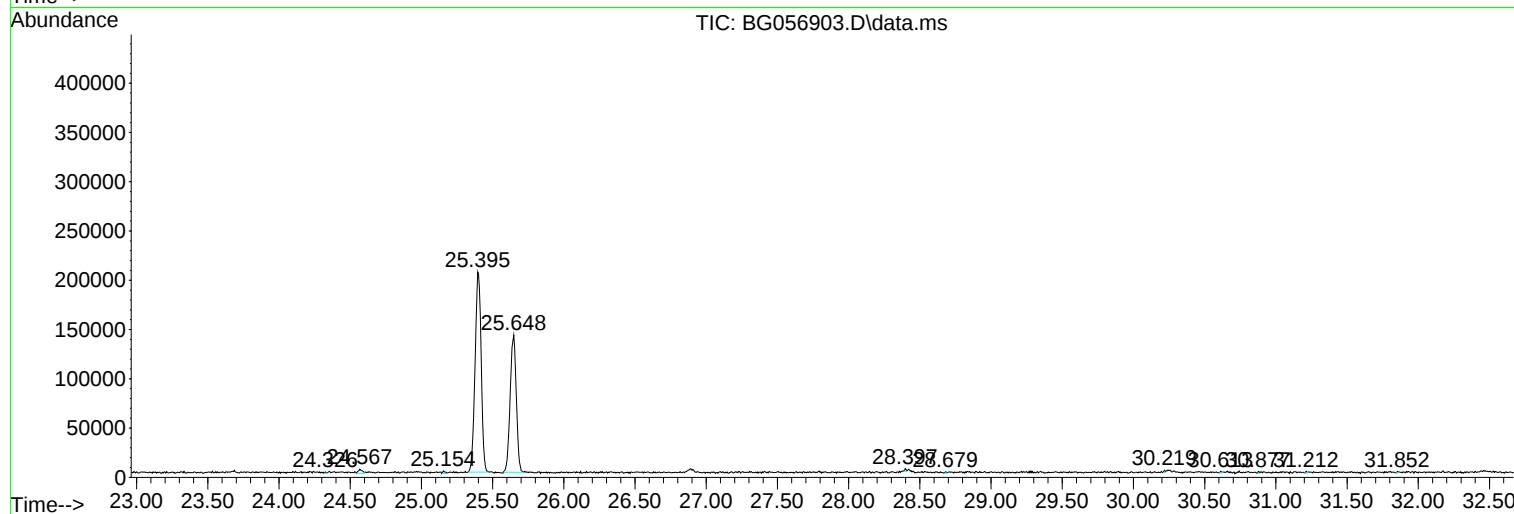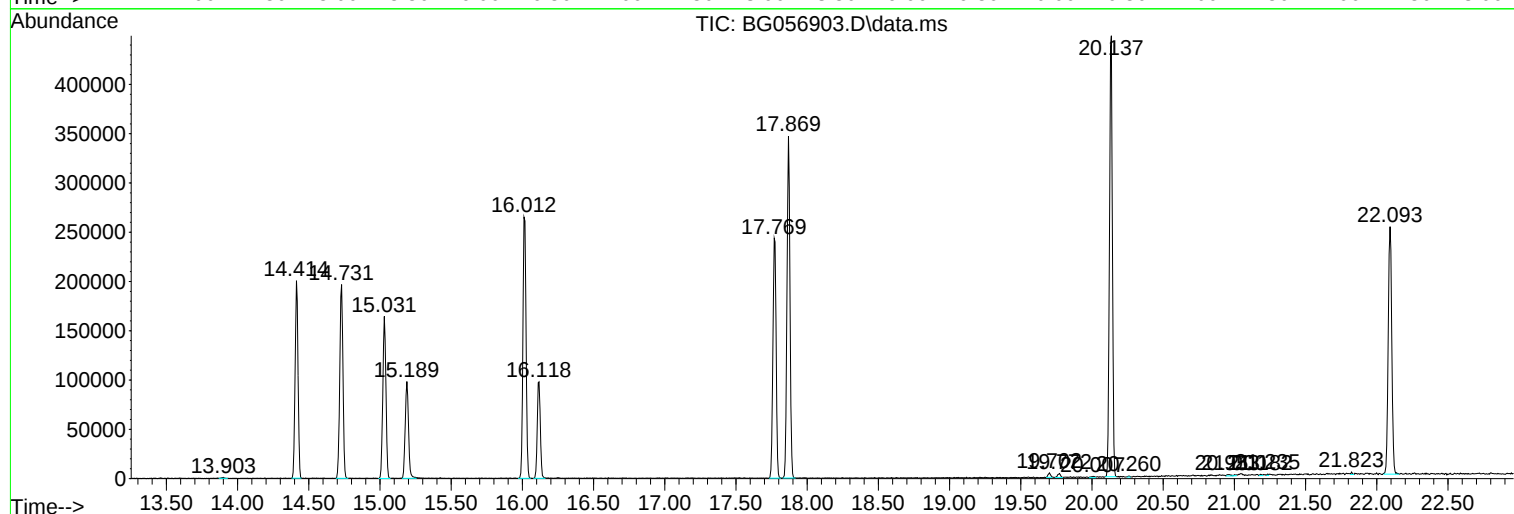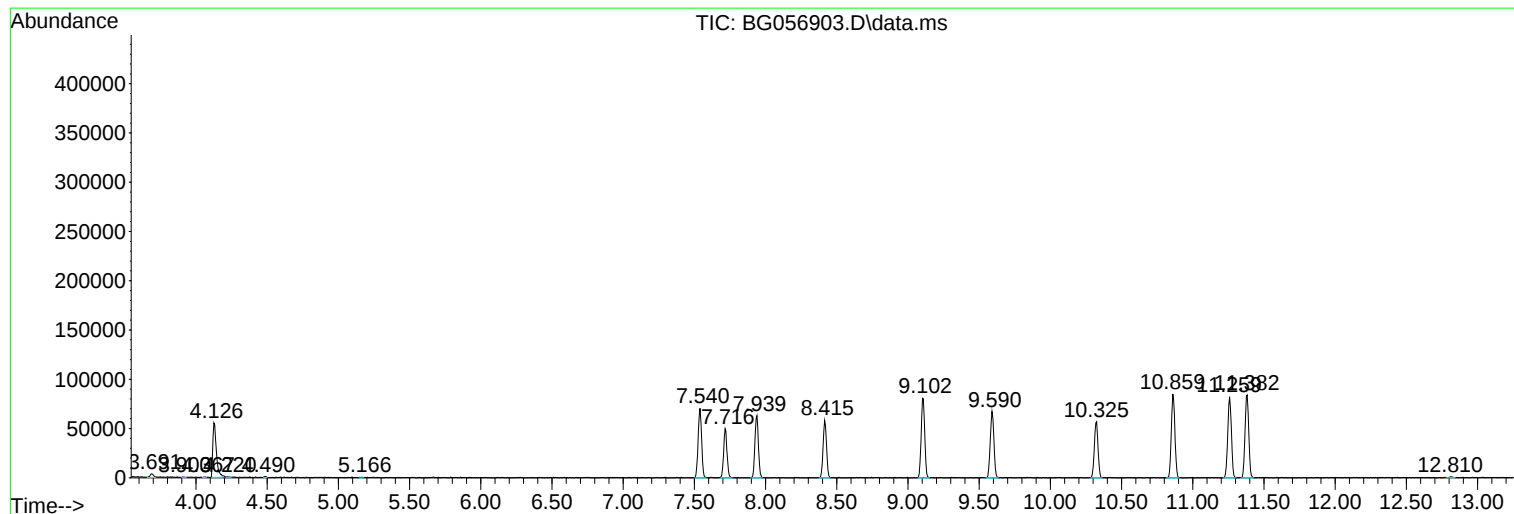

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056903.D
Acq On : 9 Mar 2023 6:52
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056903.D
Acq On : 9 Mar 2023 6:52
Operator : CG/JU
Sample : PB151235BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc