

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056909.D
 Acq On : 9 Mar 2023 11:00
 Operator : CG/JU
 Sample : 01713-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.608	10	12	14	rVB3	1339	815	0.22%	0.023%
2	3.690	23	26	31	rVB4	1636	2563	0.69%	0.072%
3	3.972	72	74	75	rBV2	1132	797	0.21%	0.022%
4	4.160	102	106	108	rBV4	916	1355	0.36%	0.038%
5	4.248	117	121	123	rBV4	2944	4154	1.11%	0.117%
6	4.331	132	135	139	rVB2	955	1064	0.28%	0.030%
7	4.384	139	144	148	rVB3	2674	4958	1.33%	0.139%
8	4.436	151	153	155	rBV	883	808	0.22%	0.023%
9	4.483	159	161	165	rVB4	1008	1213	0.32%	0.034%
10	4.595	178	180	183	rVB3	1216	1268	0.34%	0.036%
11	4.701	196	198	202	rBV3	660	932	0.25%	0.026%
12	4.824	217	219	222	rBV3	673	827	0.22%	0.023%
13	5.435	319	323	329	rVB2	5410	7435	1.99%	0.209%
14	5.518	335	337	340	rBV	798	1009	0.27%	0.028%
15	6.146	442	444	447	rBV2	552	849	0.23%	0.024%
16	6.393	483	486	489	rBV2	802	1429	0.38%	0.040%
17	6.757	545	548	552	rBV3	1184	1475	0.39%	0.041%
18	6.933	575	578	580	rBV3	742	1063	0.28%	0.030%
19	6.969	582	584	588	rVV2	697	980	0.26%	0.027%
20	7.539	675	681	687	rBV2	30935	53617	14.34%	1.504%
21	7.721	706	712	718	rBV2	22542	37320	9.98%	1.047%
22	7.938	743	749	755	rBV2	28928	47062	12.58%	1.320%
23	8.420	823	831	838	rBV	55145	95364	25.50%	2.675%
24	8.520	844	848	851	rVB3	492	803	0.21%	0.023%
25	8.720	879	882	886	rVB2	726	880	0.24%	0.025%
26	8.902	910	913	914	rBV	969	876	0.23%	0.025%
27	9.102	942	947	954	rVB2	25961	43753	11.70%	1.227%
28	9.201	961	964	967	rBV	704	967	0.26%	0.027%
29	9.243	967	971	978	rVB2	3119	5570	1.49%	0.156%
30	9.589	1022	1030	1036	rVB2	31778	55033	14.72%	1.544%
31	9.965	1091	1094	1100	rVV4	1439	2028	0.54%	0.057%
32	10.324	1148	1155	1161	rVB	27138	47082	12.59%	1.321%
33	10.805	1235	1237	1240	rBV	620	877	0.23%	0.025%
34	10.864	1240	1247	1253	rVB	36259	64606	17.27%	1.812%
35	11.258	1307	1314	1322	rBV	78965	139476	37.29%	3.912%
36	11.381	1329	1335	1341	rVB3	26118	44979	12.03%	1.262%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056909.D
 Acq On : 9 Mar 2023 11:00
 Operator : CG/JU
 Sample : 01713-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

37	12.198	1470	1474	1477	rVB3	516	854	0.23%	0.024%
38	12.427	1509	1513	1515	rBV3	640	845	0.23%	0.024%
39	12.686	1552	1557	1558	rBV	689	899	0.24%	0.025%
40	13.320	1663	1665	1669	rBV	513	906	0.24%	0.025%
41	13.655	1721	1722	1729	rVB	602	998	0.27%	0.028%
42	13.890	1759	1762	1764	rBV	1294	934	0.25%	0.026%
43	13.943	1767	1771	1775	rVB	586	806	0.22%	0.023%
44	14.413	1845	1851	1859	rVB	87343	124027	33.16%	3.479%
45	14.724	1897	1904	1911	rBV	87376	140131	37.47%	3.930%
46	15.030	1950	1956	1965	rVB	152473	232573	62.19%	6.523%
47	15.189	1977	1983	1990	rBV2	28192	43169	11.54%	1.211%
48	15.412	2018	2021	2025	rVB3	1634	1871	0.50%	0.052%
49	16.017	2116	2124	2131	rVB	126661	189993	50.80%	5.329%
50	16.111	2136	2140	2147	rVB2	35472	54138	14.48%	1.518%
51	16.364	2179	2183	2189	rVB	10294	14660	3.92%	0.411%
52	17.286	2336	2340	2344	rVB	2620	3122	0.83%	0.088%
53	17.774	2416	2423	2429	rVV	219543	336702	90.03%	9.443%
54	17.868	2433	2439	2446	rVV	145278	213840	57.18%	5.998%
55	17.932	2446	2450	2454	rVB2	2632	3253	0.87%	0.091%
56	18.608	2560	2565	2571	rBV2	19625	25468	6.81%	0.714%
57	18.984	2627	2629	2632	rVB	660	861	0.23%	0.024%
58	19.025	2632	2636	2641	rBV	5575	6607	1.77%	0.185%
59	19.137	2653	2655	2659	rVB	780	813	0.22%	0.023%
60	19.295	2680	2682	2685	rBV	838	828	0.22%	0.023%
61	19.560	2723	2727	2729	rVB	799	918	0.25%	0.026%
62	19.613	2734	2736	2738	rVV	1025	1138	0.30%	0.032%
63	19.636	2738	2740	2741	rVV	1685	1076	0.29%	0.030%
64	19.666	2741	2745	2746	rVV3	1616	1663	0.44%	0.047%
65	19.701	2747	2751	2754	rVV5	3838	4995	1.34%	0.140%
66	19.765	2758	2762	2767	rVB3	2455	3334	0.89%	0.094%
67	19.871	2775	2780	2782	rBV3	3310	4158	1.11%	0.117%
68	19.959	2792	2795	2797	rBV2	774	917	0.25%	0.026%
69	20.012	2799	2804	2807	rBV4	1964	3042	0.81%	0.085%
70	20.059	2810	2812	2813	rBV	976	797	0.21%	0.022%
71	20.136	2819	2825	2834	rVB	202012	291184	77.86%	8.167%
72	20.306	2852	2854	2856	rVB2	1553	989	0.26%	0.028%
73	20.412	2870	2872	2874	rBV2	867	925	0.25%	0.026%
74	20.453	2878	2879	2882	rBV2	1184	1001	0.27%	0.028%
75	20.553	2893	2896	2900	rBV2	8022	10825	2.89%	0.304%
76	20.758	2929	2931	2932	rBV3	1413	1061	0.28%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
 Data File : BG056909.D
 Acq On : 9 Mar 2023 11:00
 Operator : CG/JU
 Sample : 01713-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
 Title : SVOA CALIBRATION

77	20.941	2960	2962	2963	rBV2	1588	1078	0.29%	0.030%
78	21.058	2978	2982	2983	rBV2	3130	2998	0.80%	0.084%
79	21.087	2985	2987	2990	rVV2	6124	6570	1.76%	0.184%
80	21.117	2990	2992	2996	rVB4	4065	5160	1.38%	0.145%
81	21.152	2996	2998	3003	rBV4	1659	2102	0.56%	0.059%
82	21.575	3068	3070	3075	rVB5	3337	3909	1.05%	0.110%
83	21.663	3080	3085	3091	rBV2	29928	53113	14.20%	1.490%
84	21.934	3126	3131	3136	rVB	22193	32775	8.76%	0.919%
85	22.092	3151	3158	3165	rVV2	218575	373991	100.00%	10.489%
86	22.145	3165	3167	3168	rVB2	1657	812	0.22%	0.023%
87	22.251	3182	3185	3186	rBV3	2593	2808	0.75%	0.079%
88	22.527	3228	3232	3236	rVB5	6683	8919	2.38%	0.250%
89	22.727	3264	3266	3267	rBV	1593	1233	0.33%	0.035%
90	22.921	3294	3299	3300	rBV3	4948	7405	1.98%	0.208%
91	25.400	3711	3721	3732	rVB	88745	262225	70.12%	7.355%
92	25.641	3752	3762	3774	rVB2	119833	368095	98.42%	10.324%
93	25.899	3804	3806	3807	rBV2	1733	1166	0.31%	0.033%
94	26.199	3855	3857	3863	rBV6	2190	3229	0.86%	0.091%
95	26.892	3967	3975	3981	rBV8	6220	18253	4.88%	0.512%
96	27.639	4100	4102	4103	rBV2	1552	1171	0.31%	0.033%
97	27.862	4139	4140	4143	rBV3	2223	1567	0.42%	0.044%
98	29.272	4378	4380	4381	rBV	2176	1444	0.39%	0.040%
99	30.001	4502	4504	4505	rBV2	2323	1715	0.46%	0.048%
100	30.400	4570	4572	4576	rVB4	2118	2091	0.56%	0.059%




Sum of corrected areas: 3565437

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056909.D
Acq On : 9 Mar 2023 11:00
Operator : CG/JU
Sample : 01713-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

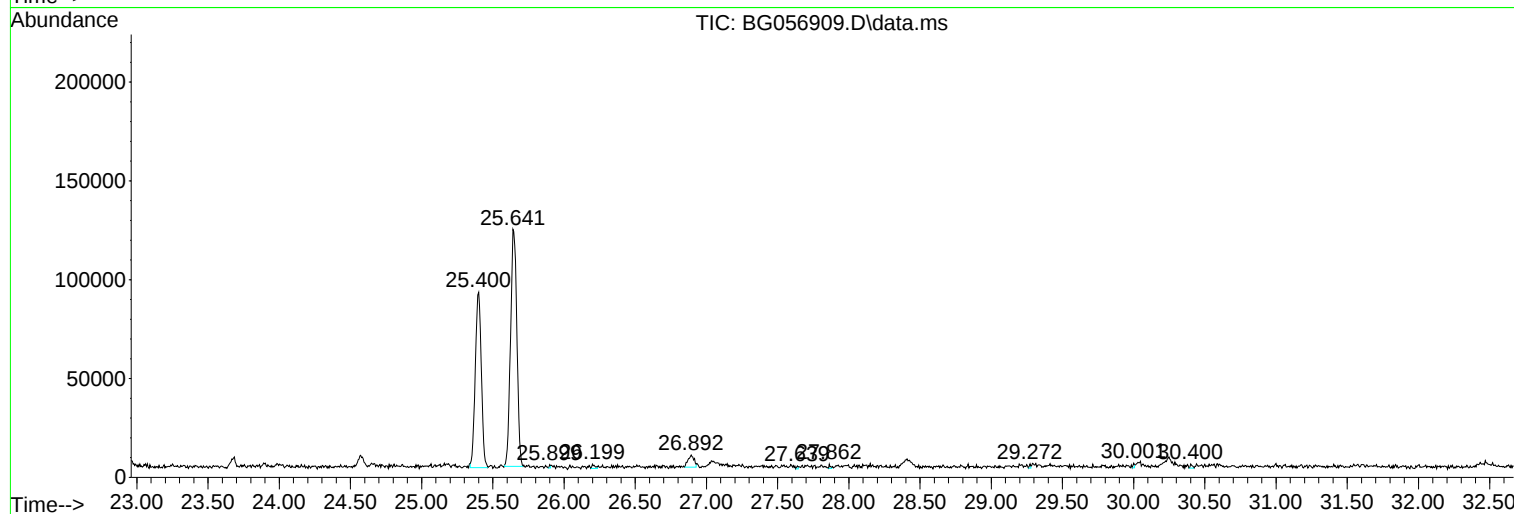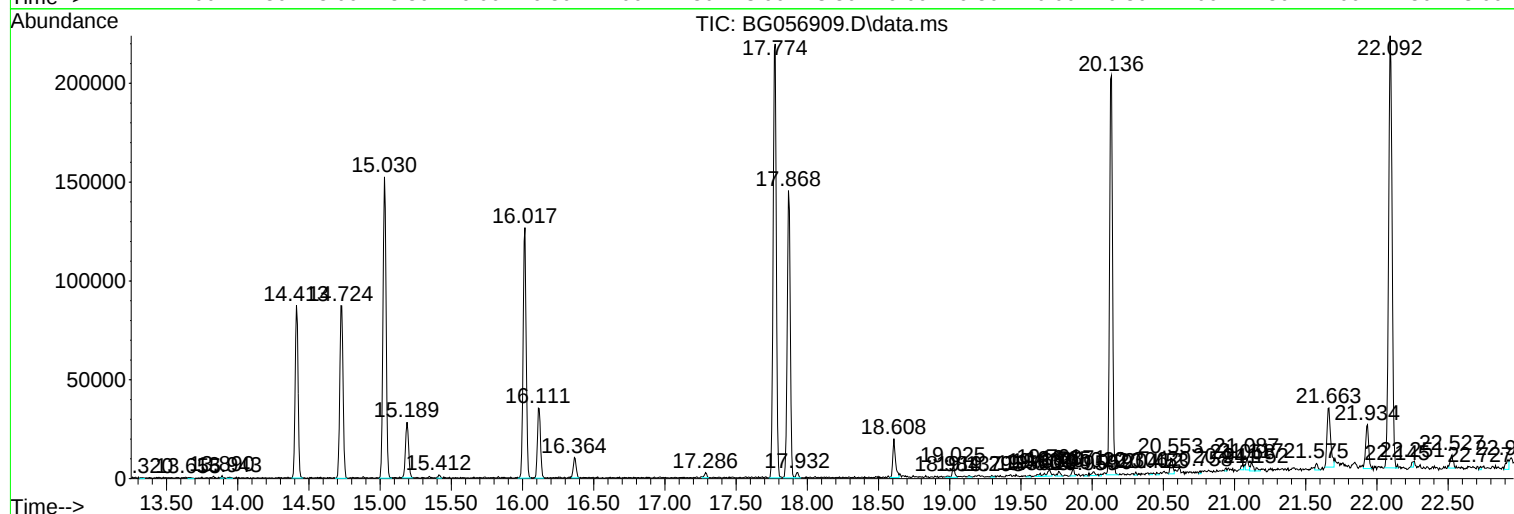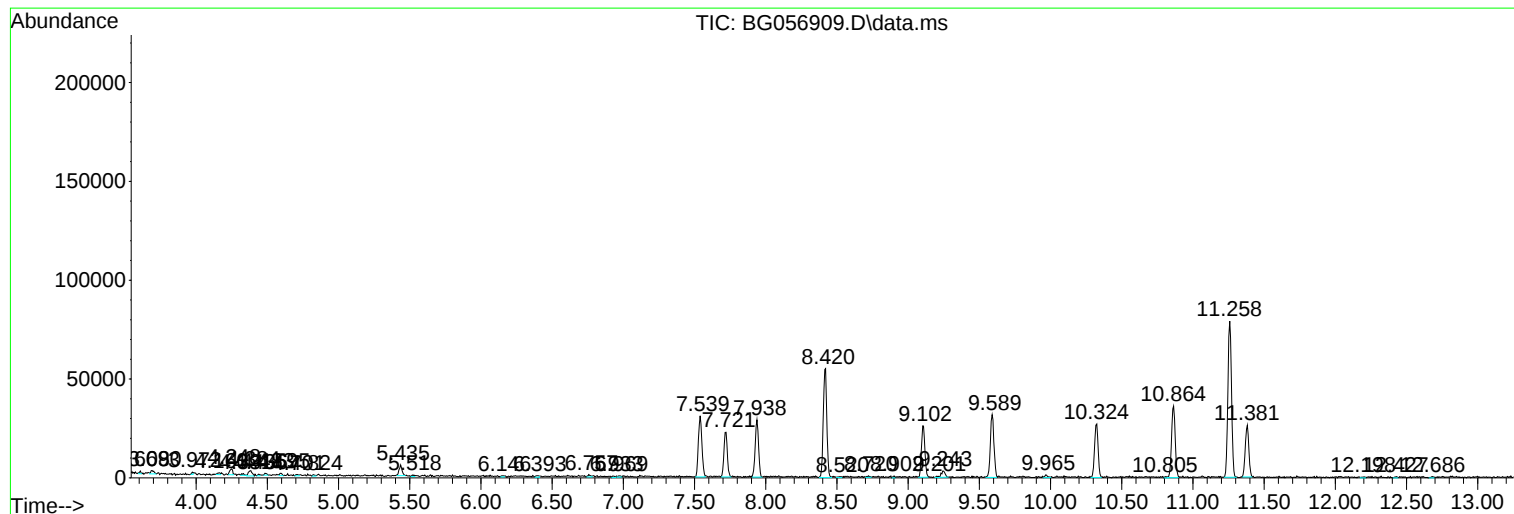

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056909.D
Acq On : 9 Mar 2023 11:00
Operator : CG/JU
Sample : 01713-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZY6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.663	2.84 ng/ul	53113	Chrysene-d12	22.092

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
2			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	91
3			1-Hexacosene	364	C26H52	018835-33-1	91
4			Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	90
5			1-Tetracosene	336	C24H48	010192-32-2	87

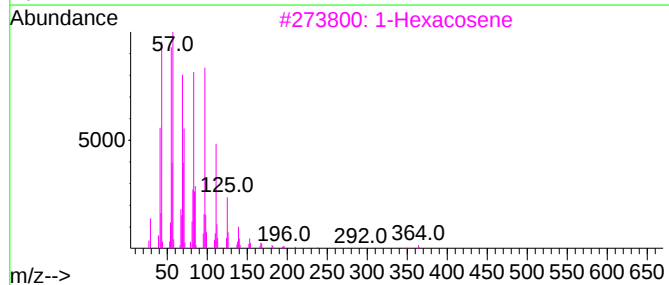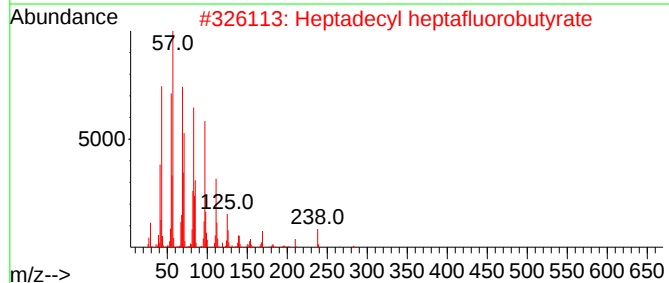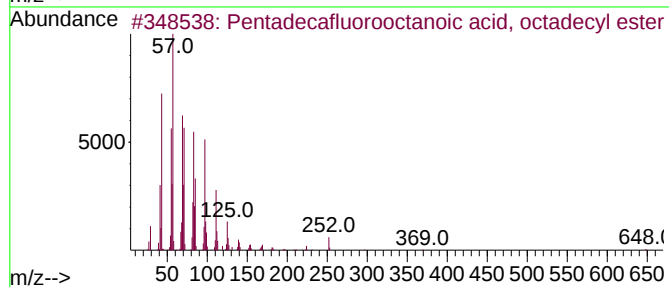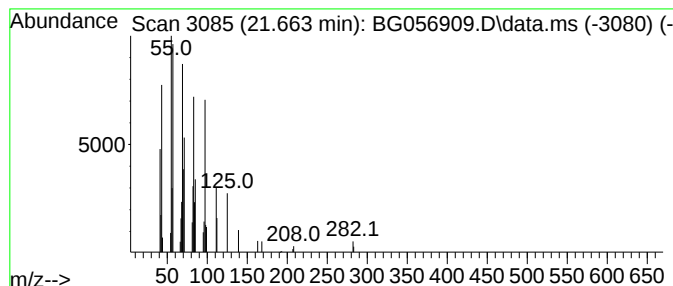

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056909.D
Acq On : 9 Mar 2023 11:00
Operator : CG/JU
Sample : 01713-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	21.663	2.8	ng/ul	53113	5	22.092	373991	20.0