


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030823\
Data File : BG056874.D
Acq On : 8 Mar 2023 8:43
Operator : CG/JU
Sample : DFTPP501
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP501

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG030723.M
Title : SVOA CALIBRATION
Last Update : Wed Mar 08 23:58:51 2023

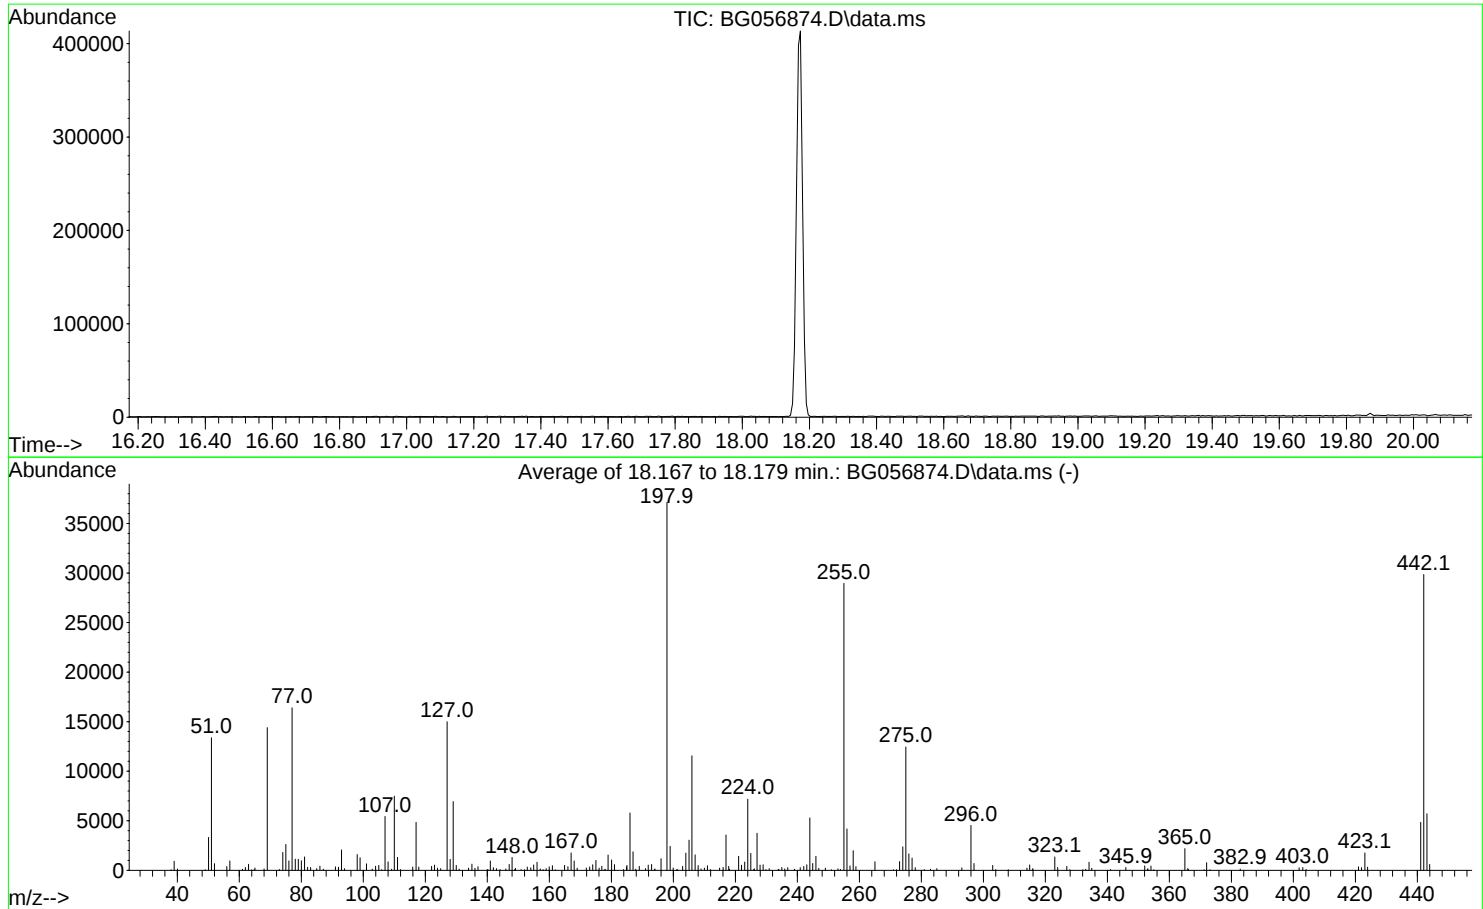

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	13382	PASS
68	69	0.00	2	0.9	136	PASS
69	198	0.00	100	38.8	14394	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.4	14988	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37123	PASS
199	198	5	9	6.5	2413	PASS
275	198	10	60	33.5	12437	PASS
365	198	1	100	5.9	2182	PASS
441	198	0.01	100	13.0	4844	PASS
442	198	50	100	80.4	29843	PASS
443	442	15	24	19.1	5708	PASS

m/z	Abundance
43.90	707.0
207.00	196.0

Instrument :

BNA_G

ClientSampleId :

DFTPP501

m/z	Abundance
38.00	181.0
39.00	1119.0
40.10	227.0
44.00	677.0
49.00	188.0
50.00	4069.0
51.00	17552.0
52.00	885.0
55.90	499.0
57.00	1054.0
61.90	296.0
63.00	585.0
65.00	410.0
68.00	407.0
69.00	17808.0
72.90	262.0
74.00	2267.0
75.00	3161.0
76.00	1320.0
77.00	20056.0
78.10	1308.0
79.00	1366.0
80.00	1142.0
81.00	1869.0
82.00	352.0
83.10	459.0
85.00	244.0
86.00	493.0
87.10	179.0
91.00	463.0
92.00	551.0
92.90	2419.0
94.00	265.0
98.00	1969.0
99.00	1443.0
101.00	666.0
102.80	155.0
104.00	530.0
105.00	809.0
105.90	192.0
107.00	6909.0
108.00	1010.0
110.00	8697.0
111.00	1418.0
112.00	197.0
115.90	415.0
117.00	5650.0
117.90	329.0
122.00	433.0
123.00	590.0
123.90	373.0
124.90	284.0
127.00	17472.0
128.00	1380.0
129.00	8329.0
130.00	611.0
130.90	182.0
133.90	176.0
135.00	764.0
136.00	262.0
137.00	441.0
140.00	225.0
140.90	1099.0
141.90	439.0
143.00	241.0
147.10	738.0
148.00	1264.0
149.00	290.0
152.00	159.0
152.90	427.0
154.00	246.0
155.00	644.0
156.10	1020.0
157.00	226.0
159.00	174.0
159.90	383.0
161.00	708.0
161.90	162.0
164.90	542.0
166.00	472.0
167.00	1924.0
168.00	1122.0
169.00	219.0
171.90	373.0
173.00	339.0
174.00	725.0
175.00	940.0
176.10	352.0
177.00	561.0
177.70	151.0
178.10	181.0
178.90	1835.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

180.00	1136.0
181.00	695.0
183.90	216.0
184.90	1026.0
186.00	6243.0
187.00	2153.0
189.10	459.0
191.00	221.0
191.90	624.0
193.00	672.0
193.90	239.0
196.00	1302.0
198.00	41192.0
198.90	2441.0
199.90	239.0
201.10	150.0
203.00	410.0
204.00	1939.0
205.00	3512.0
206.00	13425.0
207.00	1627.0
208.00	547.0
208.90	183.0
210.00	356.0
211.00	654.0
214.90	210.0
216.10	289.0
217.00	4340.0
217.80	291.0
218.10	337.0
221.00	1733.0
222.00	408.0
223.00	795.0
224.00	7924.0
225.00	1878.0
225.90	227.0
227.00	3659.0
227.90	494.0
229.00	670.0
230.90	253.0
233.80	220.0
235.00	341.0
236.00	195.0
237.00	322.0
240.90	336.0
242.00	353.0
243.00	525.0
244.00	5780.0
244.90	843.0
246.00	1722.0
246.90	270.0
249.00	268.0
251.00	150.0
253.10	240.0
255.00	31104.0
256.00	4357.0
257.00	391.0
258.00	2140.0
259.00	373.0
265.00	922.0
271.00	157.0
273.00	889.0
274.00	2277.0
275.00	13598.0
275.90	1701.0
277.00	1148.0
278.10	259.0
280.90	200.0
282.90	170.0
285.10	247.0
293.00	292.0
296.00	4696.0
296.90	589.0
303.00	593.0
304.00	208.0
314.10	235.0
314.90	608.0
315.80	280.0
323.00	1126.0
323.90	266.0
326.90	345.0
327.90	168.0
332.10	176.0
333.00	155.0
334.10	597.0
334.90	198.0
345.90	200.0
352.00	443.0
352.90	337.0
354.10	531.0
365.00	2146.0
365.90	218.0
371.20	188.0
372.00	824.0
401.90	215.0
403.00	368.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

421.00	438.0
422.00	316.0
423.10	1810.0
424.00	384.0
441.10	4497.0
442.00	28032.0
443.10	5371.0
443.90	447.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

m/z	Abundance
39.00	1245.0
44.00	701.0
50.10	3680.0
51.00	14972.0
52.00	722.0
56.00	468.0
56.90	1238.0
61.00	300.0
62.00	342.0
62.90	789.0
65.10	277.0
69.00	16944.0
74.00	1968.0
75.00	3158.0
76.00	895.0
77.00	18432.0
78.00	1484.0
79.00	1237.0
80.00	1221.0
81.10	1270.0
82.00	373.0
82.90	409.0
84.90	287.0
86.00	331.0
87.00	177.0
91.00	380.0
92.00	237.0
93.00	2370.0
93.90	259.0
98.00	1761.0
99.00	1355.0
101.00	790.0
103.90	417.0
105.00	487.0
107.00	6198.0
108.00	1102.0
109.10	320.0
110.00	8938.0
111.00	1512.0
116.00	379.0
117.00	5644.0
117.90	334.0
122.00	591.0
123.00	659.0
123.90	295.0
125.00	214.0
127.00	17520.0
128.00	1369.0
129.00	7343.0
129.90	541.0
134.00	280.0
135.00	676.0
136.00	347.0
137.00	382.0
140.20	204.0
141.00	1093.0
142.00	350.0
142.90	297.0
144.10	218.0
146.00	211.0
147.00	606.0
148.00	1814.0
149.10	337.0
150.90	207.0
153.00	361.0
154.00	355.0
154.90	538.0
155.90	830.0
157.10	206.0
158.00	244.0
158.90	173.0
160.00	376.0
161.00	420.0
164.90	524.0
166.00	465.0
167.00	2081.0
168.00	945.0
169.00	219.0
171.90	316.0
173.00	461.0
174.00	624.0
175.00	1318.0
176.00	317.0
176.90	405.0
179.00	1815.0
180.10	1251.0
181.10	687.0
185.10	949.0
186.00	6602.0
187.00	2068.0
187.90	168.0
188.90	472.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

191.00	317.0
192.00	583.0
193.00	803.0
194.10	235.0
196.00	1401.0
197.90	43856.0
199.00	3104.0
200.00	255.0
203.00	487.0
204.00	2010.0
205.10	3127.0
206.00	13045.0
207.10	1985.0
208.00	465.0
209.00	236.0
210.00	313.0
211.00	498.0
211.90	216.0
215.00	247.0
216.10	333.0
216.90	3679.0
217.90	599.0
221.10	1389.0
222.00	628.0
223.00	1025.0
224.00	8360.0
225.00	1995.0
226.10	283.0
227.00	4766.0
228.00	722.0
228.90	662.0
229.90	201.0
230.90	278.0
234.00	305.0
235.00	341.0
235.80	199.0
236.80	281.0
239.10	170.0
241.00	309.0
242.00	491.0
243.10	652.0
244.00	6109.0
245.00	790.0
246.00	1493.0
246.90	320.0
249.00	229.0
253.10	203.0
255.00	34088.0
256.00	5124.0
256.90	682.0
258.00	2356.0
258.80	456.0
265.00	1035.0
272.90	1148.0
274.00	2695.0
275.00	14892.0
276.00	1927.0
277.00	1734.0
278.00	406.0
283.00	154.0
284.90	258.0
293.10	240.0
296.00	5277.0
297.00	835.0
303.00	581.0
308.00	150.0
314.00	209.0
315.00	644.0
316.00	298.0
323.00	1516.0
324.00	393.0
326.90	474.0
333.10	165.0
334.00	1071.0
335.00	219.0
341.00	238.0
346.00	373.0
352.00	501.0
353.10	238.0
354.00	465.0
355.00	176.0
365.00	2335.0
366.10	283.0
372.00	1024.0
373.10	165.0
382.90	193.0
401.80	322.0
403.00	268.0
404.10	203.0
421.00	359.0
421.90	310.0
423.00	1901.0
424.00	288.0
441.10	5785.0
442.00	35424.0
443.00	6878.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

443.90

788.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

m/z	Abundance
39.00	393.0
40.00	206.0
44.00	460.0
50.00	2221.0
51.00	7622.0
52.00	397.0
55.90	186.0
57.00	561.0
62.00	224.0
62.90	432.0
64.00	154.0
64.80	159.0
69.00	8429.0
74.00	1185.0
75.00	1494.0
76.10	642.0
77.00	10723.0
78.00	600.0
79.00	726.0
79.90	528.0
81.00	906.0
82.00	172.0
86.00	402.0
91.00	193.0
91.90	179.0
93.00	1397.0
98.00	1022.0
98.90	993.0
101.00	522.0
102.90	214.0
104.00	284.0
104.90	167.0
107.00	3183.0
108.00	444.0
110.00	4805.0
111.00	955.0
115.90	212.0
117.00	3214.0
117.90	343.0
121.90	181.0
122.80	339.0
127.00	9971.0
128.00	596.0
129.00	5155.0
130.00	342.0
130.90	196.0
134.00	207.0
134.90	452.0
137.00	255.0
141.00	647.0
145.90	184.0
147.00	417.0
148.00	803.0
148.80	184.0
152.80	206.0
154.00	161.0
155.00	458.0
156.00	610.0
159.00	181.0
160.00	284.0
161.00	276.0
164.90	393.0
166.00	151.0
167.10	1275.0
168.00	761.0
169.00	208.0
173.00	184.0
174.10	308.0
175.00	722.0
177.00	292.0
177.90	158.0
178.90	995.0
180.00	734.0
180.90	326.0
185.00	537.0
186.00	4537.0
187.00	1384.0
187.80	209.0
189.00	258.0
191.80	362.0
192.90	309.0
194.00	163.0
196.00	810.0
198.00	26320.0
198.90	1693.0
199.90	224.0
201.40	221.0
203.10	278.0
204.00	1245.0
205.00	2486.0
206.00	8193.0
207.00	1632.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501

208.00	416.0
210.90	255.0
214.80	180.0
216.00	275.0
217.00	2665.0
217.90	312.0
221.10	1097.0
222.00	474.0
223.00	655.0
224.00	5255.0
225.00	1215.0
226.10	165.0
227.00	2772.0
228.00	379.0
228.90	330.0
235.00	160.0
236.90	205.0
239.00	151.0
240.80	181.0
242.10	349.0
242.90	229.0
243.20	254.0
244.00	3993.0
245.00	448.0
246.00	1023.0
249.00	151.0
253.90	277.0
255.00	21704.0
256.00	3049.0
256.90	261.0
258.00	1458.0
259.00	268.0
265.00	628.0
272.00	173.0
273.00	615.0
274.00	2115.0
275.00	8822.0
276.00	1333.0
276.90	828.0
278.10	161.0
293.00	202.0
296.00	3603.0
297.00	629.0
303.00	312.0
314.00	207.0
314.90	349.0
315.90	235.0
323.10	1410.0
323.90	179.0
326.80	179.0
327.00	179.0
334.00	798.0
335.00	200.0
345.90	275.0
352.10	410.0
353.00	216.0
354.00	302.0
365.00	2066.0
365.90	310.0
372.10	476.0
382.80	167.0
401.90	195.0
403.00	214.0
421.00	251.0
422.00	195.0
423.10	1565.0
423.90	275.0
441.00	4249.0
442.10	26072.0
443.00	4875.0
444.00	523.0

Instrument :
BNA_G
ClientSampleId :
DFTPP501