




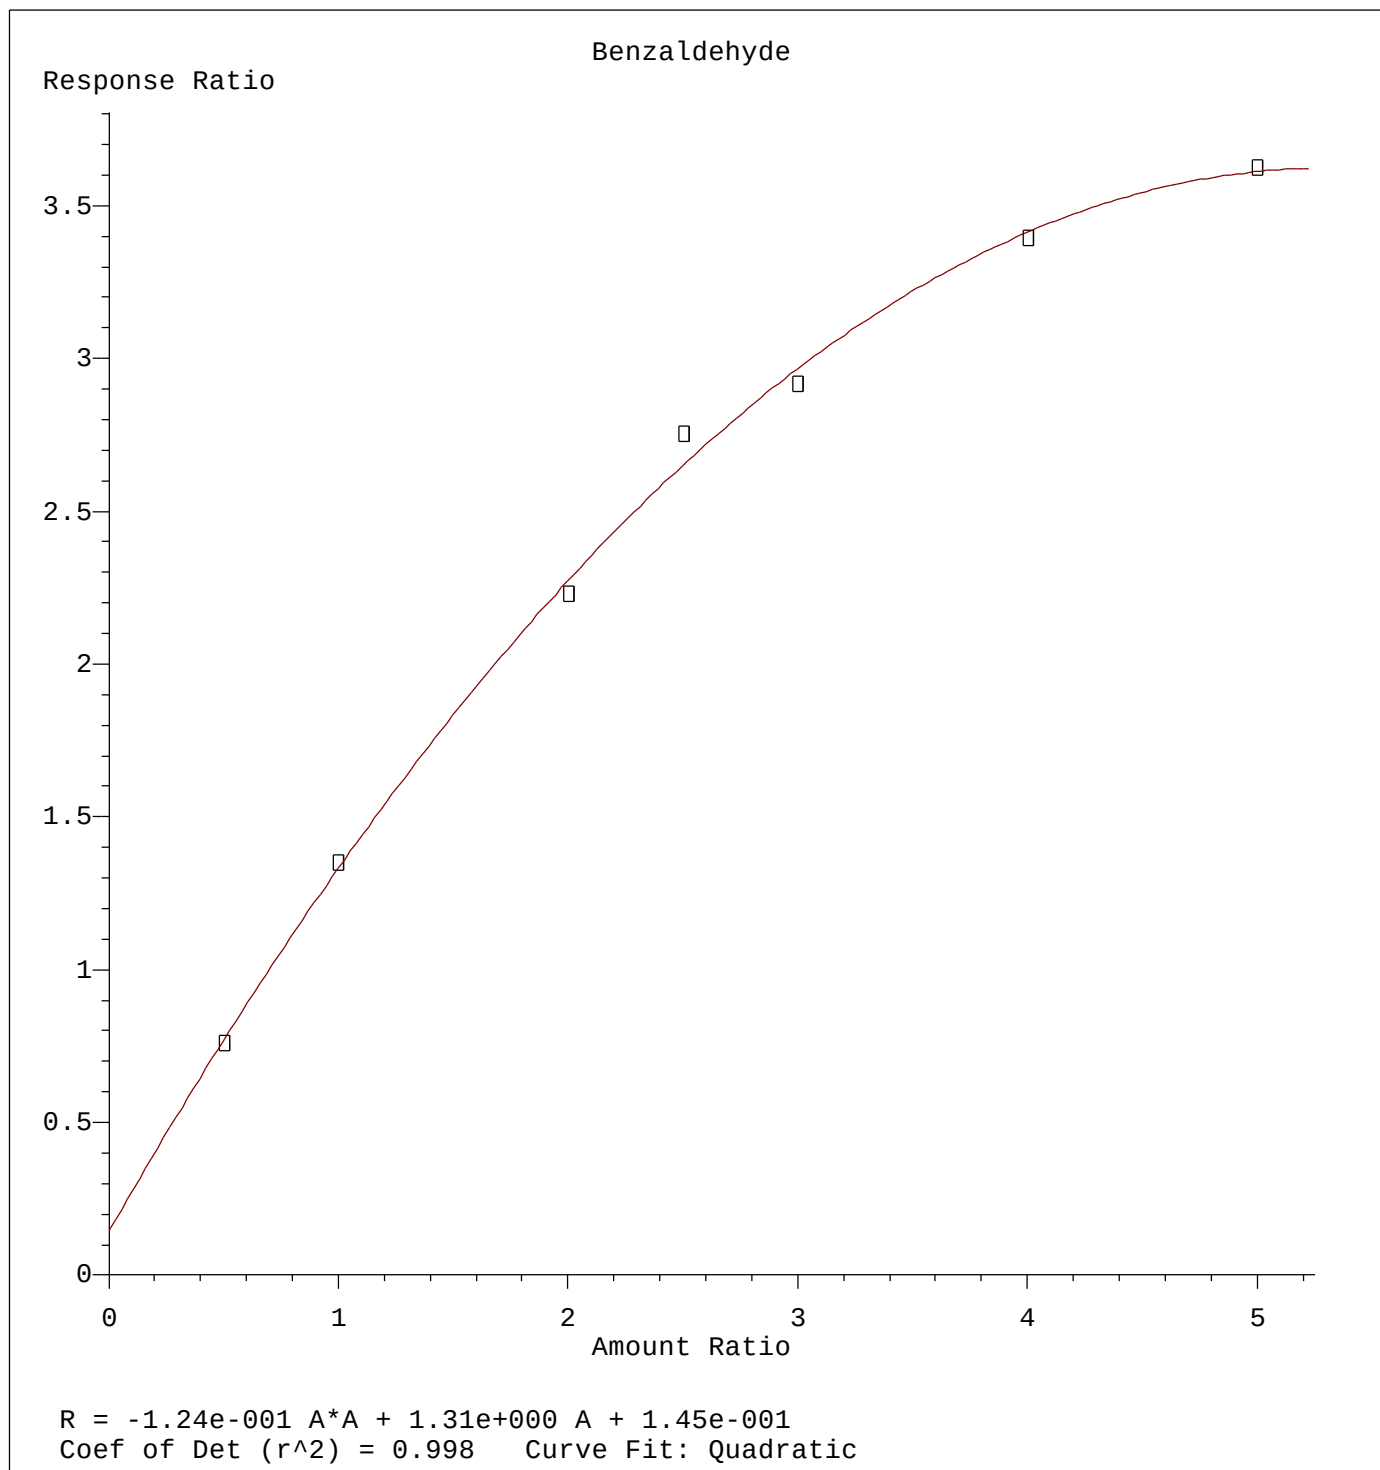

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031020.M  
Calibration Table Last Updated: Tue Mar 10 16:27:39 2020

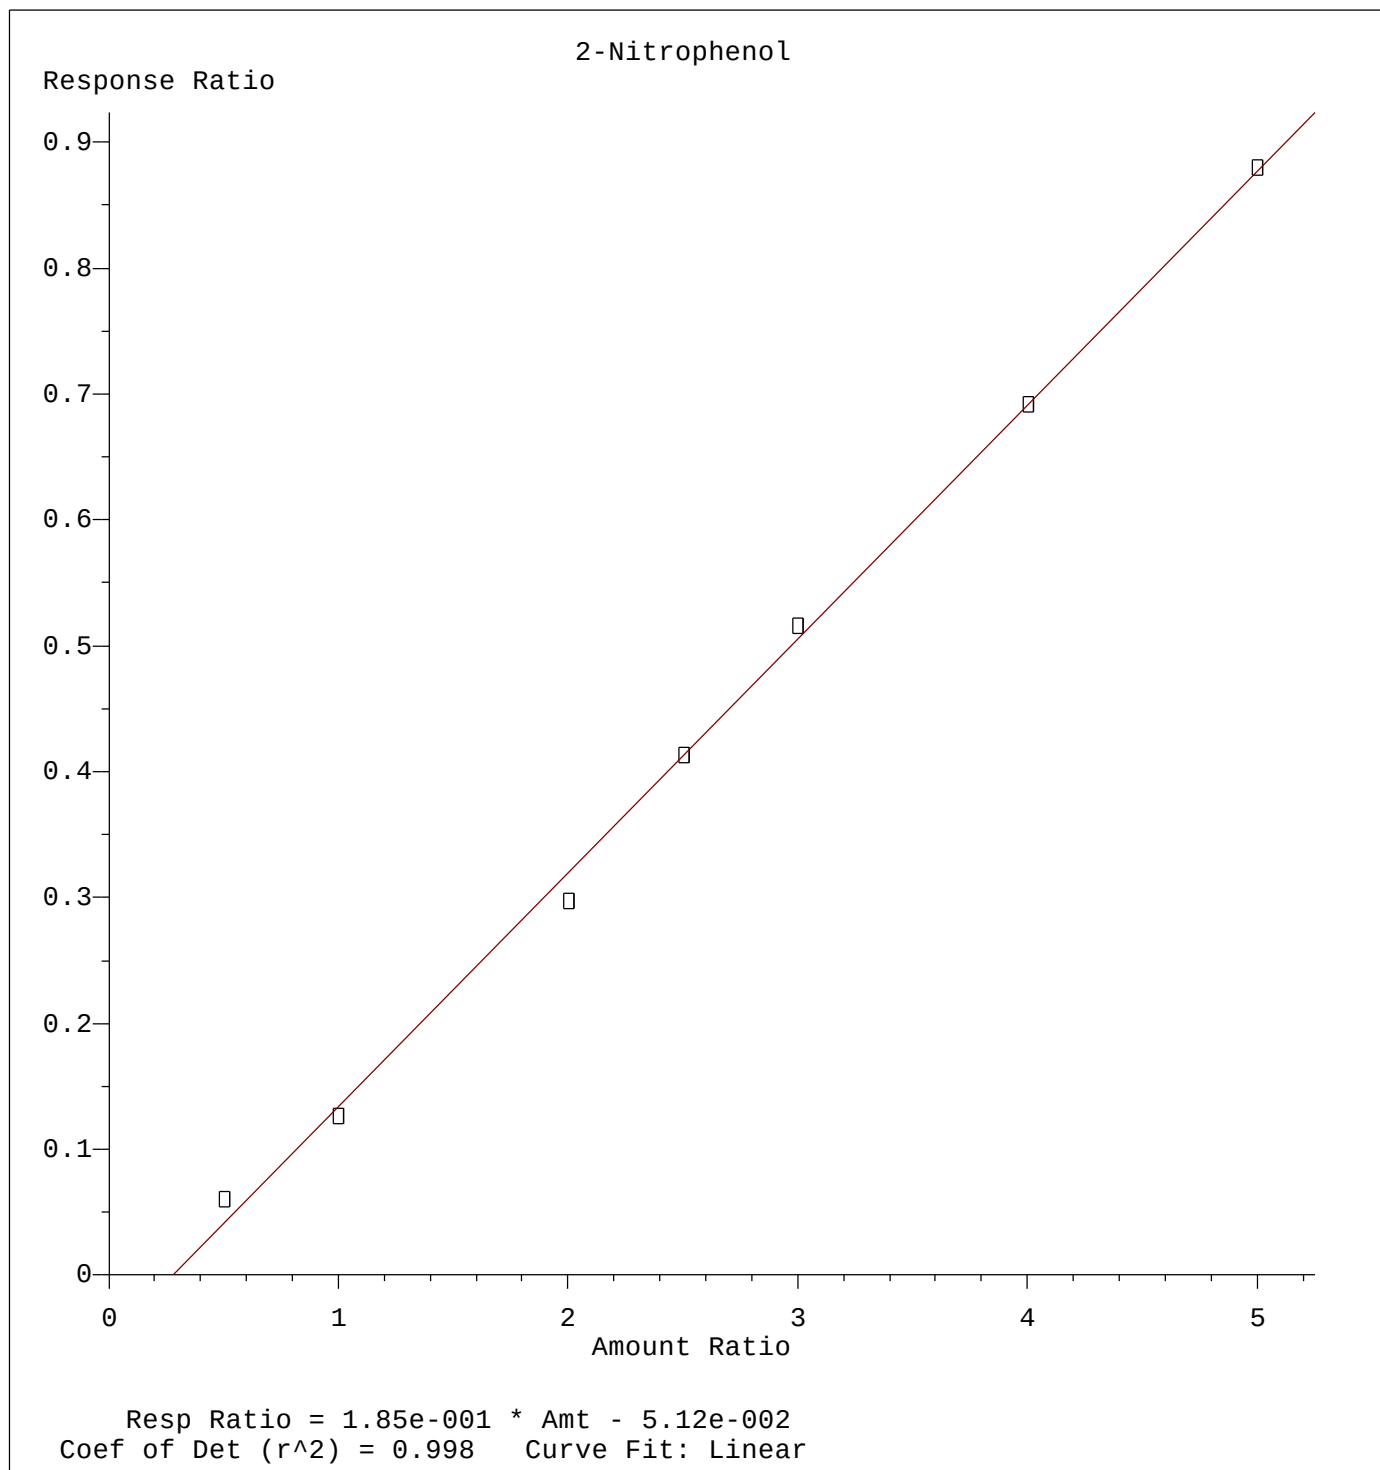


Method Name: Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031020.M  
Calibration Table Last Updated: Tue Mar 10 16:27:39 2020

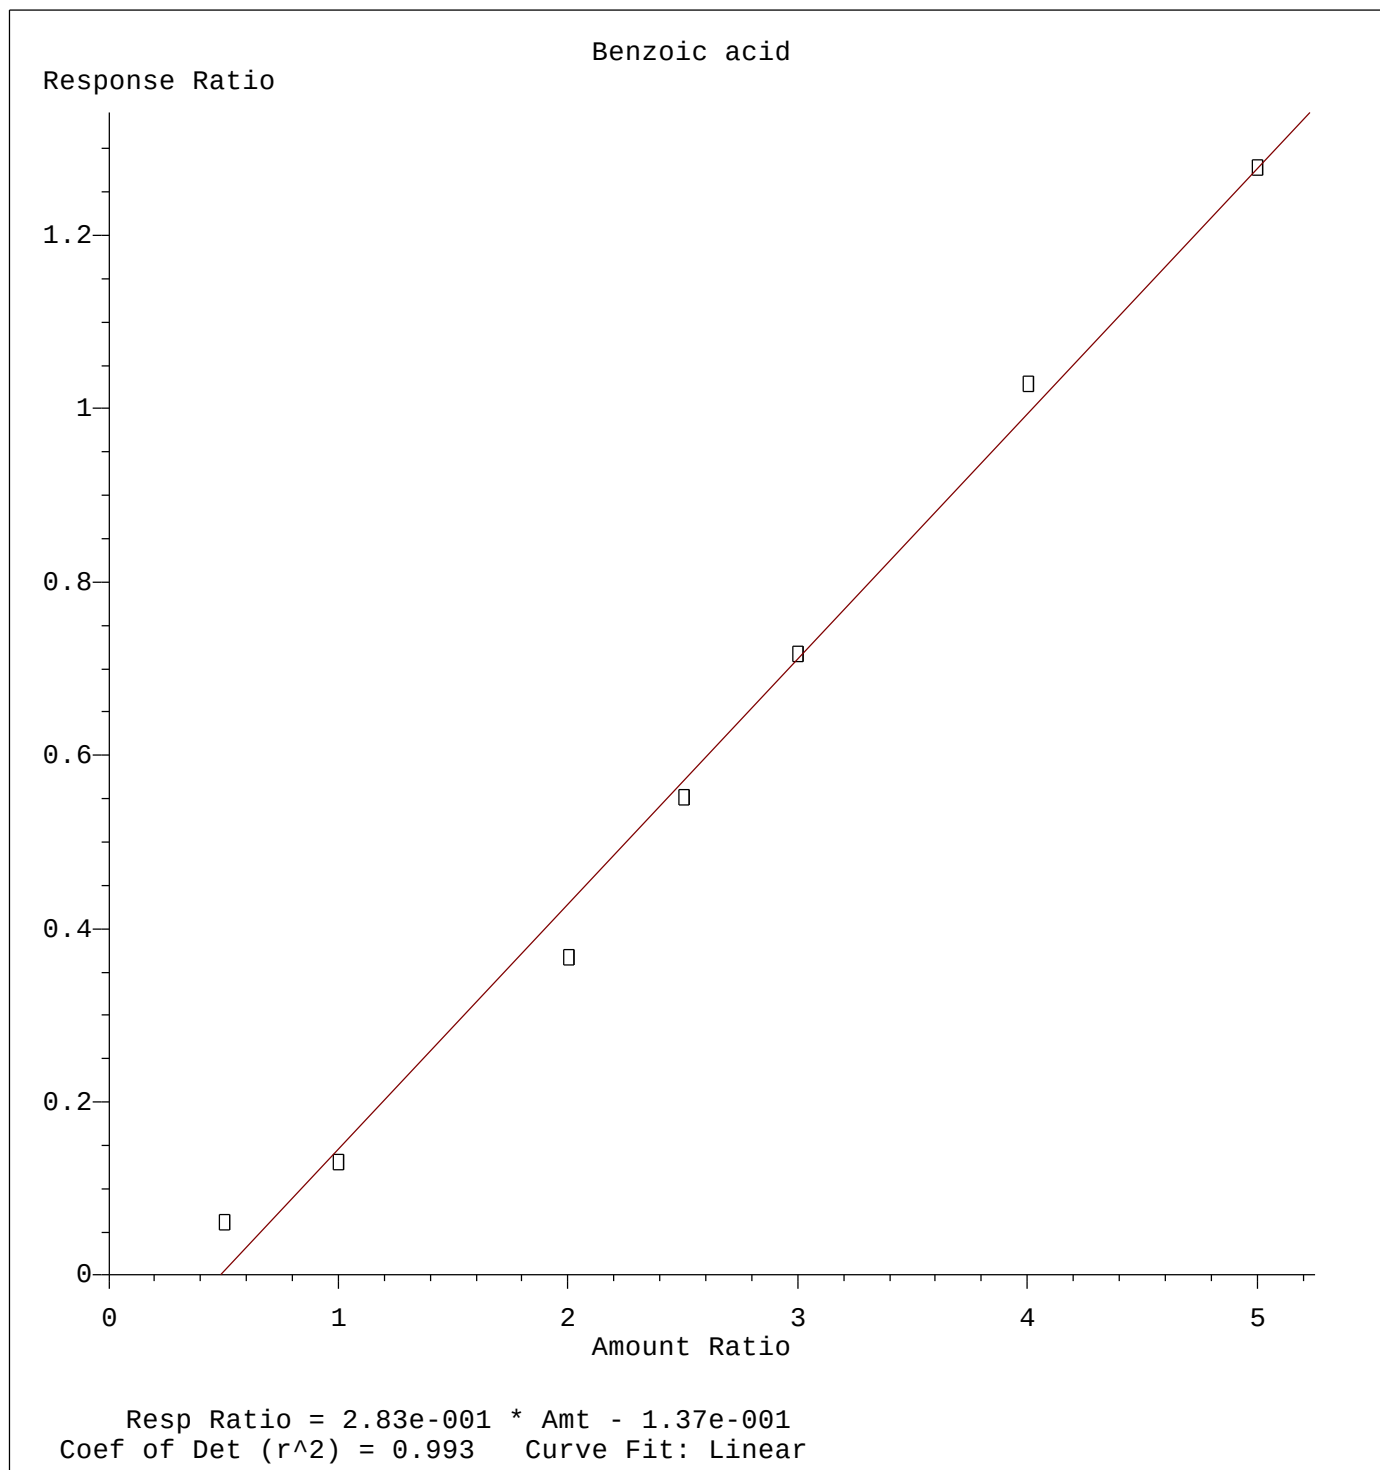

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031020.M  
Calibration Table Last Updated: Tue Mar 10 16:27:39 2020

# 2,4-Dinitrophenol

Response Ratio

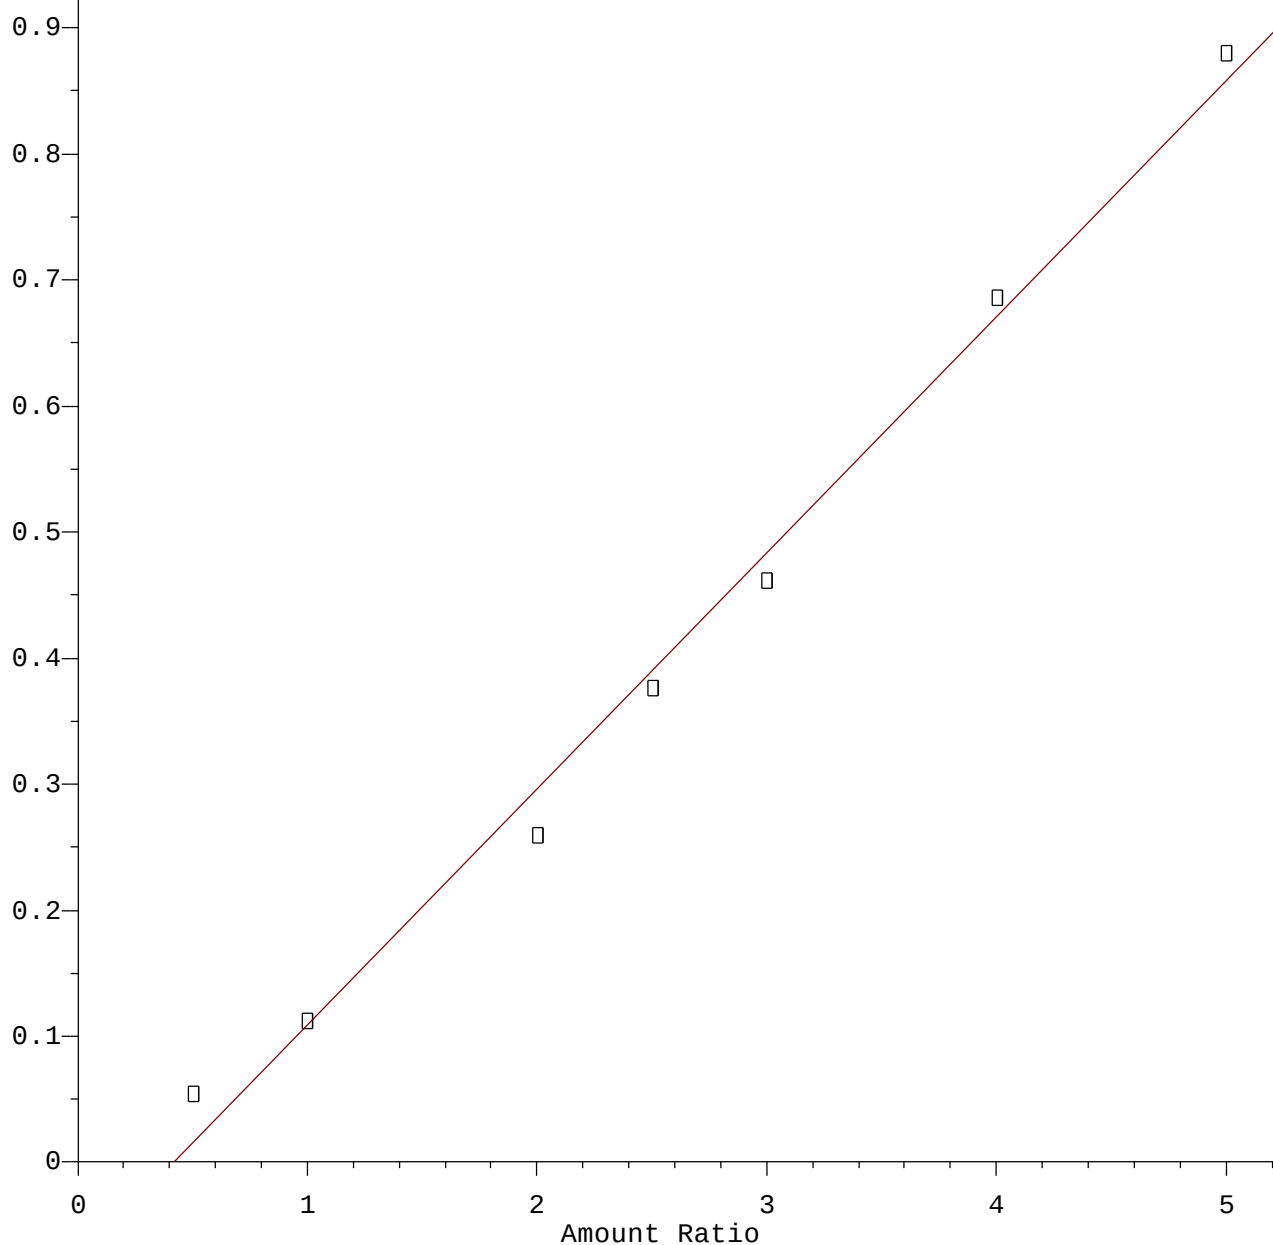


Resp Ratio =  $1.87 \times 10^{-1} \times \text{Amt} - 7.79 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.992    Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031020.M  
Calibration Table Last Updated: Tue Mar 10 16:27:39 2020

# 4,6-Dinitro-2-methylphenol

Response Ratio

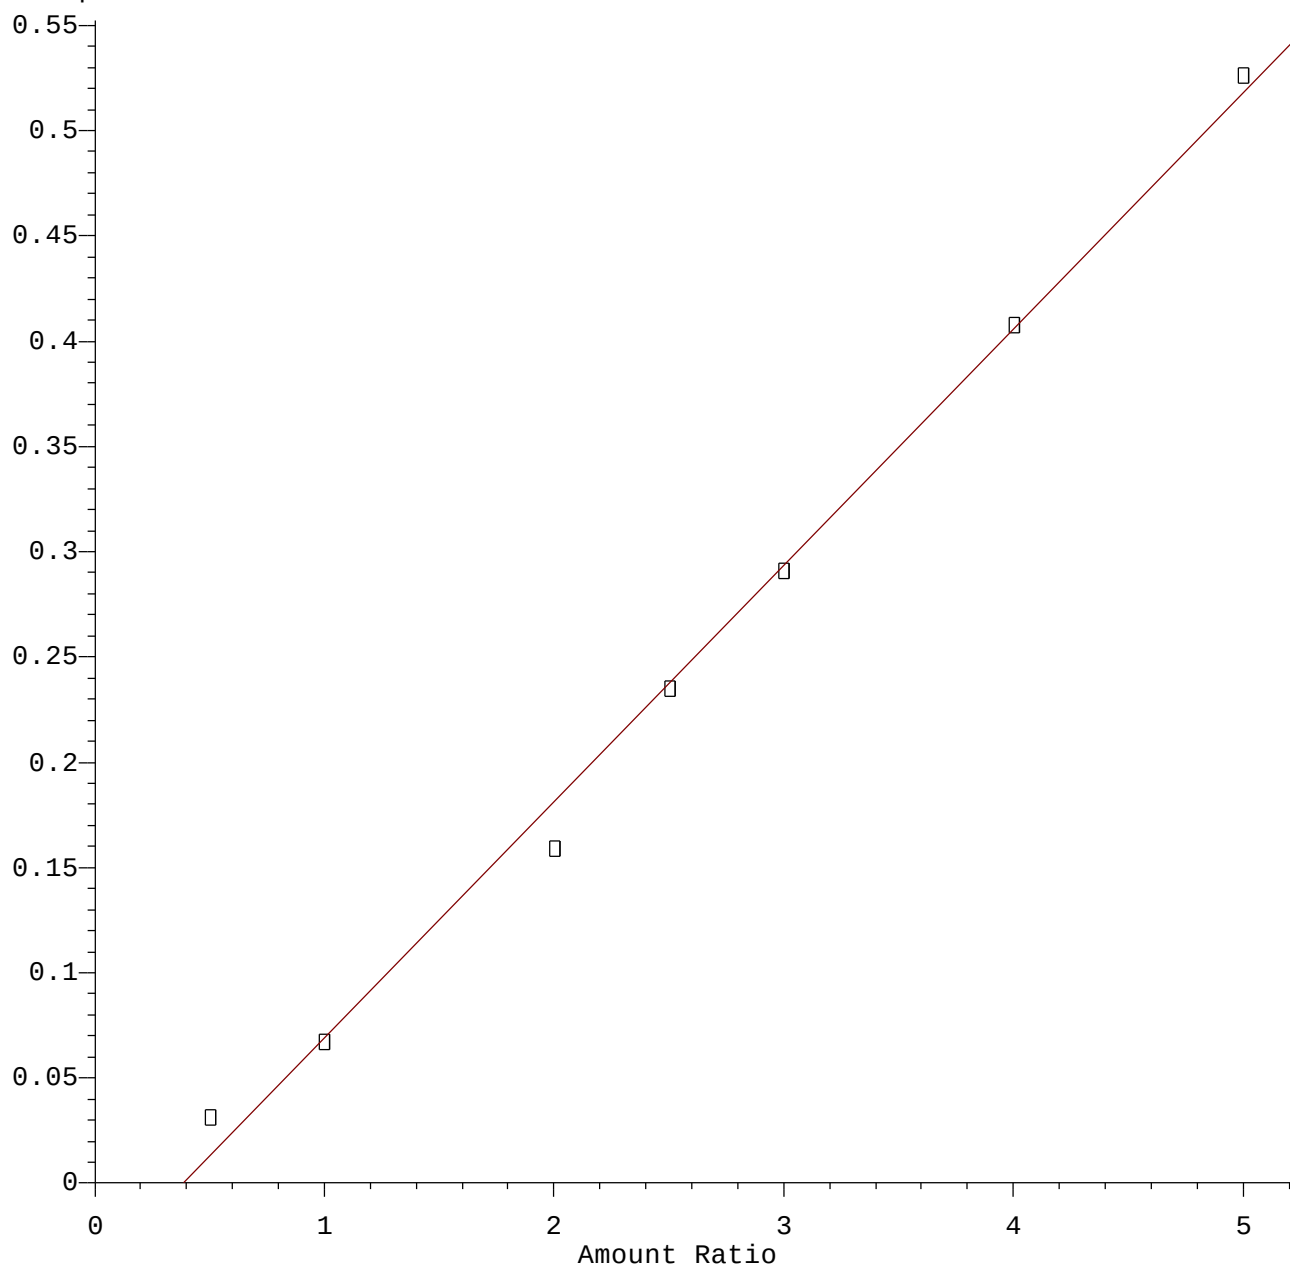

Resp Ratio =  $1.12 \times 10^{-1} \times \text{Amt} - 4.33 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031020.M  
Calibration Table Last Updated: Tue Mar 10 16:27:39 2020