


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031020\
 Data File : BG044707.D
 Acq On : 10 Mar 2020 9:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 10 16:27:39 2020

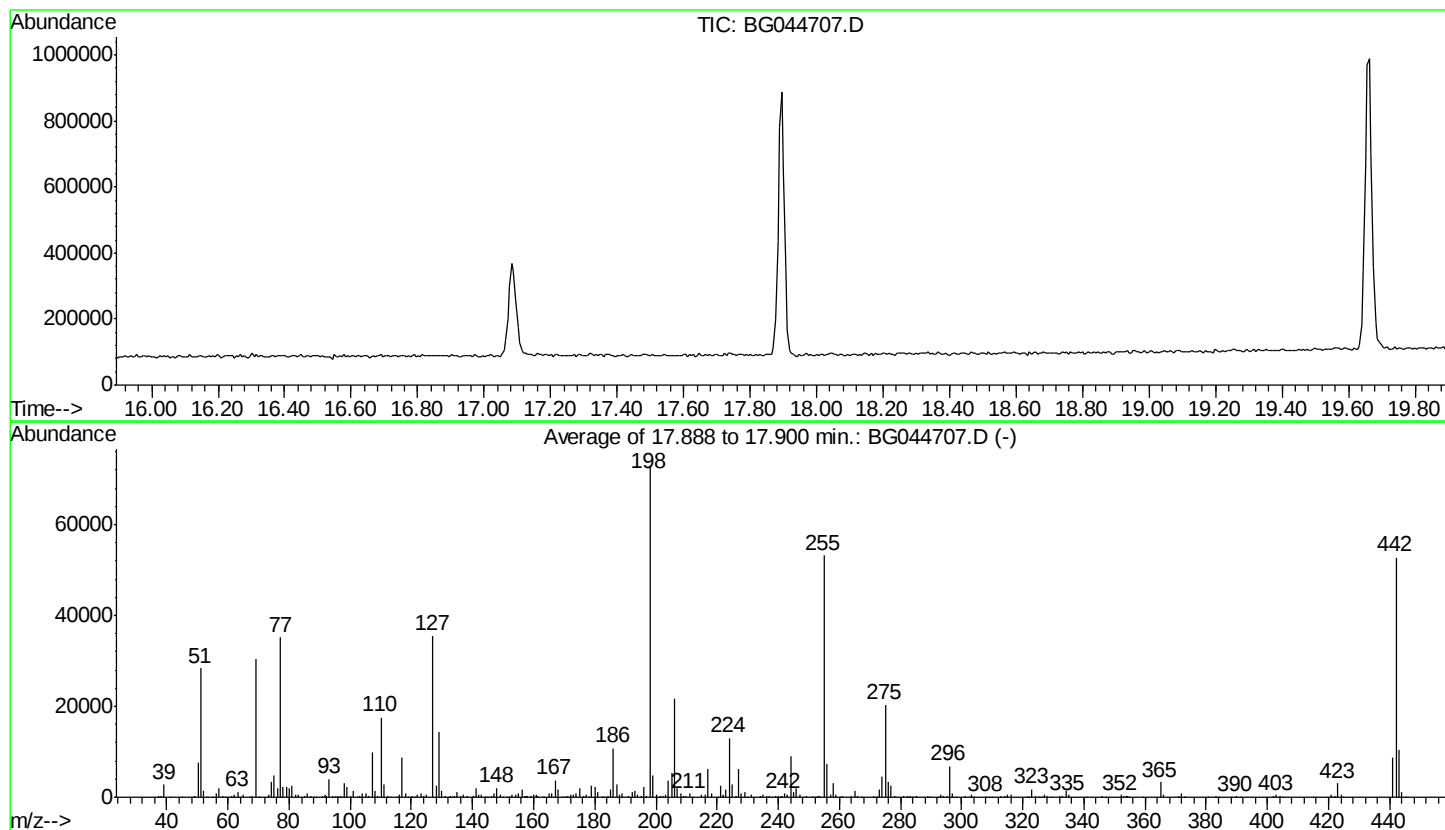

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	28394	PASS
68	69	0.00	2	0.9	261	PASS
69	198	0.00	100	41.8	30528	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	48.7	35506	PASS
197	198	0.00	2	0.3	241	PASS
198	198	100	100	100.0	72981	PASS
199	198	5	9	6.5	4750	PASS
275	198	10	60	28.0	20426	PASS
365	198	1	100	4.6	3353	PASS
441	198	0.01	100	12.0	8734	PASS
442	198	50	100	72.3	52800	PASS
443	442	15	24	19.5	10321	PASS