

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031119\
 Data File : BG039841.D
 Acq On : 11 Mar 2019 14:35
 Operator : JU/SJ
 Sample : PB117780BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB117780BL

Quant Time: Mar 12 03:35:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	40464	20.00	ng	-0.02
21) Naphthalene-d8	10.98	136	169691	20.00	ng	-0.01
39) Acenaphthene-d10	14.78	164	121282	20.00	ng	-0.01
64) Phenanthrene-d10	17.52	188	318740	20.00	ng	-0.01
76) Chrysene-d12	21.81	240	354998	20.00	ng	-0.02
87) Perylene-d12	25.18	264	345101	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	293107	123.58	ng	0.00
7) Phenol-d6	7.30	99	426590	120.62	ng	-0.01
23) Nitrobenzene-d5	9.33	82	244531	77.94	ng	-0.01
42) 2,4,6-Tribromophenol	16.26	330	171121	121.05	ng	-0.01
45) 2-Fluorobiphenyl	13.40	172	644804	75.70	ng	-0.01
79) Terphenyl-d14	20.12	244	1194254	74.07	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.33	70	31908	12.535	ng	# 65
51) 2,6-Dinitrotoluene	14.78	165	15484	7.202	ng	# 24
57) 2,4-Dinitrotoluene	14.78	165	15484	5.126	ng	# 19
67) 4-Bromophenyl-phenylether	16.26	248	13239	3.711	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031119\
Data File : BG039841.D
Acq On : 11 Mar 2019 14:35
Operator : JU/SJ
Sample : PB117780BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117780BL

Quant Time: Mar 12 03:35:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

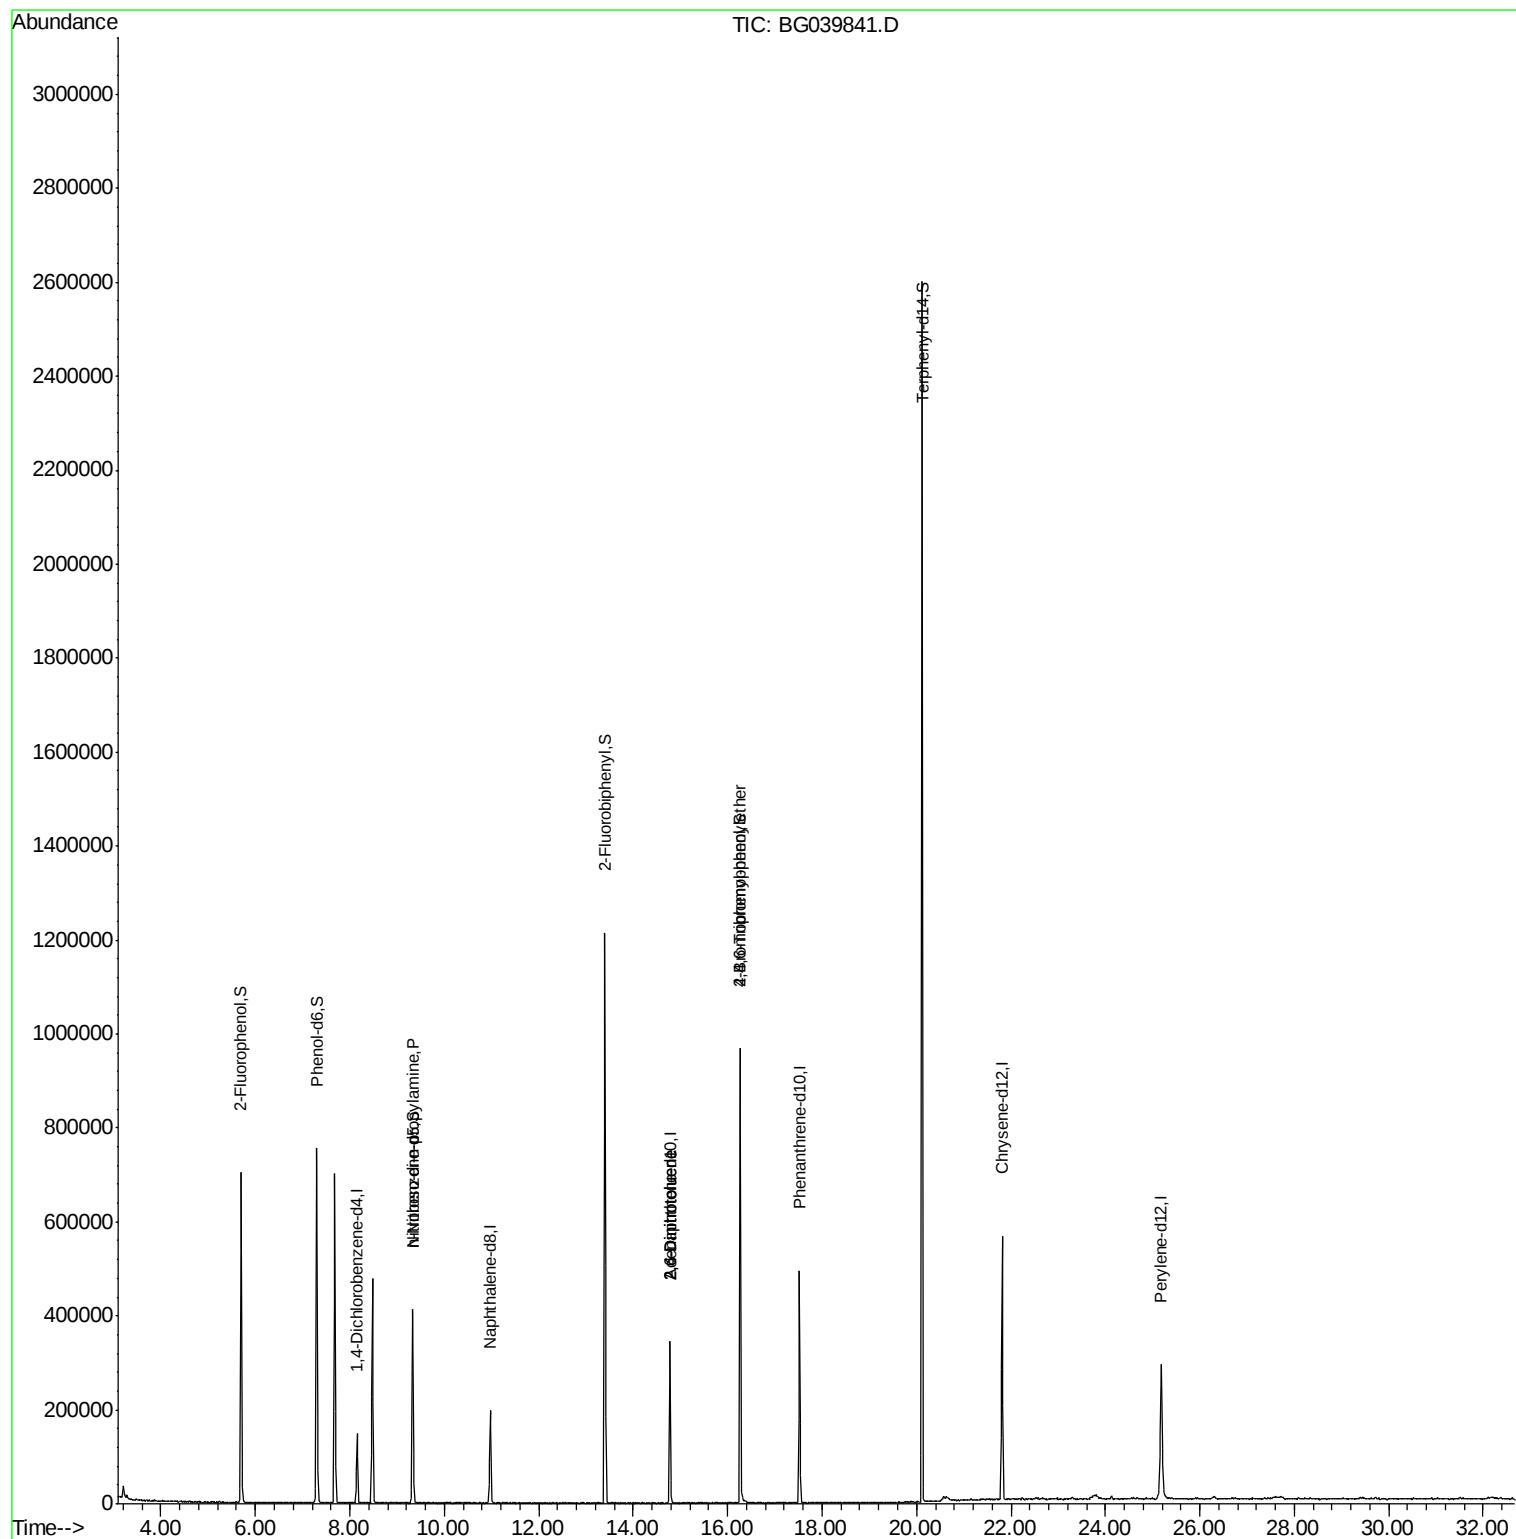




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 862
Delta R.T. -0.02 min
Lab File: BG039841.D
Acq: 11 Mar 2019 14:35

Instrument :
BNA_G
ClientSampleId :
PB117780BL

Tgt Ion:152 Resp: 40464
Ion Ratio Lower Upper
152 100
150 153.5 123.7 185.5
115 59.1 45.9 68.9

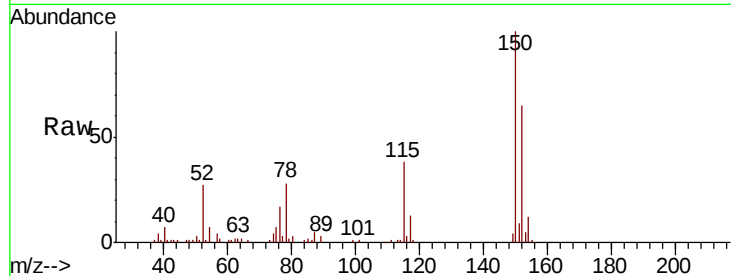


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

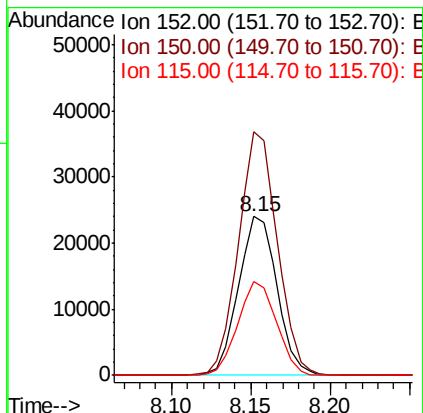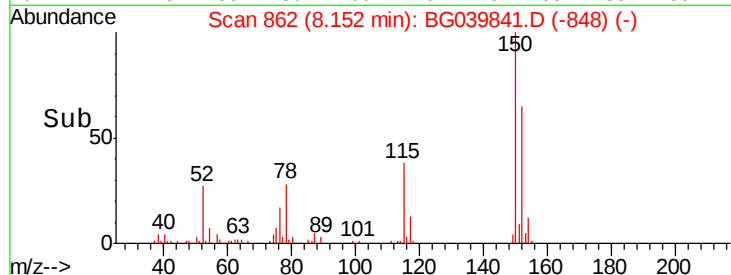



#5

2-Fluorophenol
Concen: 123.577 ng
RT: 5.70 min Scan# 445
Delta R.T. -0.01 min
Lab File: BG039841.D
Acq: 11 Mar 2019 14:35

Tgt Ion:112 Resp: 293107
Ion Ratio Lower Upper
112 100
64 67.3 57.8 86.8
63 35.7 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

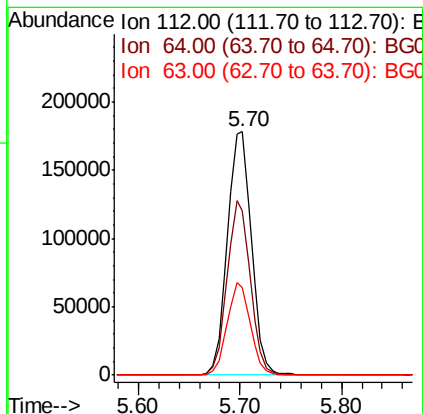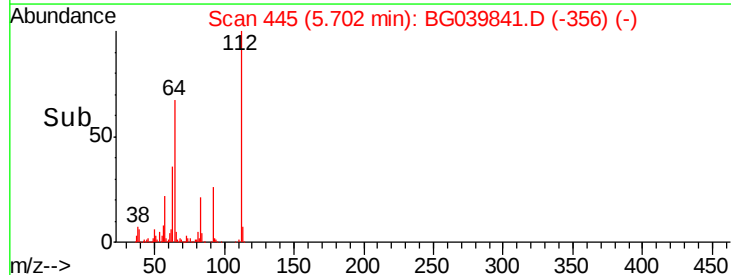



#7

Phenol-d6

Concen: 120.623 ng

RT: 7.30 min Scan# 717

Delta R.T. -0.01 min

Lab File: BG039841.D

Acq: 11 Mar 2019 14:35

Instrument :

BNA_G

ClientSampleId :

PB117780BL


Tgt Ion: 99 Resp: 426590

Ion Ratio Lower Upper




99 100

42 19.7 18.2 27.2

71 35.5 28.0 42.0

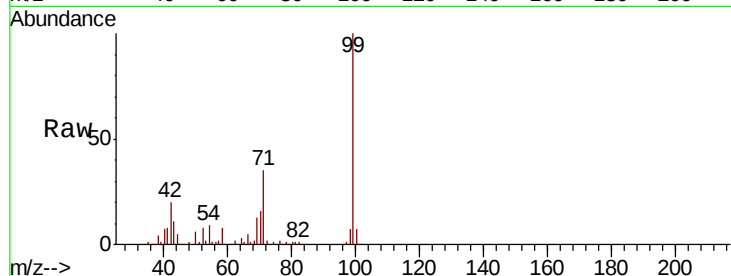

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

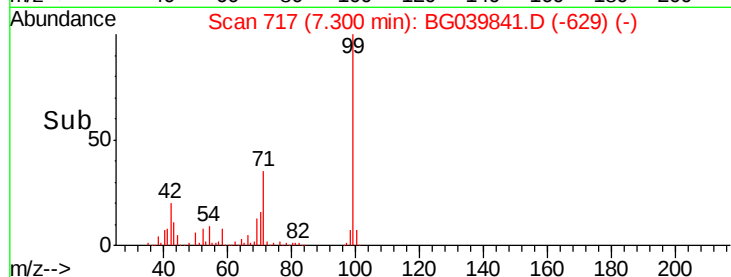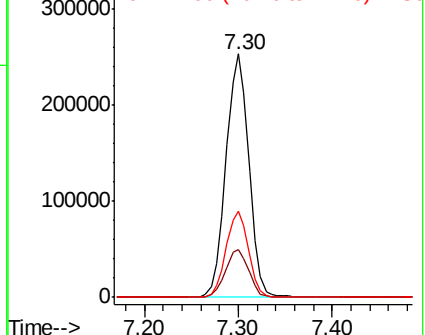

#19

n-Nitroso-di-n-propylamine

Concen: 12.535 ng

RT: 9.33 min Scan# 1062

Delta R.T. 0.36 min

Lab File: BG039841.D

Acq: 11 Mar 2019 14:35

Tgt Ion: 70 Resp: 31908


Ion Ratio Lower Upper

70 100



42 46.8 60.4 90.6#

101 0.0 7.5 11.3#

130 1.0 16.9 25.3#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

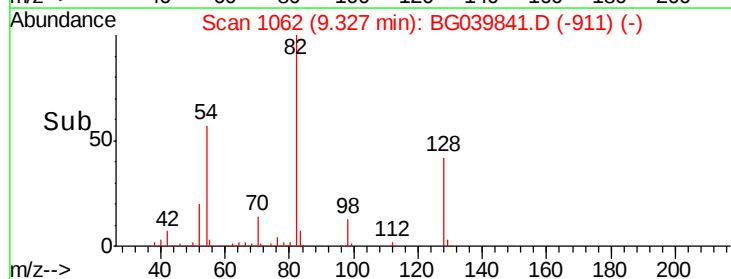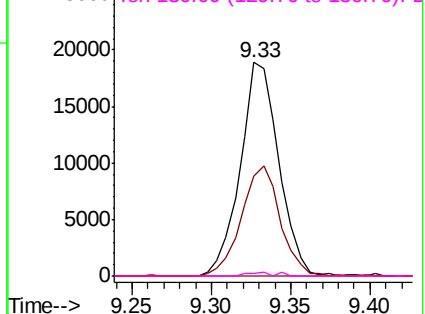







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.98 min Scan# 1343
Delta R.T. -0.01 min
Lab File: BG039841.D
Acq: 11 Mar 2019 14:35

Instrument :
BNA_G
ClientSampleId :
PB117780BL

Tgt Ion:	136	Resp:	169691
Ion	Ratio	Lower	Upper
136	100		
137	10.2	9.1	13.7
54	10.5	9.4	14.2
68	6.1	4.2	6.4




Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

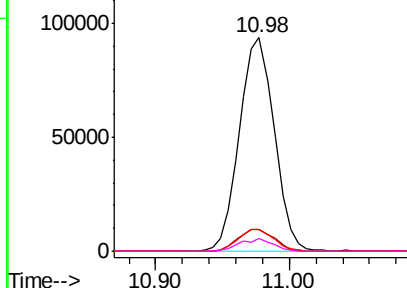
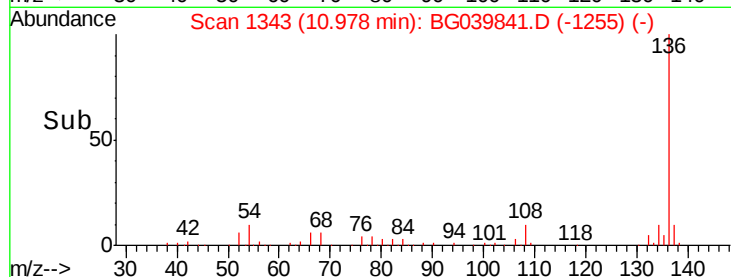



#23
Nitrobenzene-d5
Concen: 77.937 ng
RT: 9.33 min Scan# 1063
Delta R.T. -0.01 min
Lab File: BG039841.D
Acq: 11 Mar 2019 14:35

Tgt Ion:	82	Resp:	244531
Ion	Ratio	Lower	Upper
82	100		
128	44.4	31.3	46.9
54	59.5	50.9	76.3



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

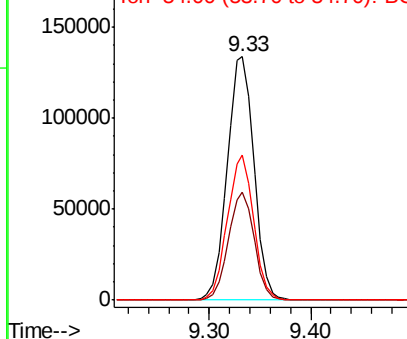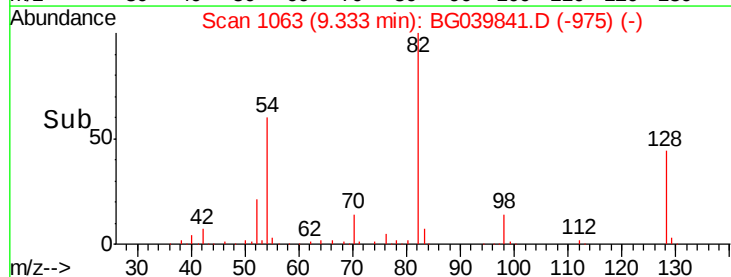

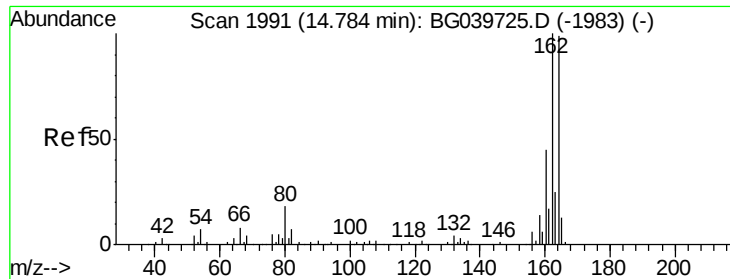

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.78 min Scan# 1990

Delta R.T. -0.01 min

Lab File: BG039841.D

Acq: 11 Mar 2019 14:35

Instrument :

BNA_G

ClientSampleId :

PB117780BL


Tgt Ion:164 Resp: 121282

Ion Ratio Lower Upper

164 100

162 103.8 81.6 122.4




160 46.9 34.2 51.2

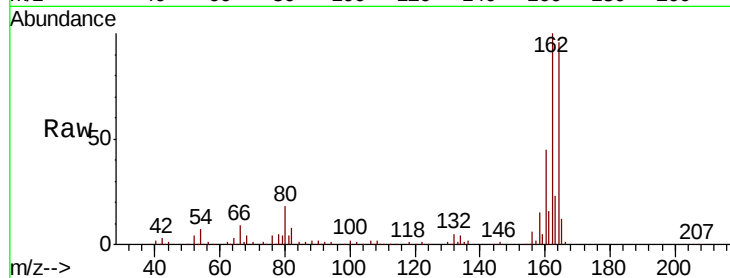

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

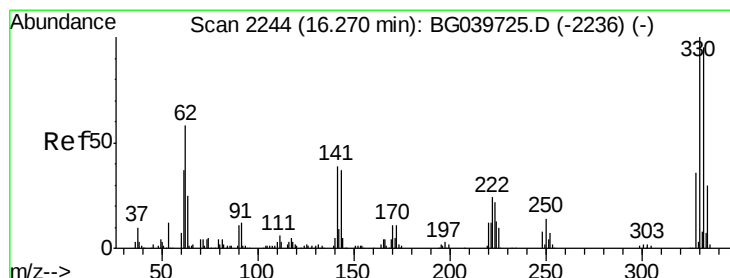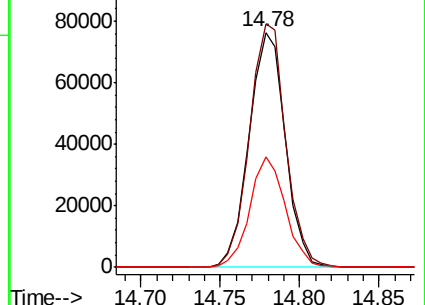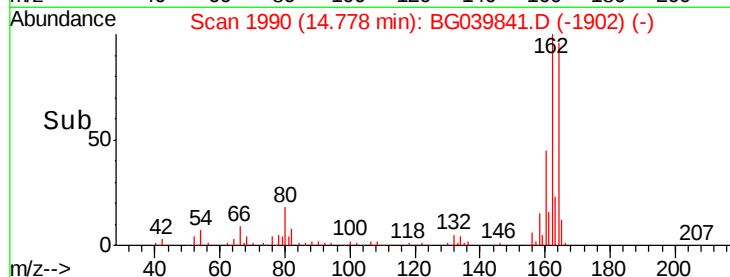

#42

2,4,6-Tribromophenol

Concen: 121.051 ng

RT: 16.26 min Scan# 2243

Delta R.T. -0.01 min

Lab File: BG039841.D

Acq: 11 Mar 2019 14:35


Tgt Ion:330 Resp: 171121

Ion Ratio Lower Upper

330 100

332 94.1 75.7 113.5



141 39.9 35.6 53.4

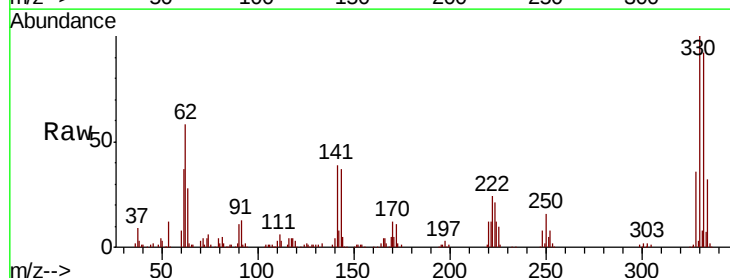

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

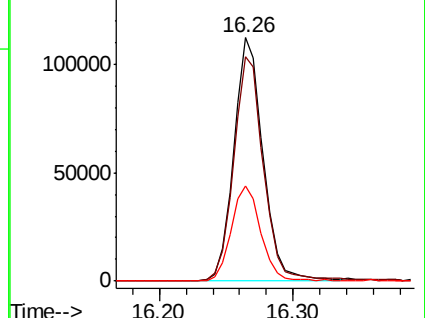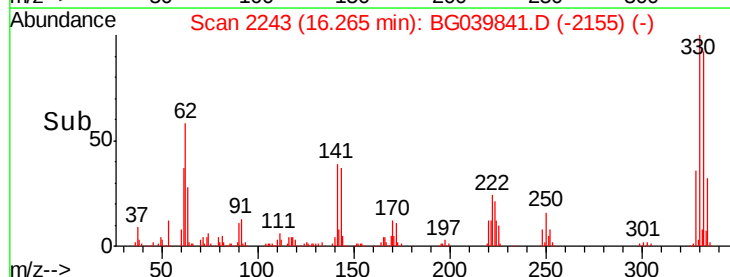







#45
 2-Fluorobiphenyl
 Concen: 75.699 ng
 RT: 13.40 min Scan# 1756
 Delta R.T. -0.01 min
 Lab File: BG039841.D
 Acq: 11 Mar 2019 14:35

Instrument :
 BNA_G
 ClientSampleId :
 PB117780BL

Tgt Ion:172 Resp: 644804
 Ion Ratio Lower Upper
 172 100
 171 36.5 30.8 46.2
 170 24.6 20.2 30.4

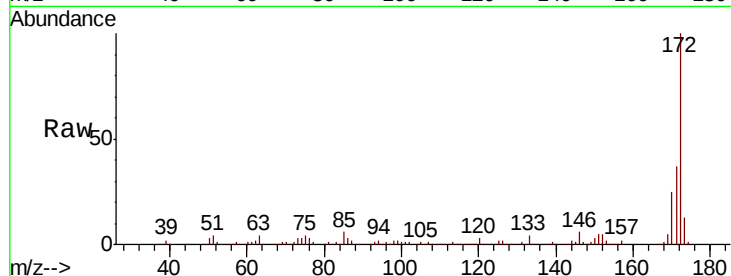


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

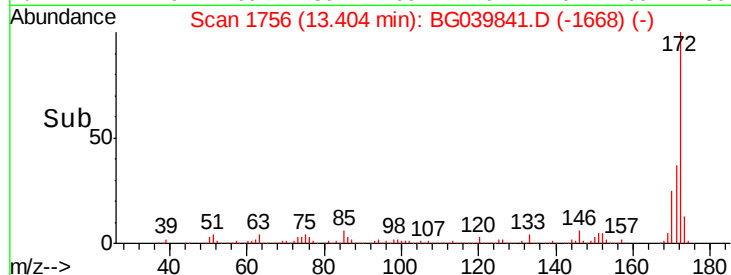
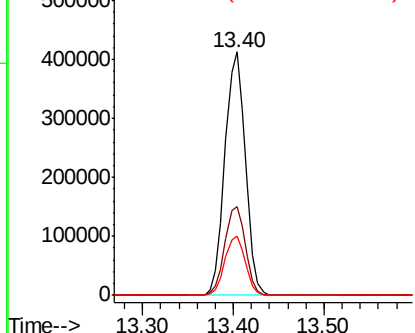



#51
 2,6-Dinitrotoluene
 Concen: 7.202 ng
 RT: 14.78 min Scan# 1990
 Delta R.T. 0.41 min
 Lab File: BG039841.D
 Acq: 11 Mar 2019 14:35

Tgt Ion:165 Resp: 15484
 Ion Ratio Lower Upper
 165 100
 63 2.9 47.0 70.6#
 89 0.0 45.8 68.8#

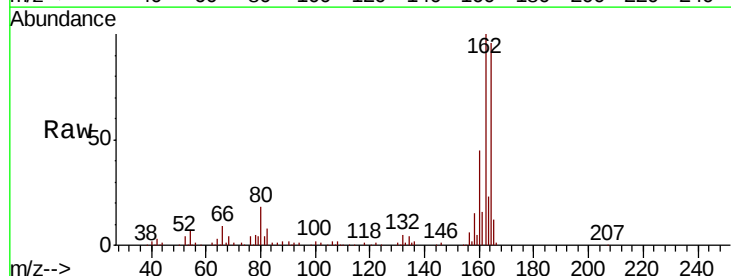

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC

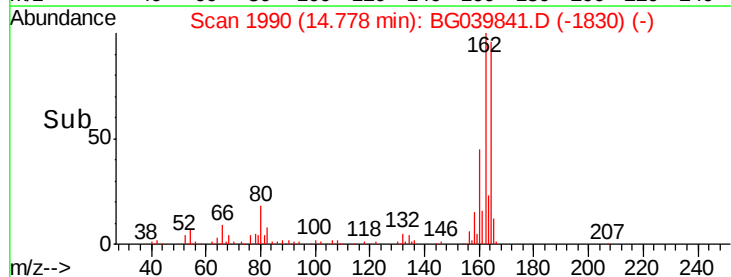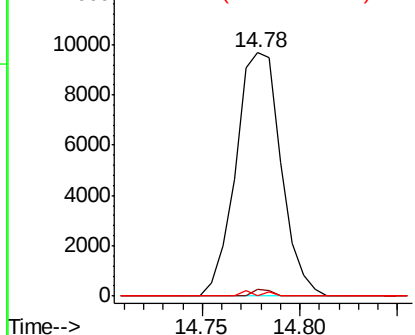


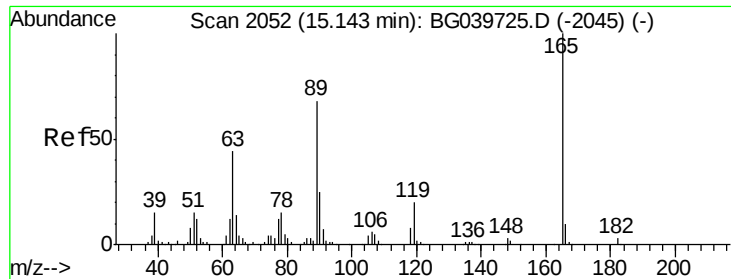

#57
 2,4-Dinitrotoluene
 Concen: 5.126 ng
 RT: 14.78 min Scan# 1990
 Delta R.T. -0.37 min
 Lab File: BG039841.D
 Acq: 11 Mar 2019 14:35

Instrument :
 BNA_G
 ClientSampleId :
 PB117780BL

Tgt Ion	Ratio	Lower	Upper
165	100		
63	2.9	41.0	61.6#
89	0.0	64.6	96.8#
182	0.0	2.0	3.0#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

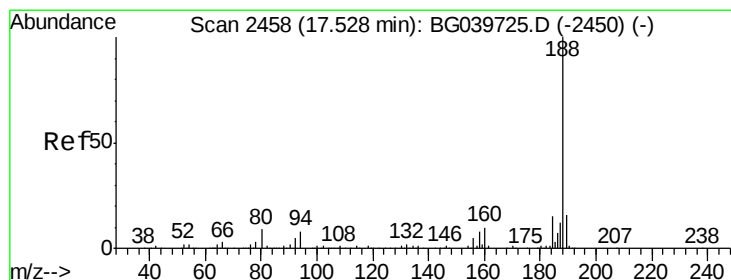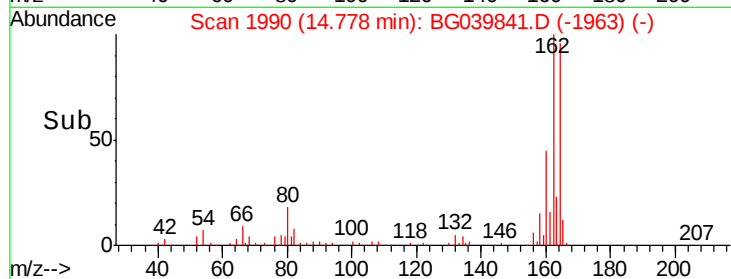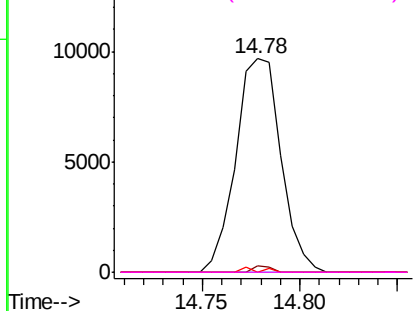

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.52 min Scan# 2457
 Delta R.T. -0.01 min
 Lab File: BG039841.D
 Acq: 11 Mar 2019 14:35



Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.4	6.9	10.3
80	9.8	8.1	12.1

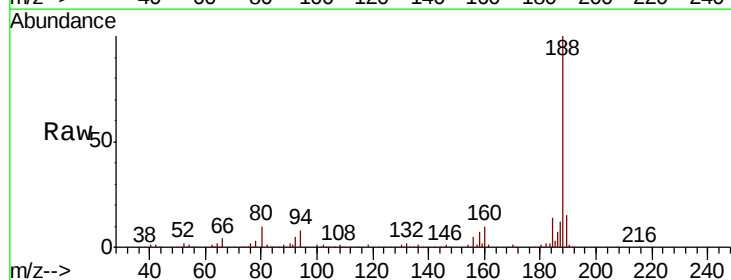


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

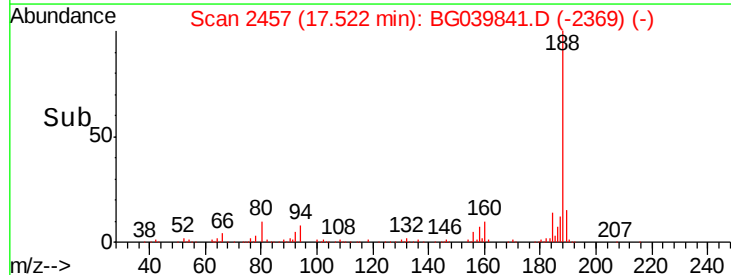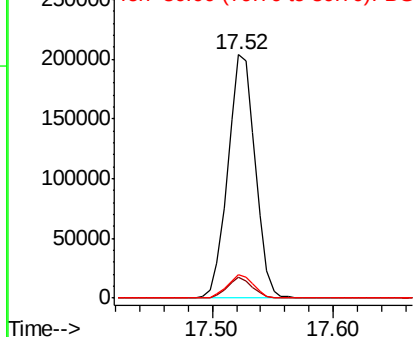


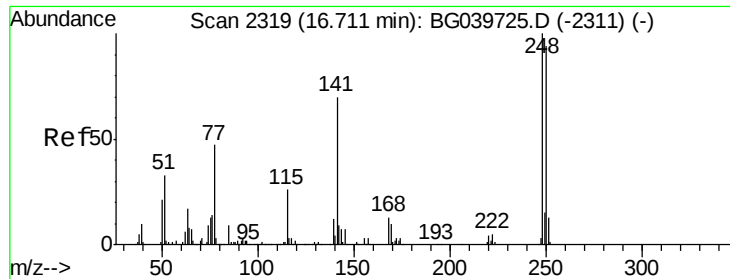




#67
 4-Bromophenyl-phenylether
 Concen: 3.711 ng
 RT: 16.26 min Scan# 2243
 Delta R.T. -0.45 min
 Lab File: BG039841.D
 Acq: 11 Mar 2019 14:35

Instrument :
 BNA_G
 ClientSampleId :
 PB117780BL

Tgt Ion:248 Resp: 13239
 Ion Ratio Lower Upper
 248 100
 250 202.6 77.6 116.4#
 141 494.0 63.9 95.9#

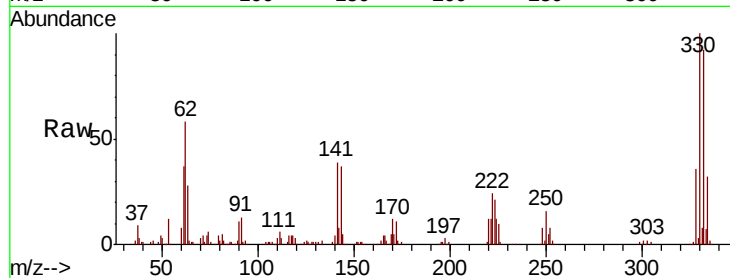


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

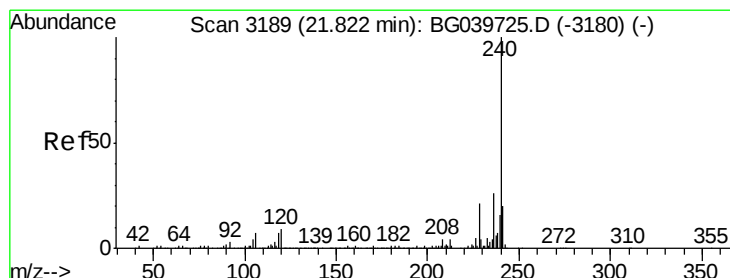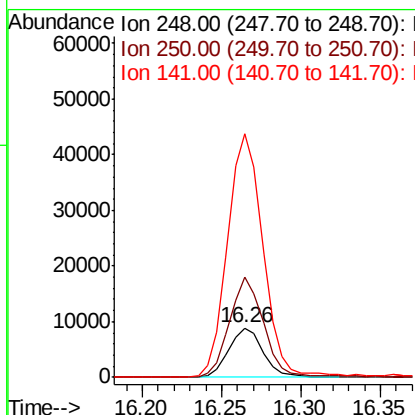
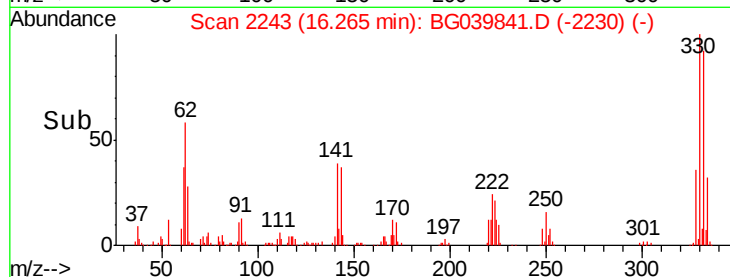



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.81 min Scan# 3187
 Delta R.T. -0.02 min
 Lab File: BG039841.D
 Acq: 11 Mar 2019 14:35

Tgt Ion:240 Resp: 354998
 Ion Ratio Lower Upper
 240 100
 120 9.1 7.0 10.6
 236 25.7 21.0 31.4

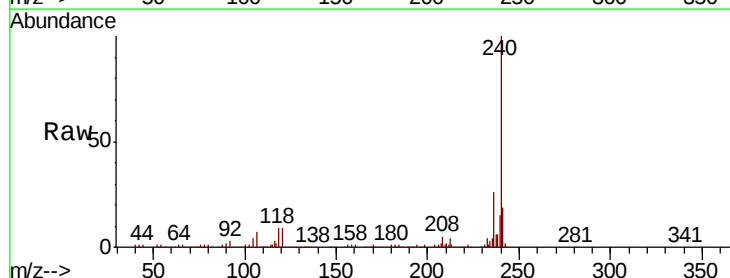

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

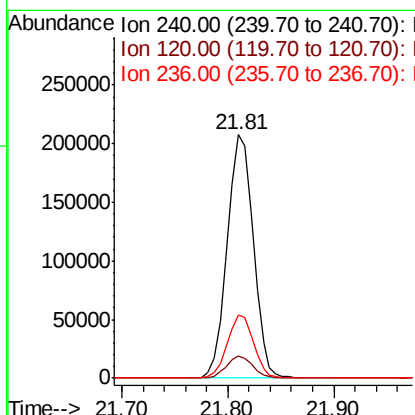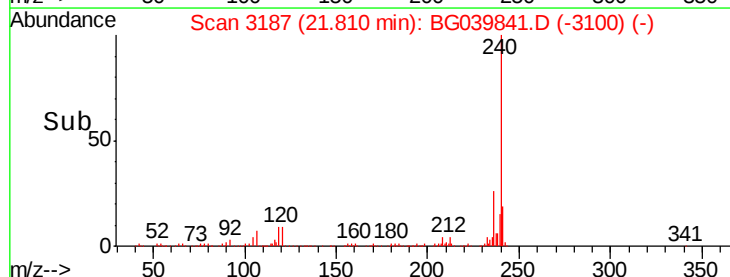

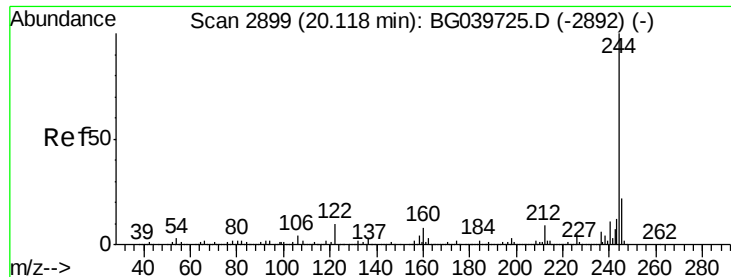

#79

Terphenyl-d14

Concen: 74.071 ng

RT: 20.12 min Scan# 2899

Delta R.T. -0.01 min

Lab File: BG039841.D

Acq: 11 Mar 2019 14:35

Instrument :

BNA_G

ClientSampleId :

PB117780BL


Tgt Ion:244 Resp: 1194254

Ion Ratio Lower Upper

244 100

212 9.1 7.3 10.9




122 9.8 8.4 12.6

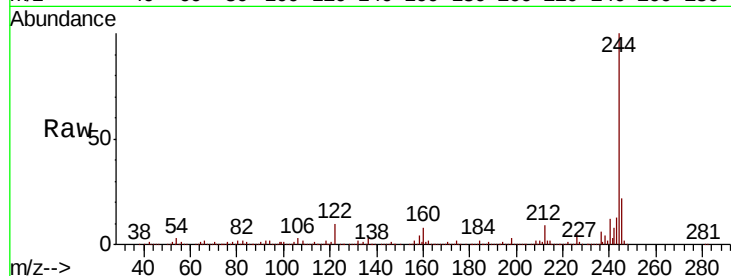

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

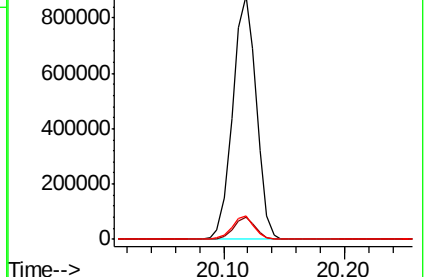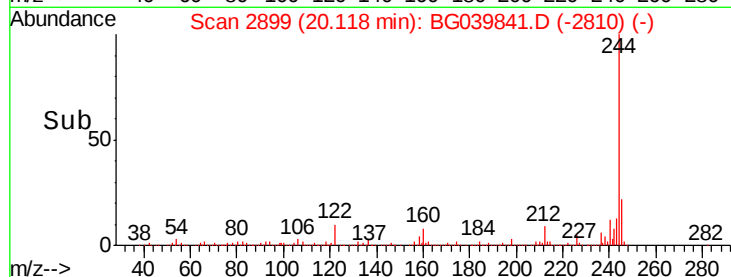

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.18 min Scan# 3761

Delta R.T. -0.02 min

Lab File: BG039841.D

Acq: 11 Mar 2019 14:35


Tgt Ion:264 Resp: 345101

Ion Ratio Lower Upper

264 100

260 23.2 18.2 27.4

265 21.2 18.5 27.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

