

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG031119\  
 Data File : BG039862.D  
 Acq On : 12 Mar 2019 5:38  
 Operator : JU/SJ  
 Sample : K1822-03  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 3-8-BOD

Quant Time: Mar 12 09:33:55 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Mar 04 14:38:15 2019  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc   | Units | Dev(Min)    |
|--------------------------------|-------|------|----------|--------|-------|-------------|
| 1) 1,4-Dichlorobenzene-d4      | 8.15  | 152  | 41800    | 20.00  | ng    | -0.02       |
| 21) Naphthalene-d8             | 10.97 | 136  | 174830   | 20.00  | ng    | -0.02       |
| 39) Acenaphthene-d10           | 14.78 | 164  | 112300   | 20.00  | ng    | -0.02       |
| 64) Phenanthrene-d10           | 17.52 | 188  | 263656   | 20.00  | ng    | 0.00        |
| 76) Chrysene-d12               | 21.81 | 240  | 304272   | 20.00  | ng    | -0.02       |
| 87) Perylene-d12               | 25.18 | 264  | 315015   | 20.00  | ng    | -0.02       |
| System Monitoring Compounds    |       |      |          |        |       |             |
| 5) 2-Fluorophenol              | 5.70  | 112  | 327814   | 133.79 | ng    | 0.00        |
| 7) Phenol-d6                   | 7.30  | 99   | 425331   | 116.42 | ng    | -0.02       |
| 23) Nitrobenzene-d5            | 9.33  | 82   | 327698   | 101.37 | ng    | -0.02       |
| 42) 2,4,6-Tribromophenol       | 16.27 | 330  | 194529   | 148.62 | ng    | 0.00        |
| 45) 2-Fluorobiphenyl           | 13.40 | 172  | 789717   | 100.13 | ng    | -0.02       |
| 79) Terphenyl-d14              | 20.12 | 244  | 1213904  | 87.84  | ng    | 0.00        |
| Target Compounds               |       |      |          |        |       |             |
| 15) Benzyl Alcohol             | 8.39  | 79   | 9583     | 3.307  | ng    | Qvalue # 83 |
| 19) n-Nitroso-di-n-propylamine | 9.33  | 70   | 43483    | 16.536 | ng    | # 67        |
| 31) Naphthalene                | 11.03 | 128  | 52891    | 5.714  | ng    | 98          |
| 32) Benzoic acid               | 10.22 | 122  | 896      | 7.040  | ng    | 91          |
| 37) 2-Methylnaphthalene        | 12.61 | 142  | 21452    | 3.100  | ng    | 95          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG031119\  
Data File : BG039862.D  
Acq On : 12 Mar 2019 5:38  
Operator : JU/SJ  
Sample : K1822-03  
Misc :  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD

Quant Time: Mar 12 09:33:55 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 14:38:15 2019  
Response via : Initial Calibration

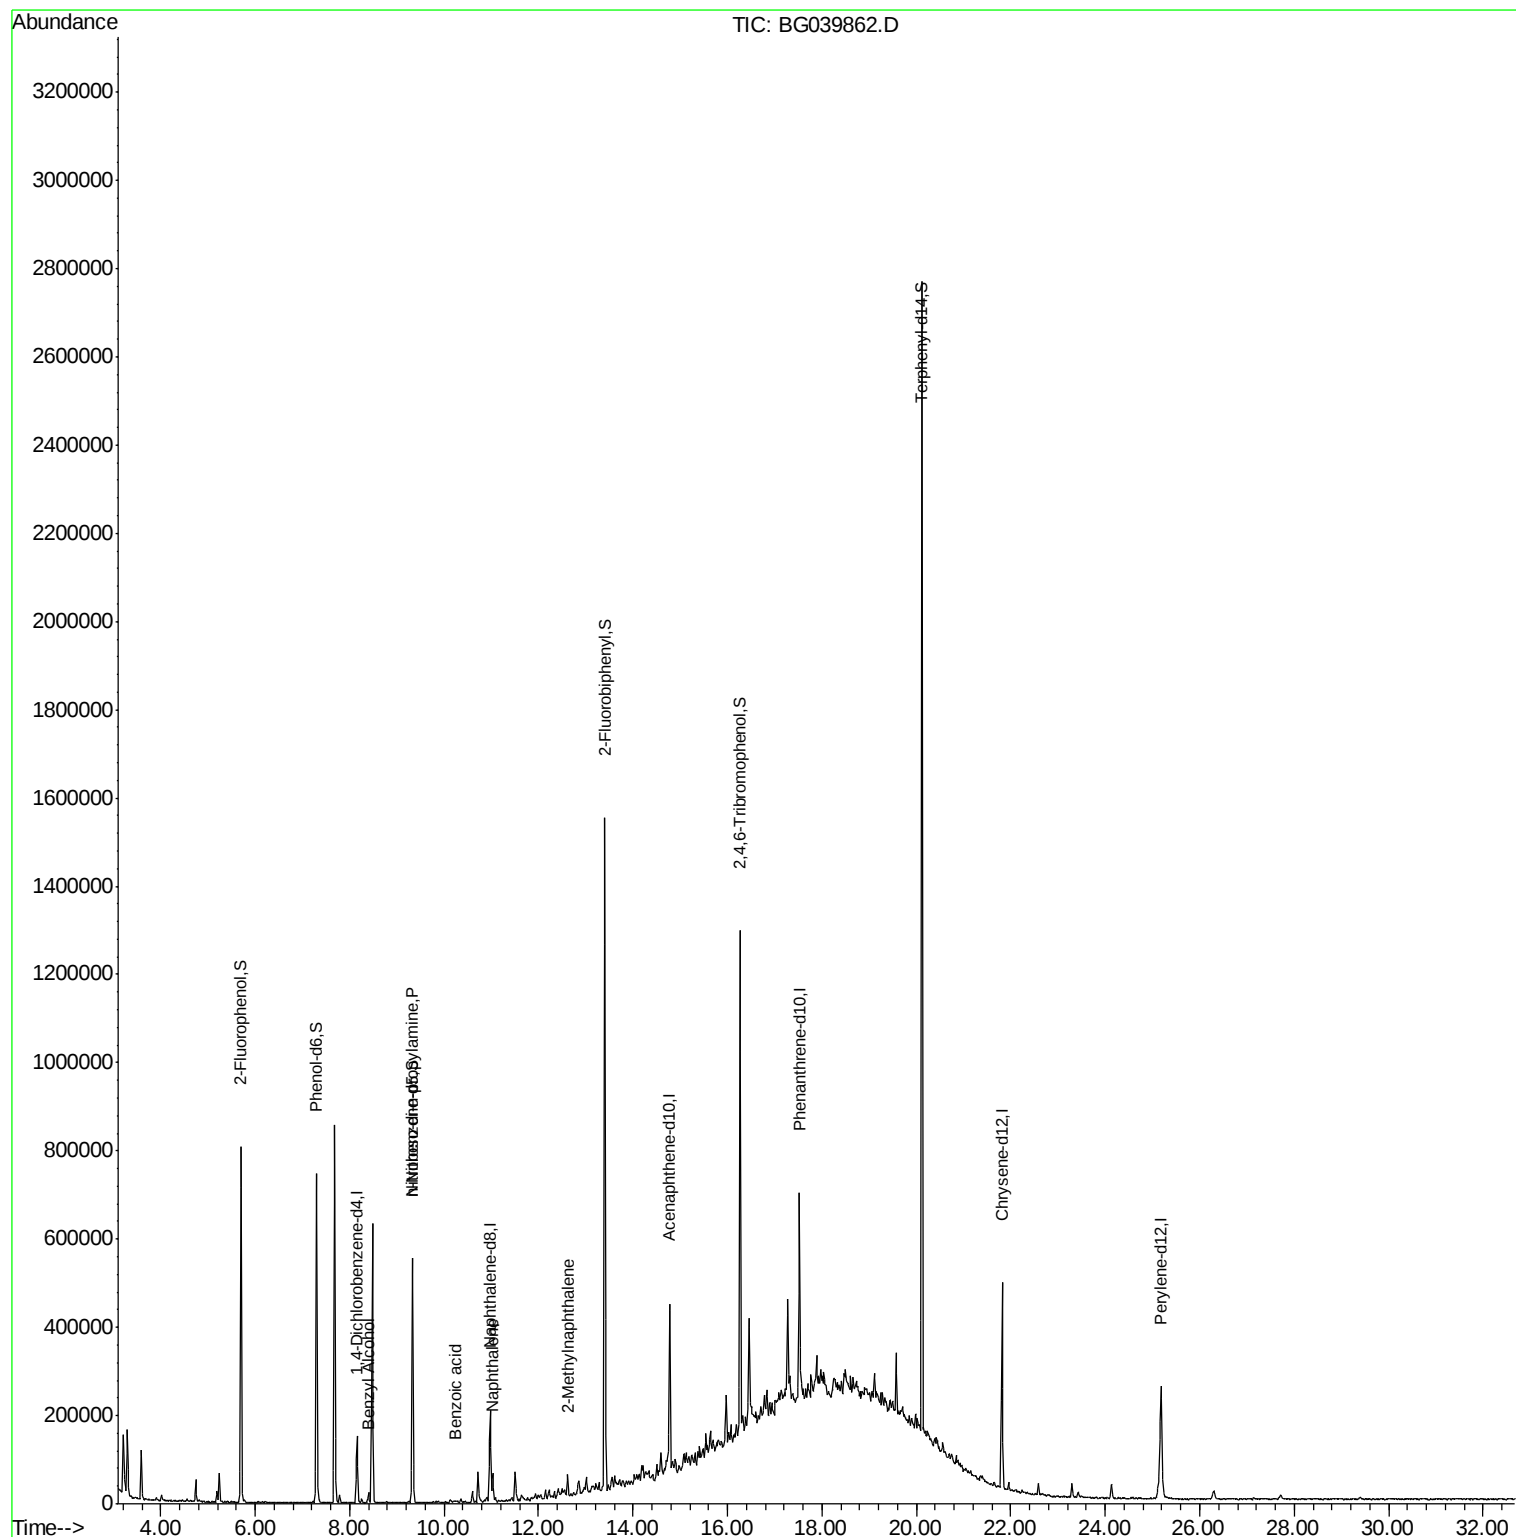

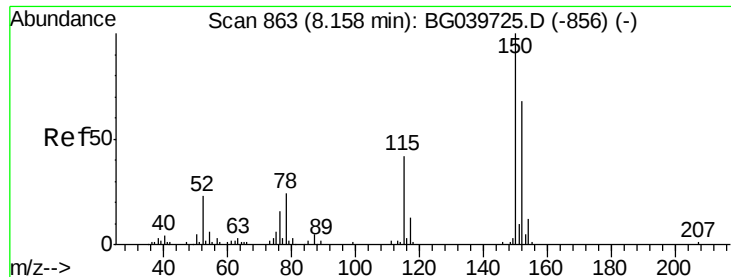


#1




1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 8.15 min Scan# 862  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD

Tgt Ion:152 Resp: 41800  
Ion Ratio Lower Upper  
152 100  
150 155.6 123.7 185.5  
115 57.3 45.9 68.9




Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

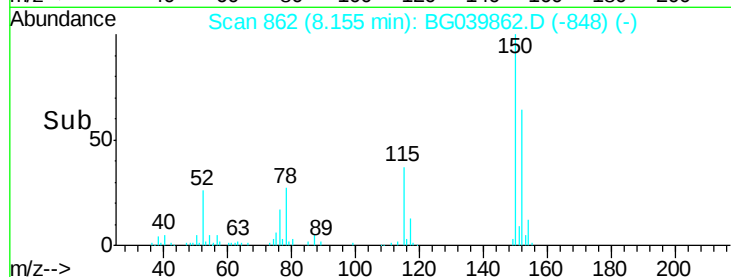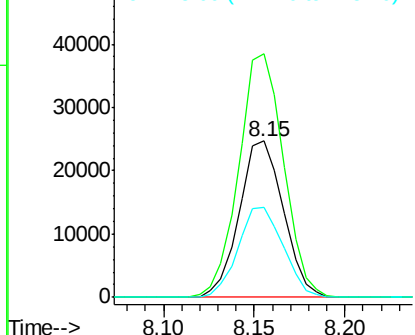



#5


2-Fluorophenol  
Concen: 133.793 ng  
RT: 5.70 min Scan# 444  
Delta R.T. -0.01 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Tgt Ion:112 Resp: 327814  
Ion Ratio Lower Upper  
112 100  
64 69.6 57.8 86.8  
63 37.8 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BGO  
Ion 63.00 (62.70 to 63.70): BGO

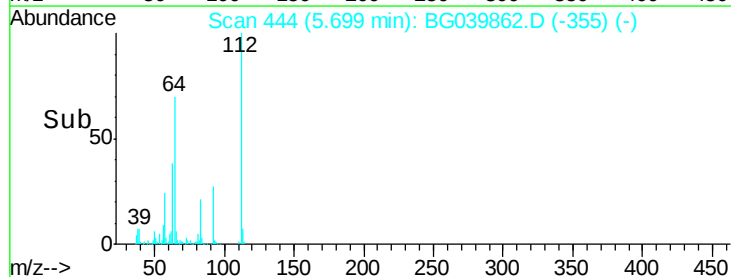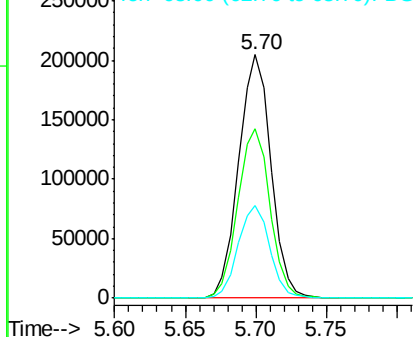

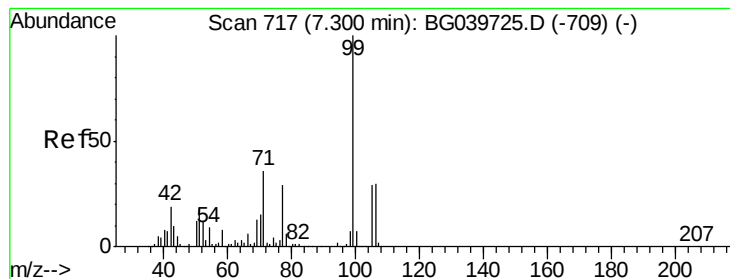

#7

Phenol-d6

Concen: 116.423 ng

RT: 7.30 min Scan# 716

Delta R.T. -0.02 min

Lab File: BG039862.D

Acq: 12 Mar 2019 5:38

Instrument :

BNA\_G

ClientSampleId :

3-8-BOD


Tgt Ion: 99 Resp: 425331

Ion Ratio Lower Upper




99 100

42 20.4 18.2 27.2

71 36.7 28.0 42.0

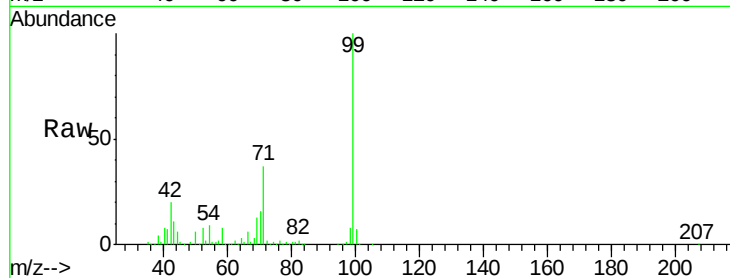

Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

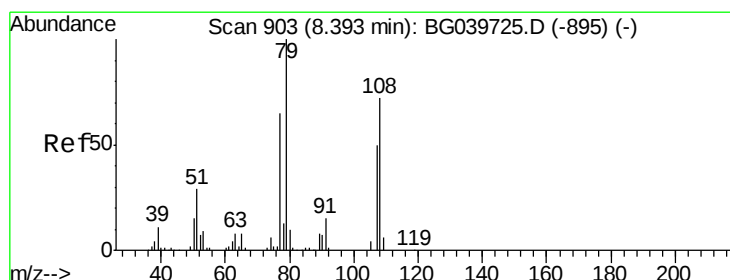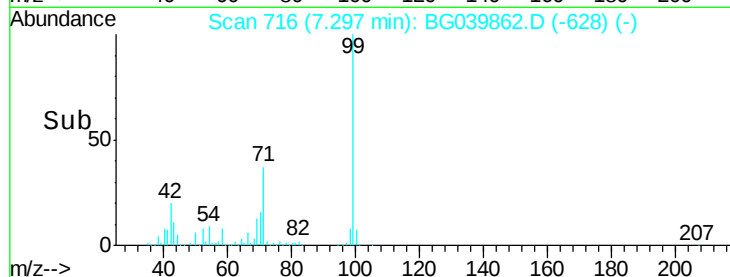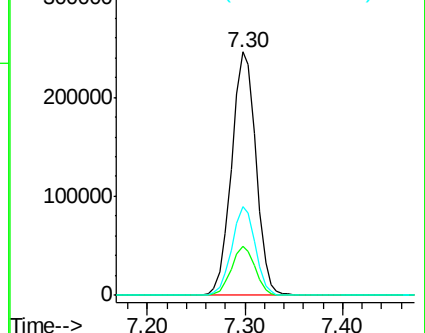

#15

Benzyl Alcohol

Concen: 3.307 ng

RT: 8.39 min Scan# 902

Delta R.T. -0.02 min

Lab File: BG039862.D

Acq: 12 Mar 2019 5:38


Tgt Ion: 79 Resp: 9583

Ion Ratio Lower Upper



79 100


108 59.5 57.8 86.6

77 48.9 51.1 76.7#

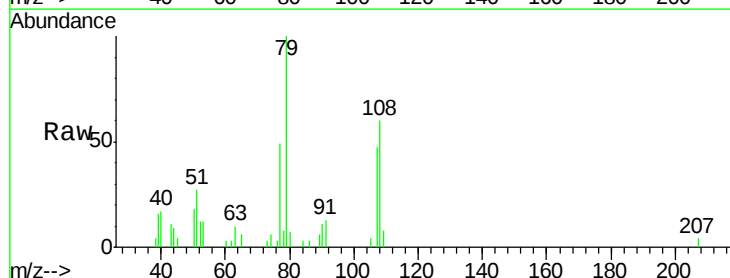

Abundance Ion 79.00 (78.70 to 79.70): BGC  
Ion 108.00 (107.70 to 108.70): BGC  
Ion 77.00 (76.70 to 77.70): BGC



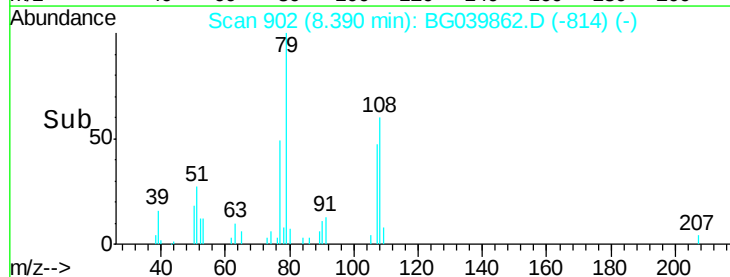
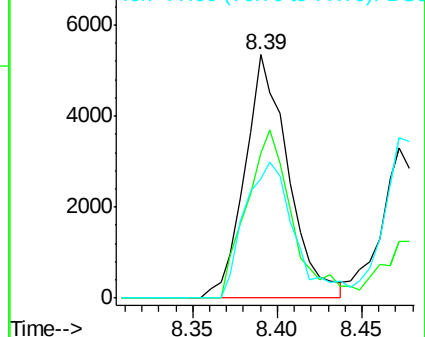


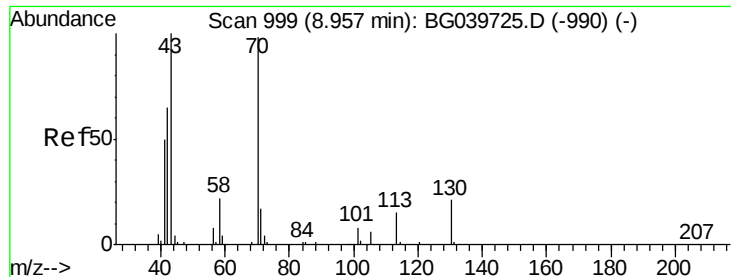

#19  
n-Nitroso-di-n-propylamine  
Concen: 16.536 ng  
RT: 9.33 min Scan# 1062  
Delta R.T. 0.36 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38




Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD


Tgt Ion: 70 Resp: 43483  
Ion Ratio Lower Upper  
70 100  
42 47.6 60.4 90.6#  
101 0.0 7.5 11.3#  
130 3.6 16.9 25.3#

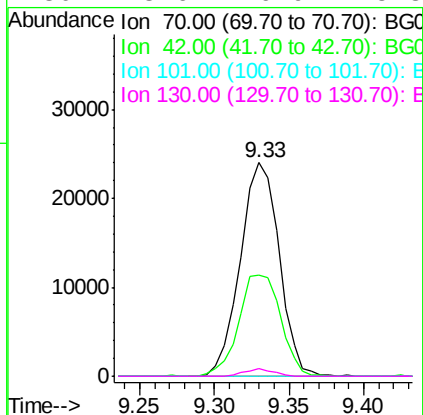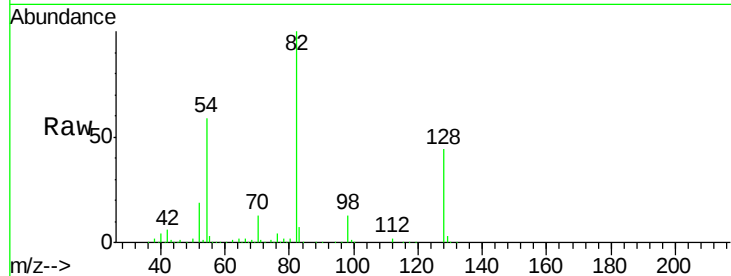

#21  
Naphthalene-d8  
Concen: 20.000 ng  
RT: 10.97 min Scan# 1342  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Tgt Ion: 136 Resp: 174830  
Ion Ratio Lower Upper  
136 100  
137 10.2 9.1 13.7  
54 10.6 9.4 14.2  
68 6.2 4.2 6.4


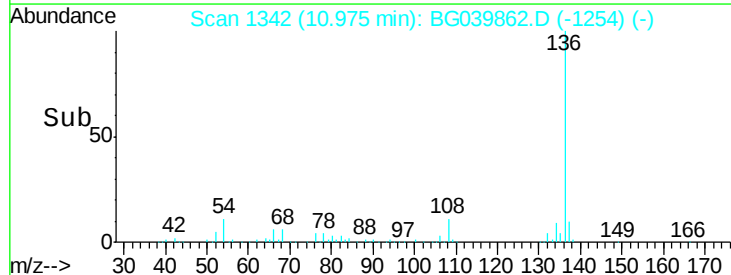
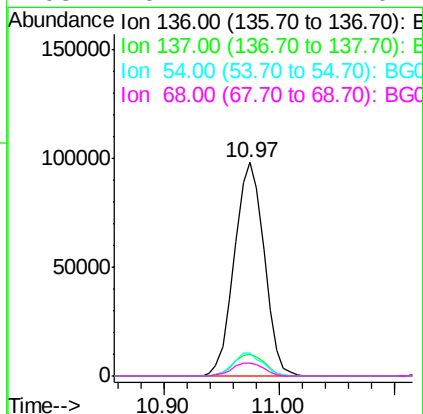



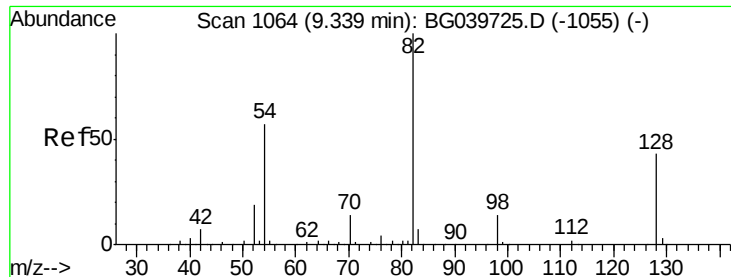

#23  
Nitrobenzene-d5  
Concen: 101.374 ng  
RT: 9.33 min Scan# 1062  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38




Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD


Tgt Ion: 82 Resp: 327698  
Ion Ratio Lower Upper  
82 100  
128 43.7 31.3 46.9  
54 58.6 50.9 76.3

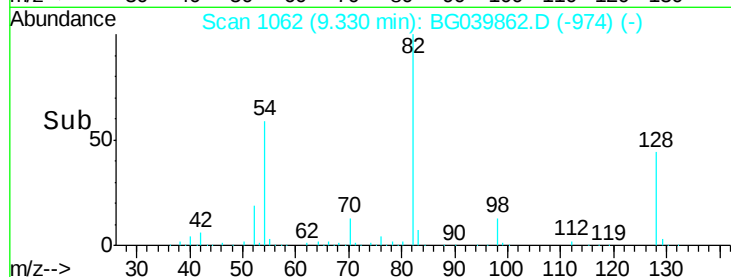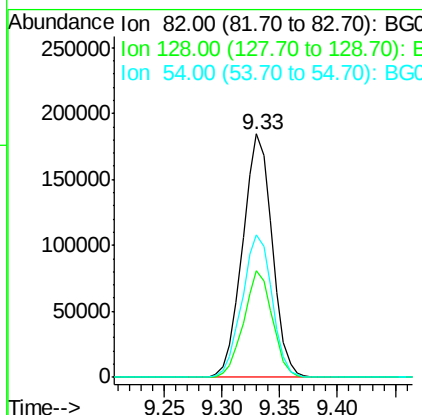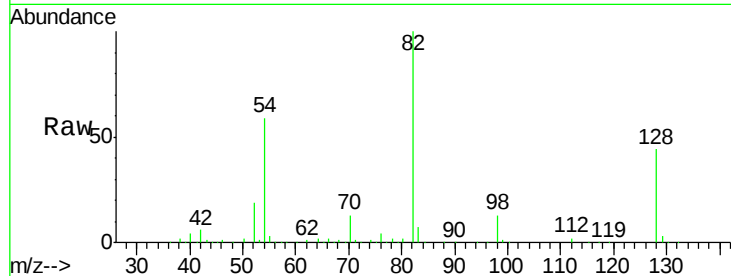

#31  
Naphthalene  
Concen: 5.714 ng  
RT: 11.03 min Scan# 1351  
Delta R.T. -0.01 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Tgt Ion: 128 Resp: 52891  
Ion Ratio Lower Upper  
128 100  
129 10.0 8.7 13.1  
127 12.6 10.8 16.2


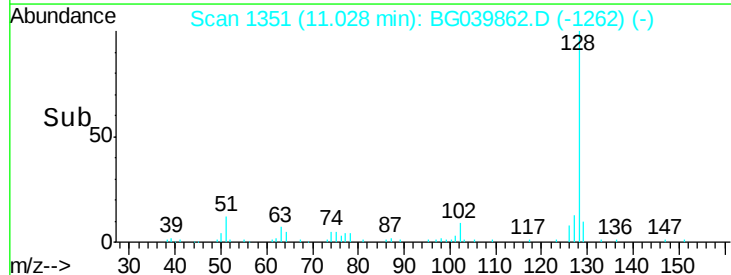
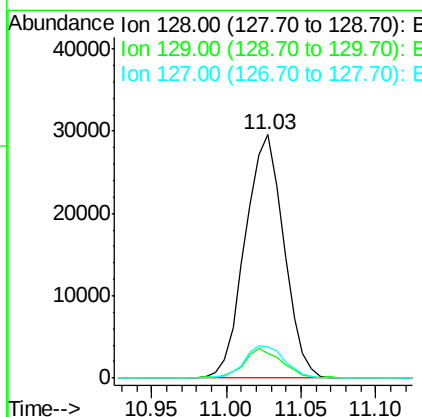





#32  
Benzoic acid  
Concen: 7.040 ng  
RT: 10.22 min Scan# 1214  
Delta R.T. -0.04 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38




Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD


Tgt Ion:122 Resp: 896  
Ion Ratio Lower Upper  
122 100  
105 113.4 101.8 141.8  
77 86.2 76.3 116.3

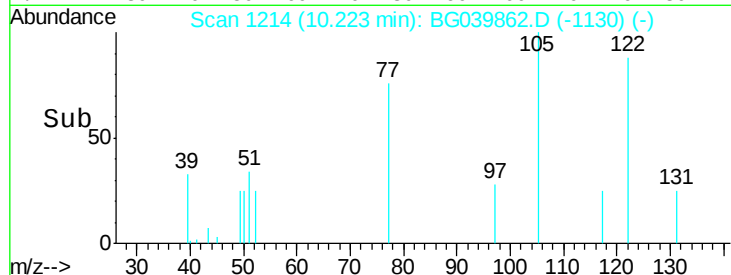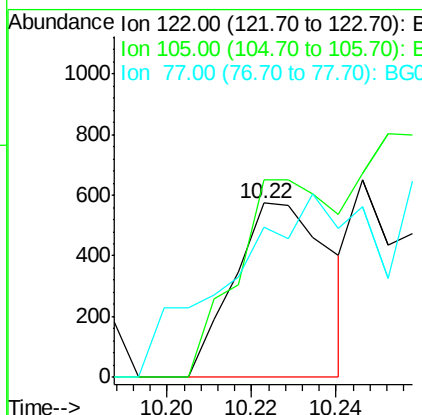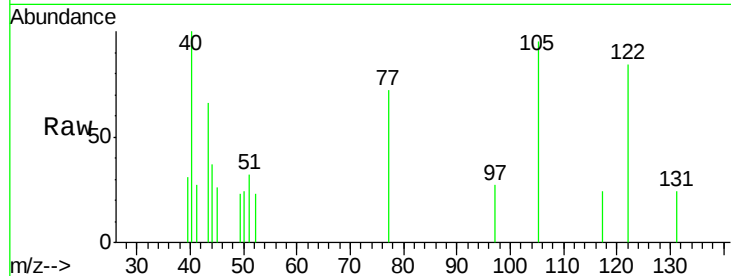

#37  
2-Methylnaphthalene  
Concen: 3.100 ng  
RT: 12.61 min Scan# 1621  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Tgt Ion:142 Resp: 21452  
Ion Ratio Lower Upper  
142 100  
141 94.7 73.5 110.3  
115 31.6 30.8 46.2

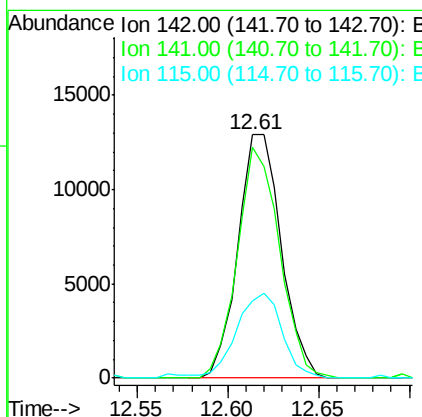







#39  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 14.78 min Scan# 1989  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD

Tgt Ion:164 Resp: 112300  
Ion Ratio Lower Upper  
164 100  
162 101.5 81.6 122.4  
160 42.4 34.2 51.2




Abundance Ion 164.00 (163.70 to 164.70): E  
Ion 162.00 (161.70 to 162.70): E  
Ion 160.00 (159.70 to 160.70): E

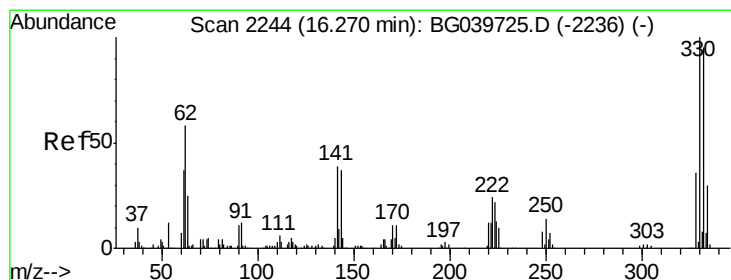
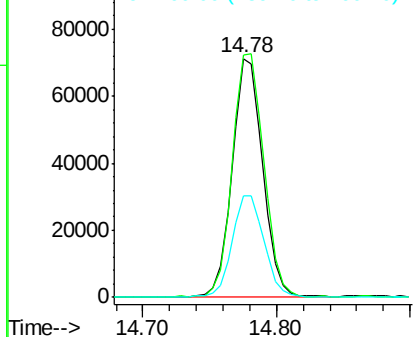



#42  
2,4,6-Tribromophenol  
Concen: 148.616 ng  
RT: 16.27 min Scan# 2243  
Delta R.T. -0.01 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Tgt Ion:330 Resp: 194529  
Ion Ratio Lower Upper  
330 100  
332 95.9 75.7 113.5  
141 42.8 35.6 53.4

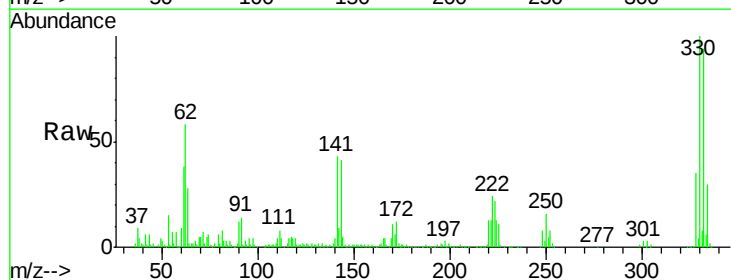

Abundance Ion 329.80 (329.50 to 330.50): E  
Ion 331.80 (331.50 to 332.50): E  
Ion 141.00 (140.70 to 141.70): E



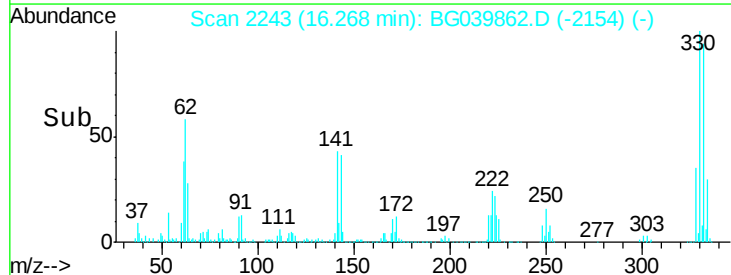
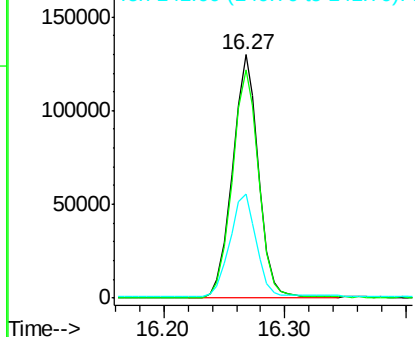




#45  
 2-Fluorobiphenyl  
 Concen: 100.127 ng  
 RT: 13.40 min Scan# 1755  
 Delta R.T. -0.02 min  
 Lab File: BG039862.D  
 Acq: 12 Mar 2019 5:38




Instrument :  
 BNA\_G  
 ClientSampleId :  
 3-8-BOD


Tgt Ion:172 Resp: 789717  
 Ion Ratio Lower Upper  
 172 100  
 171 38.0 30.8 46.2  
 170 25.7 20.2 30.4

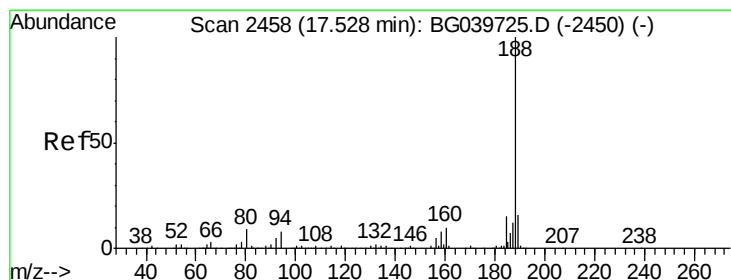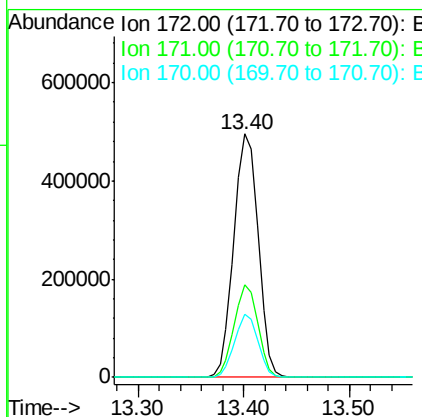

#64  
 Phenanthrene-d10  
 Concen: 20.000 ng  
 RT: 17.52 min Scan# 2457  
 Delta R.T. -0.01 min  
 Lab File: BG039862.D  
 Acq: 12 Mar 2019 5:38

Tgt Ion:188 Resp: 263656  
 Ion Ratio Lower Upper  
 188 100  
 94 8.2 6.9 10.3  
 80 9.1 8.1 12.1



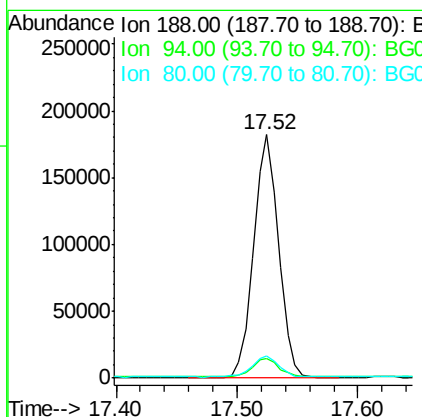
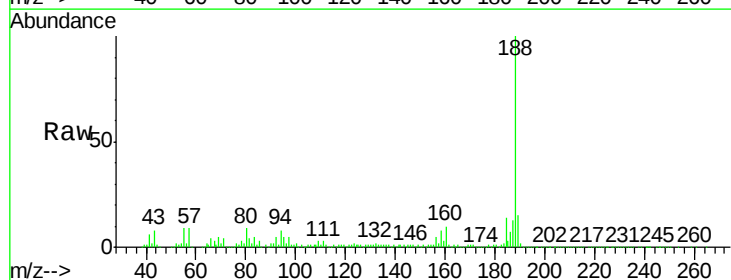




#76  
Chrysene-d12  
Concen: 20.000 ng  
RT: 21.81 min Scan# 3187  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38




Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD


Tgt Ion:240 Resp: 304272  
Ion Ratio Lower Upper  
240 100  
120 8.0 7.0 10.6  
236 26.7 21.0 31.4

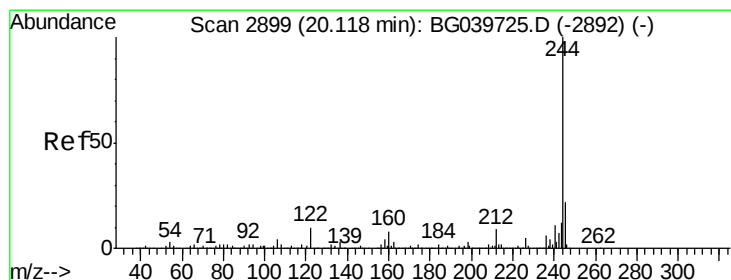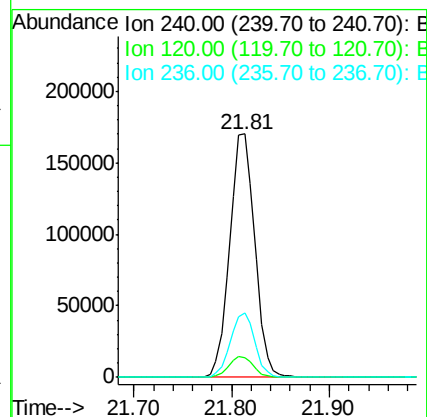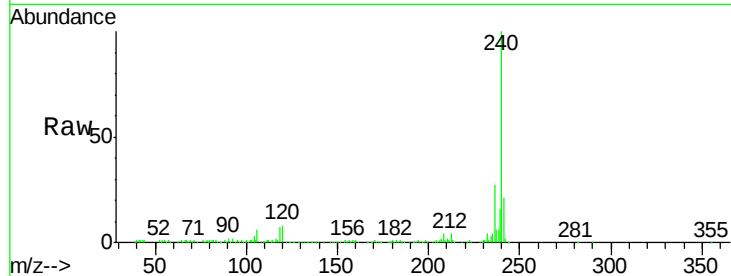

#79  
Terphenyl-d14  
Concen: 87.842 ng  
RT: 20.12 min Scan# 2898  
Delta R.T. -0.01 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Tgt Ion:244 Resp: 1213904  
Ion Ratio Lower Upper  
244 100  
212 9.5 7.3 10.9  
122 9.9 8.4 12.6

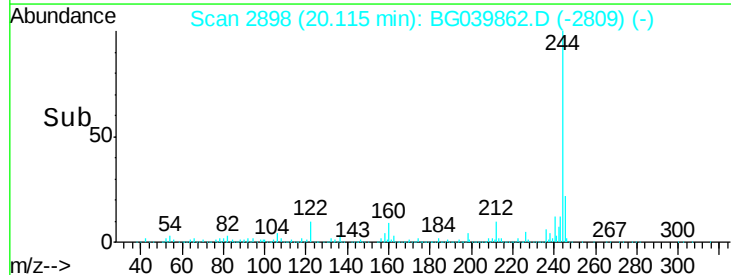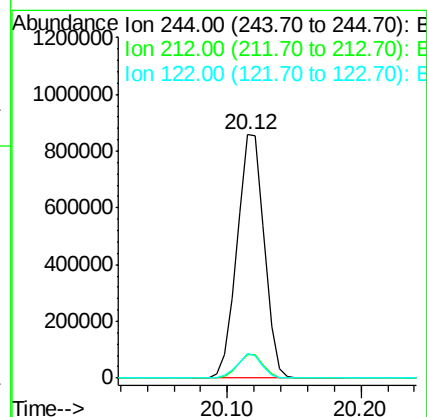


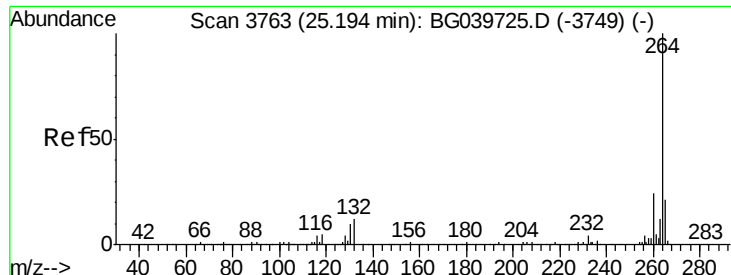

#87  
Perylene-d12  
Concen: 20.000 ng  
RT: 25.18 min Scan# 3761  
Delta R.T. -0.02 min  
Lab File: BG039862.D  
Acq: 12 Mar 2019 5:38

Instrument :  
BNA\_G  
ClientSampleId :  
3-8-BOD

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 264     | 100   |       |       |
| 260     | 24.6  | 18.2  | 27.4  |
| 265     | 21.0  | 18.5  | 27.7  |

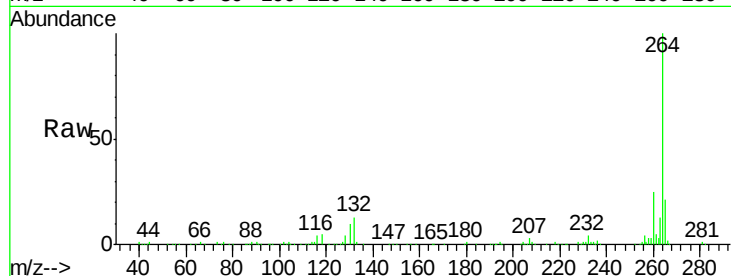

Abundance Ion 264.00 (263.70 to 264.70): E  
Ion 260.00 (259.70 to 260.70): E  
Ion 265.00 (264.70 to 265.70): E

