
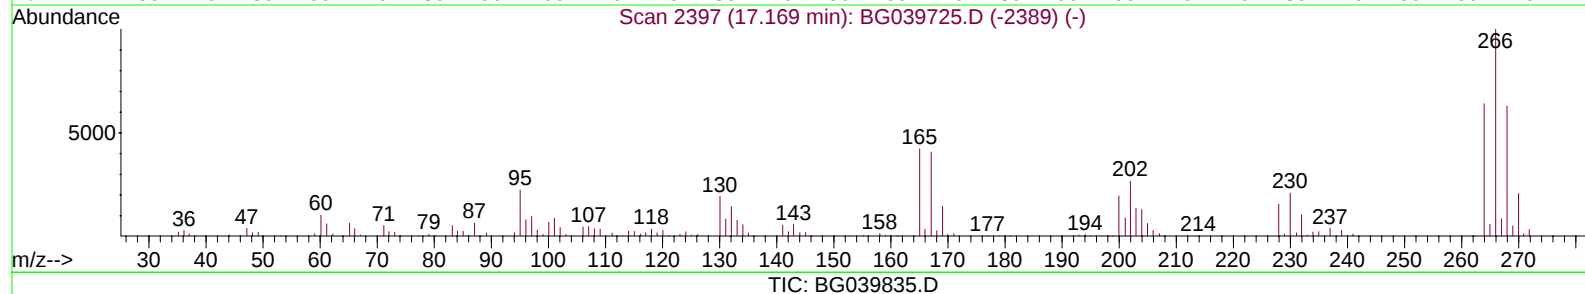
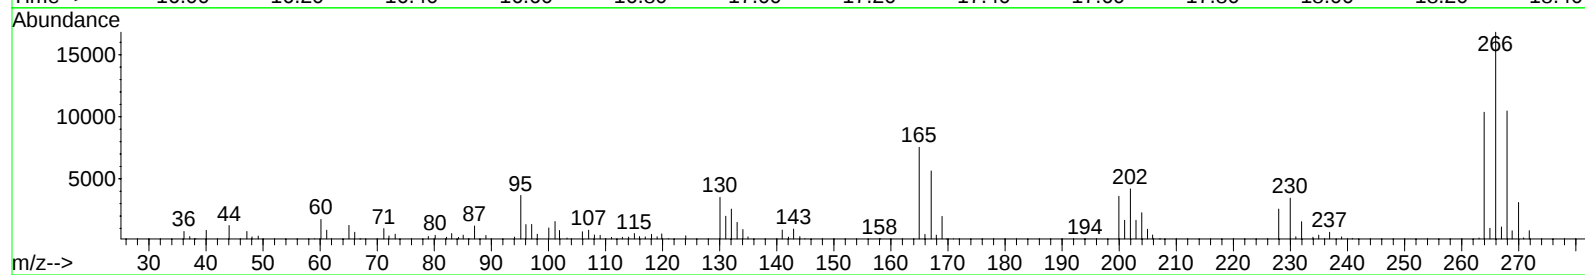


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031119\
Data File : BG039835.D
Acq On : 11 Mar 2019 9:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 16:31:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

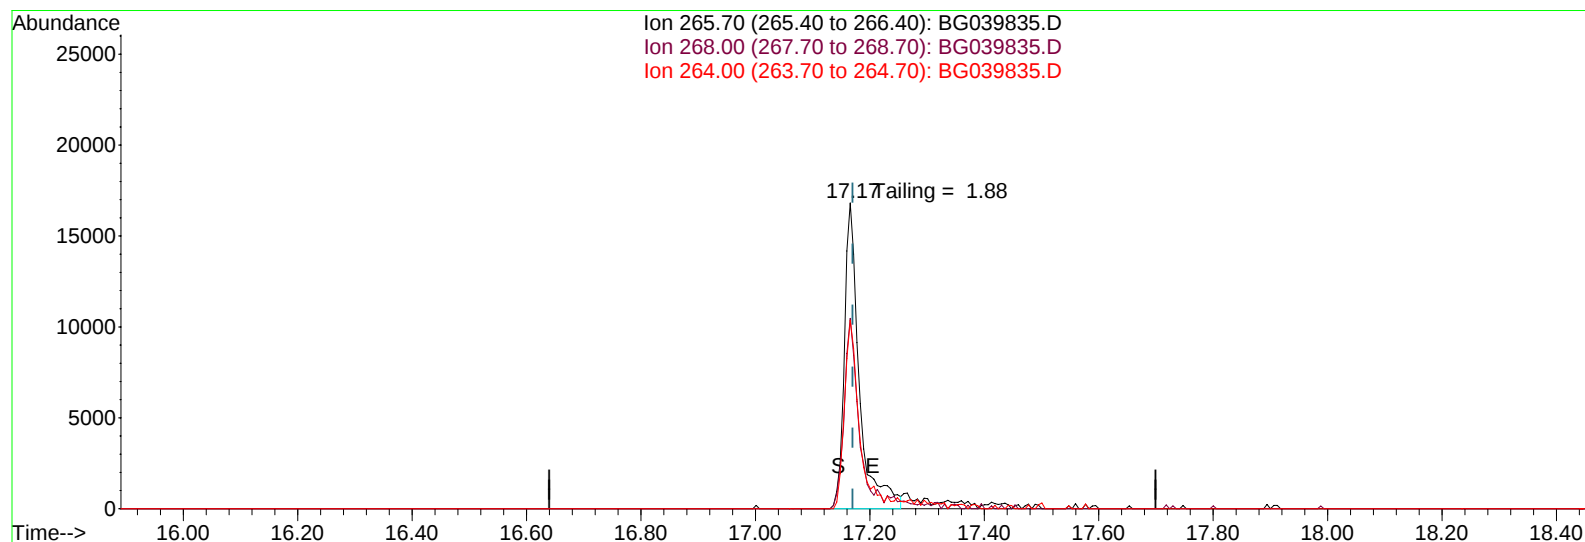

(70) Pentachlorophenol (C)




17.166min (-0.004) 24996.54ng

response 30772

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.28
264.00	65.10	61.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031119\
 Data File : BG039835.D
 Acq On : 11 Mar 2019 9:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 16:31:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

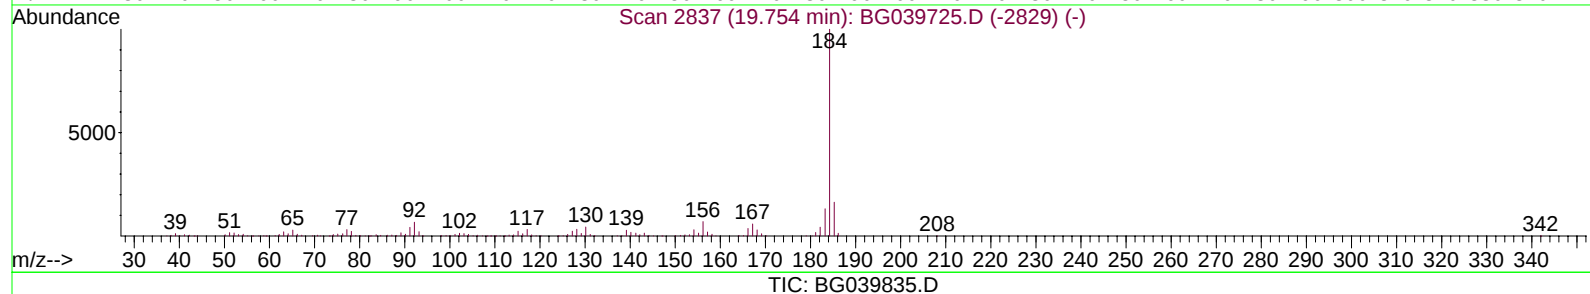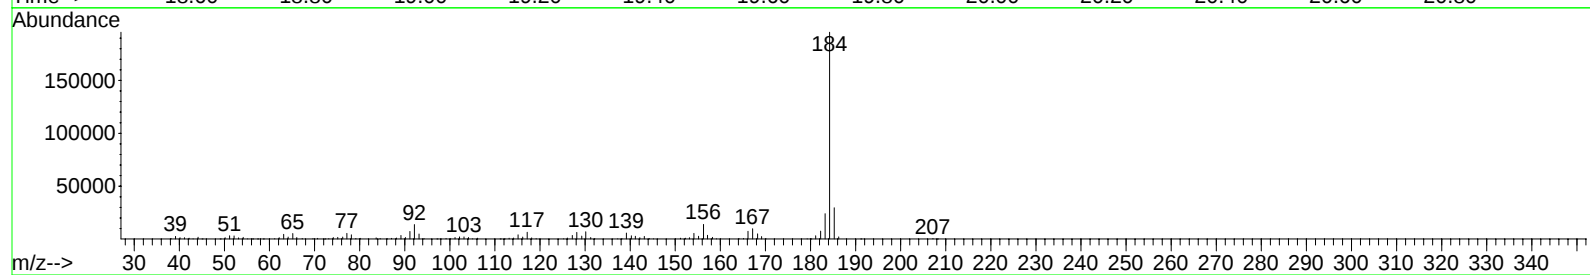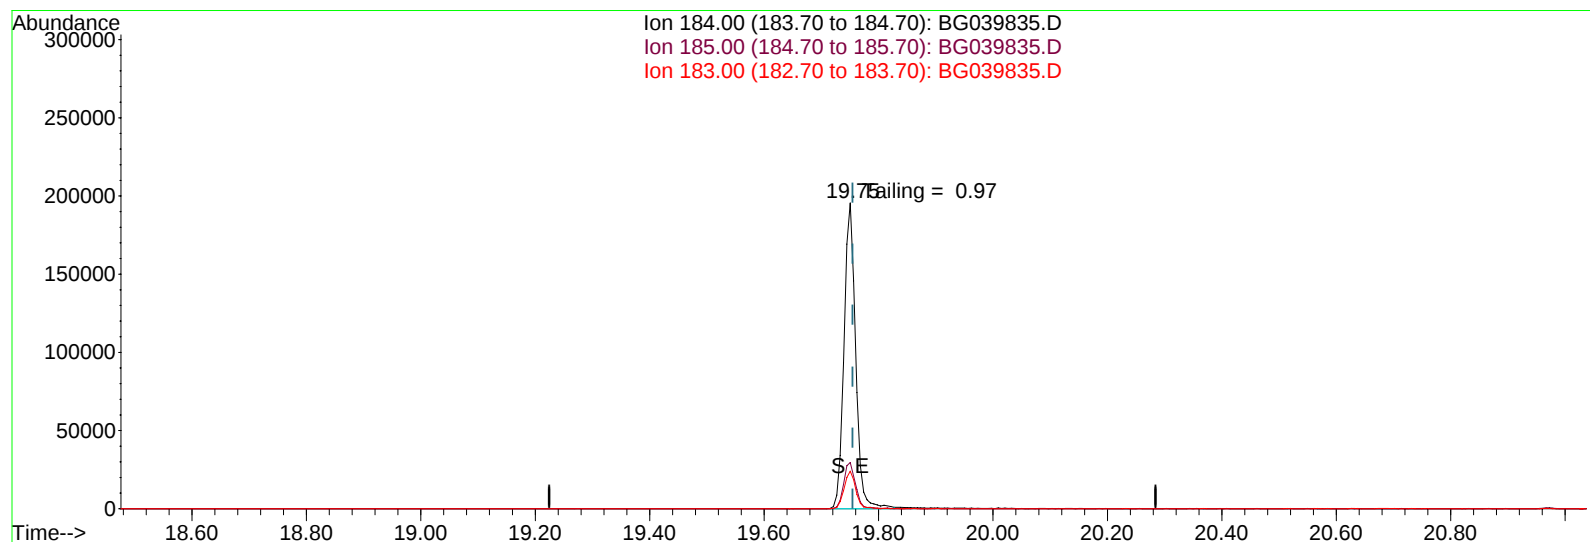

(77) Benzidine

19.751min (-0.004) 33653.57ng

response 278729

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.15
183.00	13.20	12.29
0.00	0.00	0.00