


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031119\
 Data File : BG039854.D
 Acq On : 12 Mar 2019 00:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

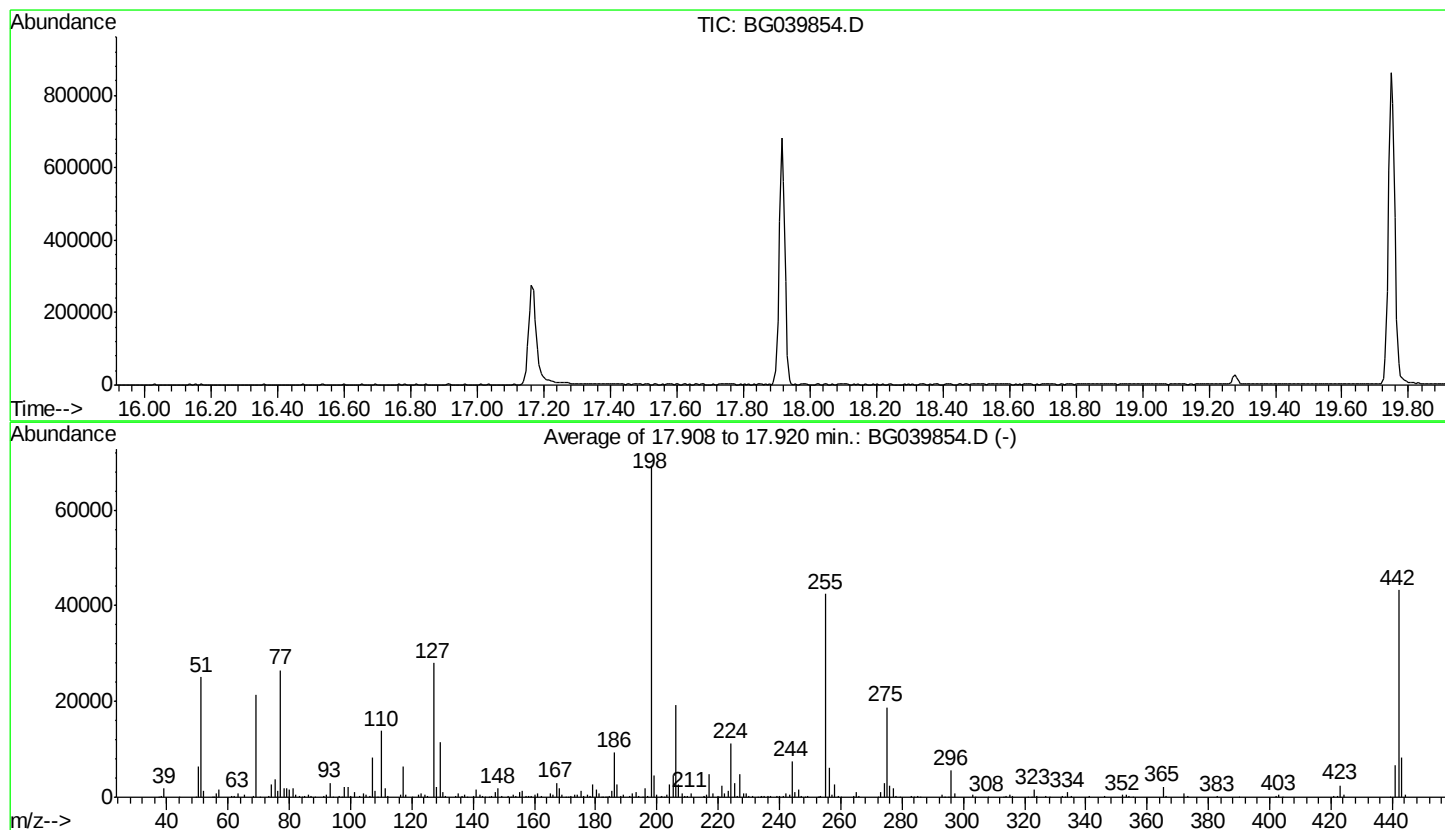

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	25130	PASS
68	69	0.00	2	0.9	199	PASS
69	198	0.00	100	31.1	21530	PASS
70	69	0.00	2	0.2	52	PASS
127	198	10	80	40.4	27978	PASS
197	198	0.00	2	0.3	197	PASS
198	198	100	100	100.0	69261	PASS
199	198	5	9	6.6	4594	PASS
275	198	10	60	27.1	18739	PASS
365	198	1	100	3.2	2219	PASS
441	198	0.01	100	9.8	6811	PASS
442	198	50	100	62.5	43296	PASS
443	442	15	24	19.2	8327	PASS