
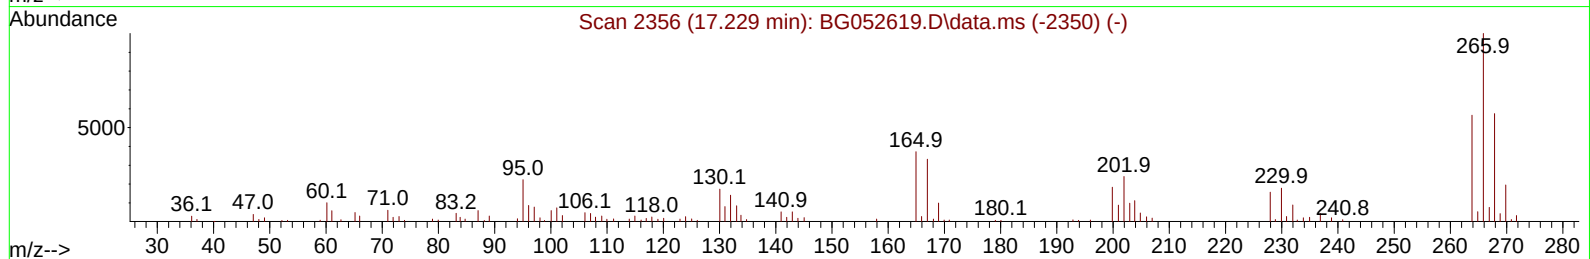
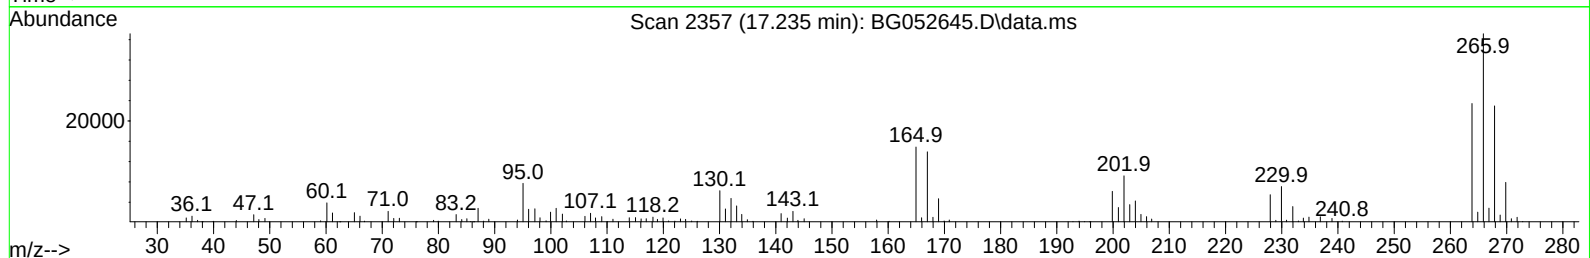


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052645.D
Acq On : 11 Mar 2022 13:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 14:02:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

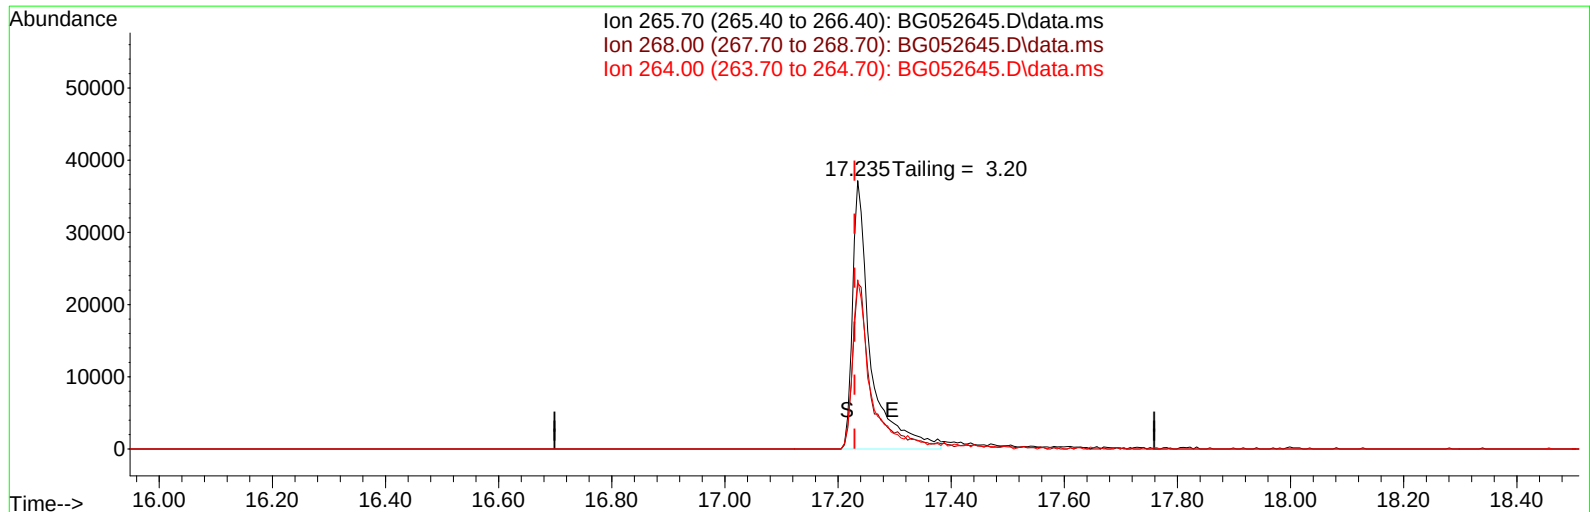

TIC: BG052645.D\data.ms

(70) Pentachlorophenol (C)




17.235min (+ 0.006) 194681.34 ng

response 81987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.76
264.00	56.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052645.D
Acq On : 11 Mar 2022 13:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 14:02:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

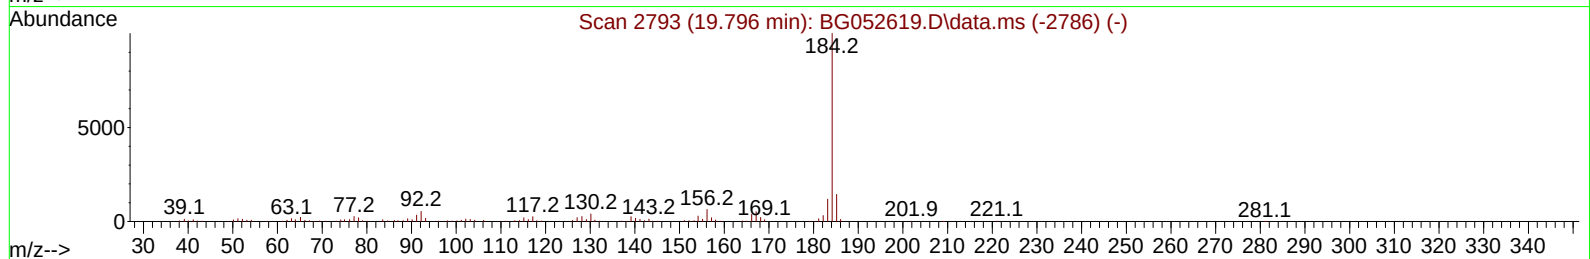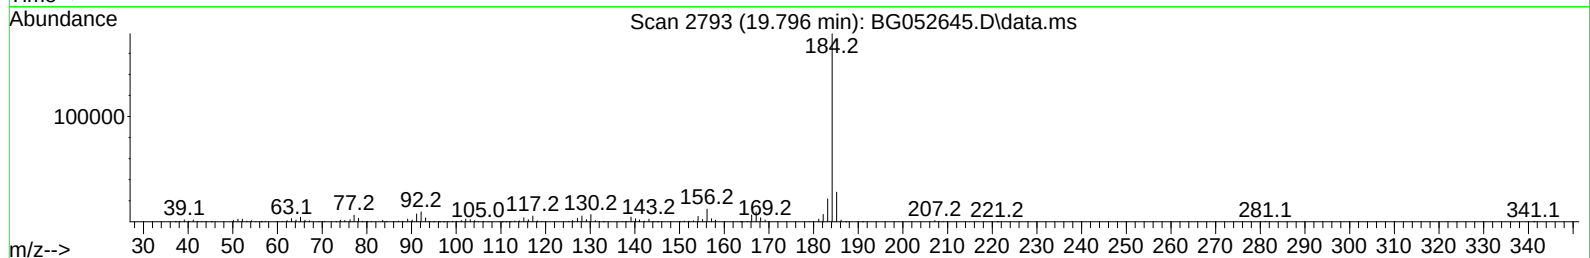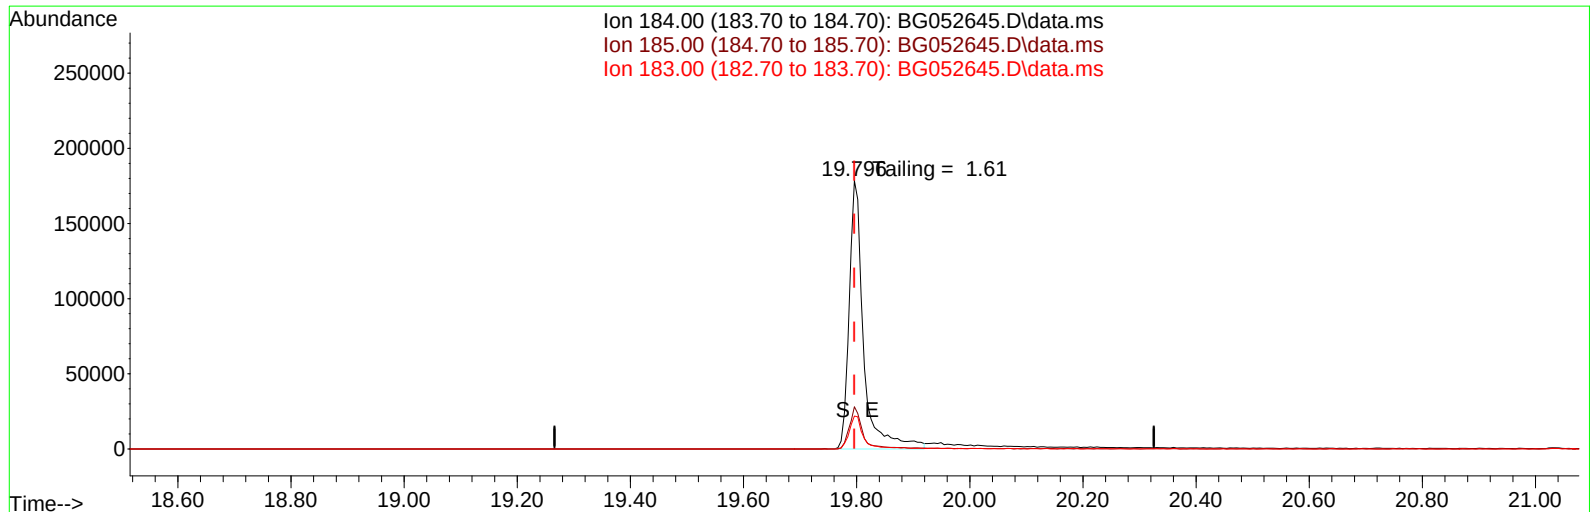

TIC: BG052645.D\data.ms

(77) Benzidine**19.796min (+ 0.000) 275781.70 ng****response 308932**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.78
183.00	11.80	12.29
0.00	0.00	0.00