

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
 Data File : BG052655.D
 Acq On : 11 Mar 2022 20:10
 Operator : CG/JU
 Sample : N1845-01 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.215	306	311	316	rVB2	8516	13987	2.65%	0.342%
2	5.702	388	394	403	rBV	70566	117636	22.26%	2.875%
3	7.323	663	670	682	rBV	81920	151177	28.61%	3.694%
4	8.169	806	814	823	rBV	134773	229895	43.51%	5.618%
5	9.344	1007	1014	1022	rBV2	54345	103303	19.55%	2.524%
6	11.007	1288	1297	1310	rBV	182407	333687	63.15%	8.154%
7	13.445	1705	1712	1722	rBV	167470	261375	49.46%	6.387%
8	14.825	1940	1947	1953	rBV	302767	465395	88.07%	11.373%
9	14.884	1954	1957	1965	rVB2	4737	6351	1.20%	0.155%
10	15.871	2119	2125	2129	rBV6	7577	11809	2.23%	0.289%
11	16.311	2196	2200	2211	rVB2	55716	93636	17.72%	2.288%
12	17.298	2363	2368	2374	rBV8	6158	13026	2.47%	0.318%
13	17.574	2408	2415	2420	rBV	336778	528422	100.00%	12.913%
14	17.615	2420	2422	2429	rVB	64435	84854	16.06%	2.074%
15	17.709	2435	2438	2443	rVB	13988	17515	3.31%	0.428%
16	17.980	2478	2484	2486	rBV5	5497	8770	1.66%	0.214%
17	18.050	2491	2496	2498	rBV5	4732	6659	1.26%	0.163%
18	18.455	2558	2565	2568	rBV2	12579	24420	4.62%	0.597%
19	18.502	2568	2573	2578	rVB	14411	25486	4.82%	0.623%
20	18.649	2594	2598	2601	rBV6	10996	16730	3.17%	0.409%
21	18.843	2629	2631	2636	rBV6	5918	9132	1.73%	0.223%
22	18.943	2644	2648	2649	rBV3	8072	7239	1.37%	0.177%
23	19.354	2716	2718	2723	rVB5	10226	14338	2.71%	0.350%
24	19.624	2759	2764	2769	rBV	95178	136959	25.92%	3.347%
25	19.983	2822	2825	2832	rVB	79069	123824	23.43%	3.026%
26	20.171	2852	2857	2865	rBV	256163	332182	62.86%	8.118%
27	21.886	3142	3149	3155	rBV	269230	507283	96.00%	12.396%
28	25.323	3727	3734	3745	rVB2	152117	447080	84.61%	10.925%




Sum of corrected areas: 4092170

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052655.D
Acq On : 11 Mar 2022 20:10
Operator : CG/JU
Sample : N1845-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

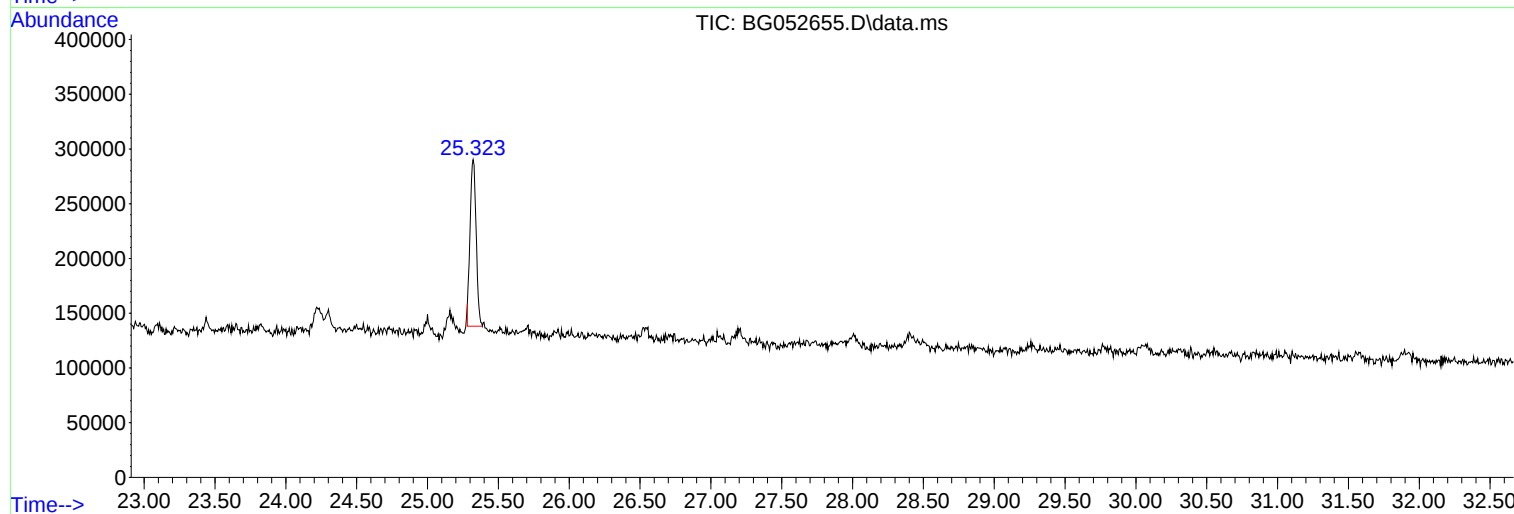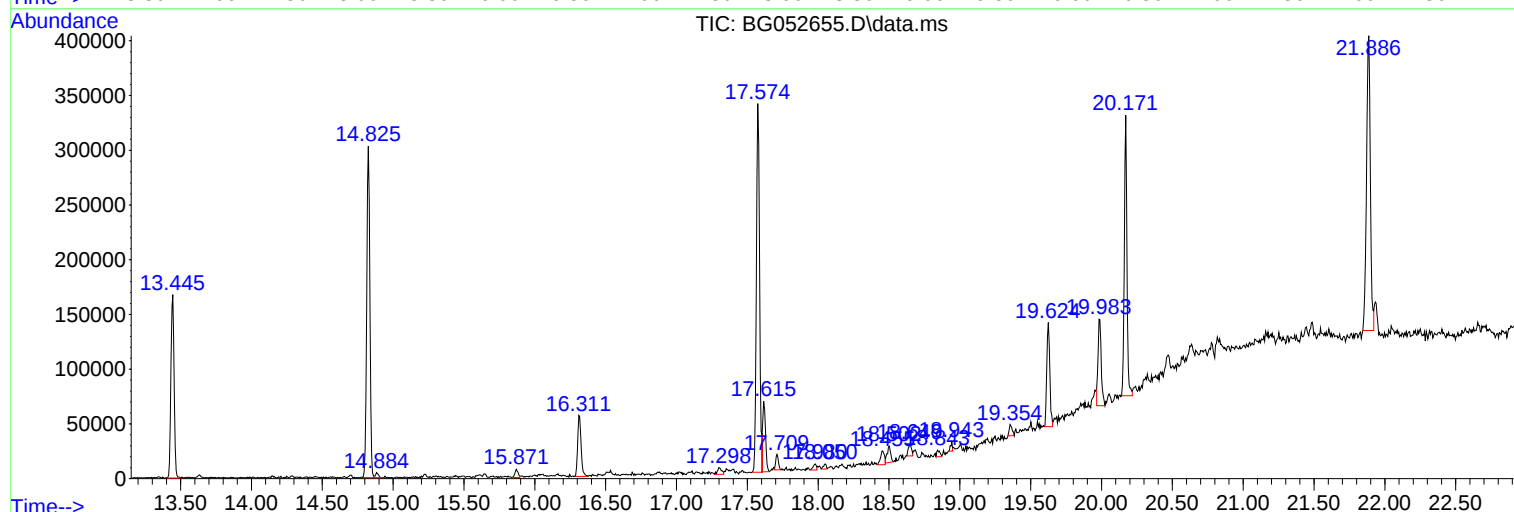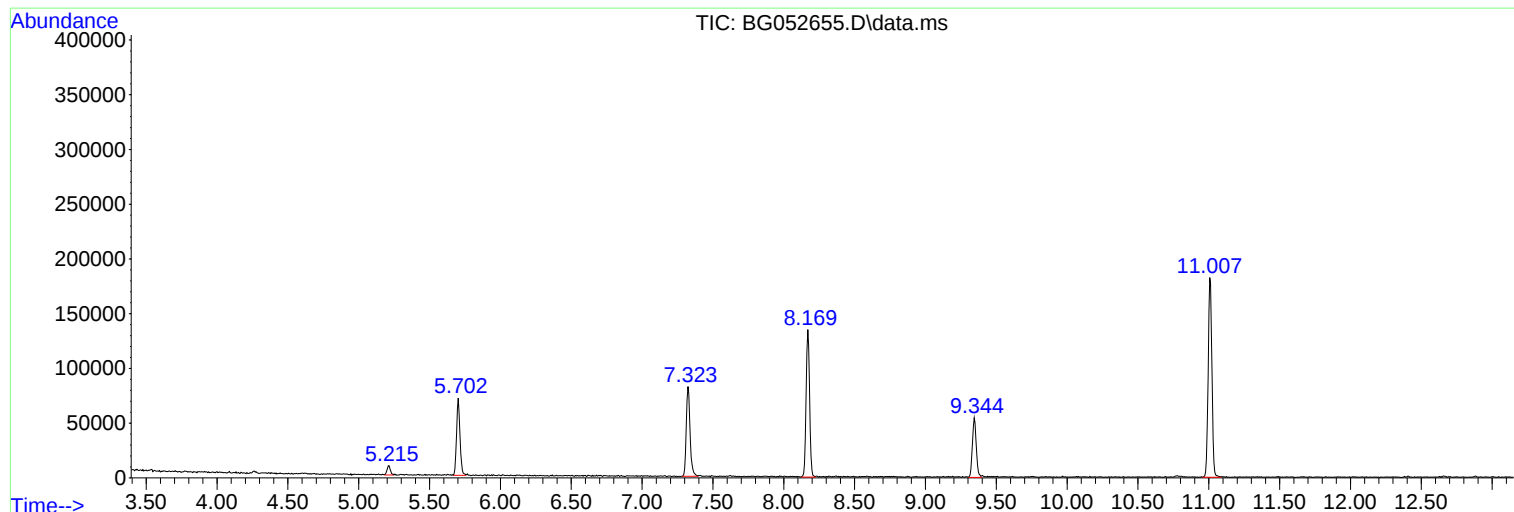

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052655.D
Acq On : 11 Mar 2022 20:10
Operator : CG/JU
Sample : N1845-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052655.D
Acq On : 11 Mar 2022 20:10
Operator : CG/JU
Sample : N1845-01 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------