
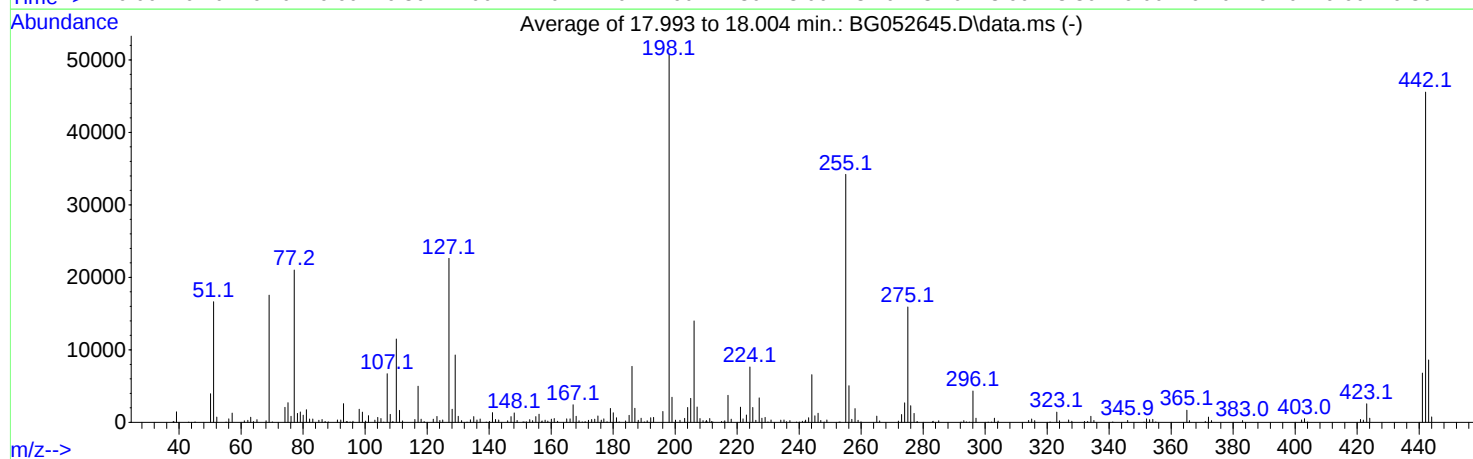


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
 Data File : BG052645.D
 Acq On : 11 Mar 2022 13:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 06:37:54 2022

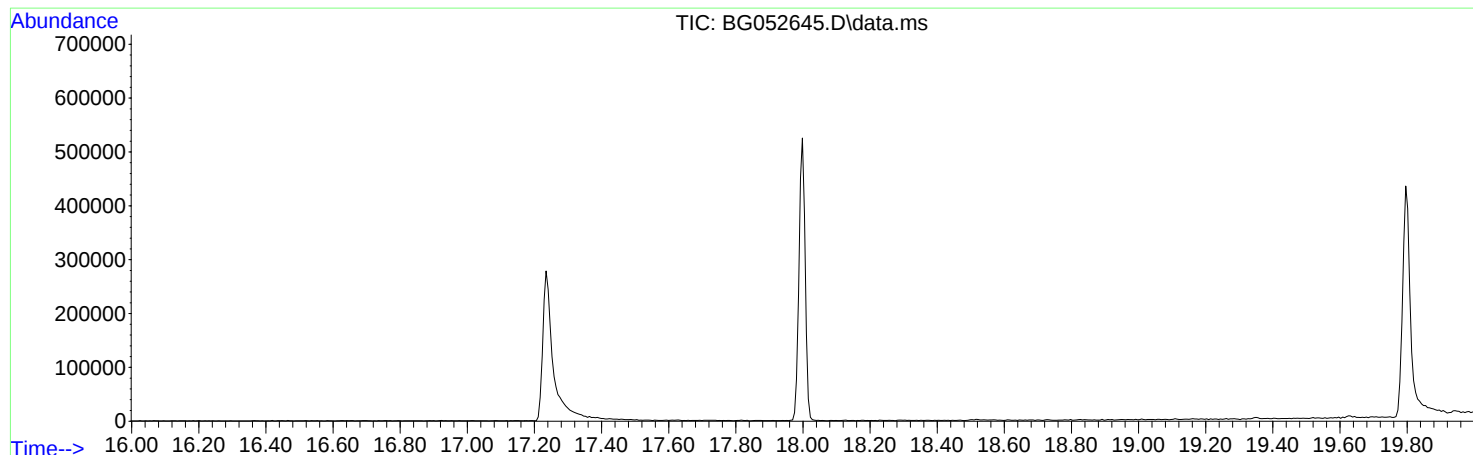




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	16646	PASS
68	69	0.00	2	1.3	233	PASS
69	198	0.00	100	34.6	17543	PASS
70	69	0.00	2	0.4	62	PASS
127	198	10	80	44.6	22619	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50744	PASS
199	198	5	9	6.8	3456	PASS
275	198	10	60	31.4	15918	PASS
365	198	1	100	3.3	1687	PASS
441	198	0.01	100	13.4	6796	PASS
442	442	50	100	100.0	45549	PASS
443	442	15	24	18.9	8601	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052645.D
Acq On : 11 Mar 2022 13:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 11 14:02:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

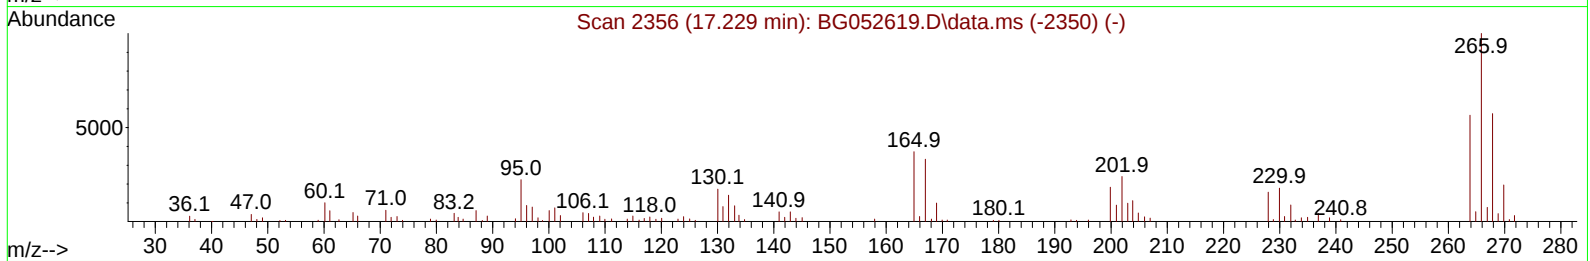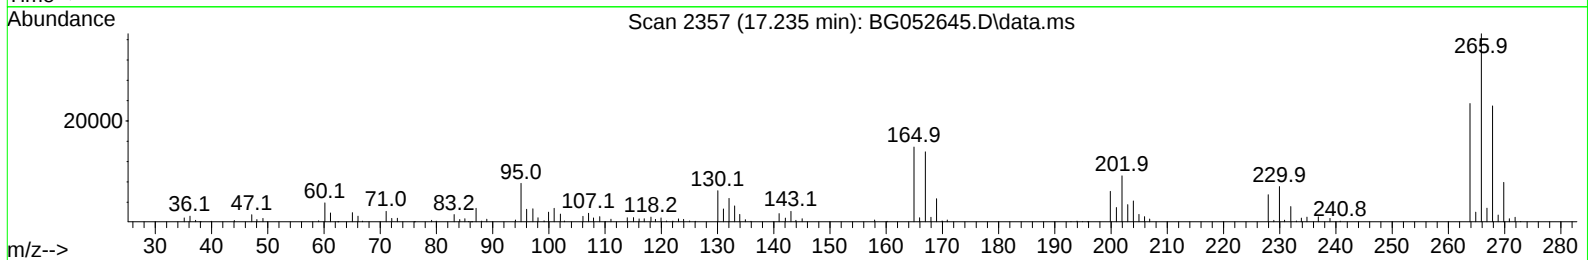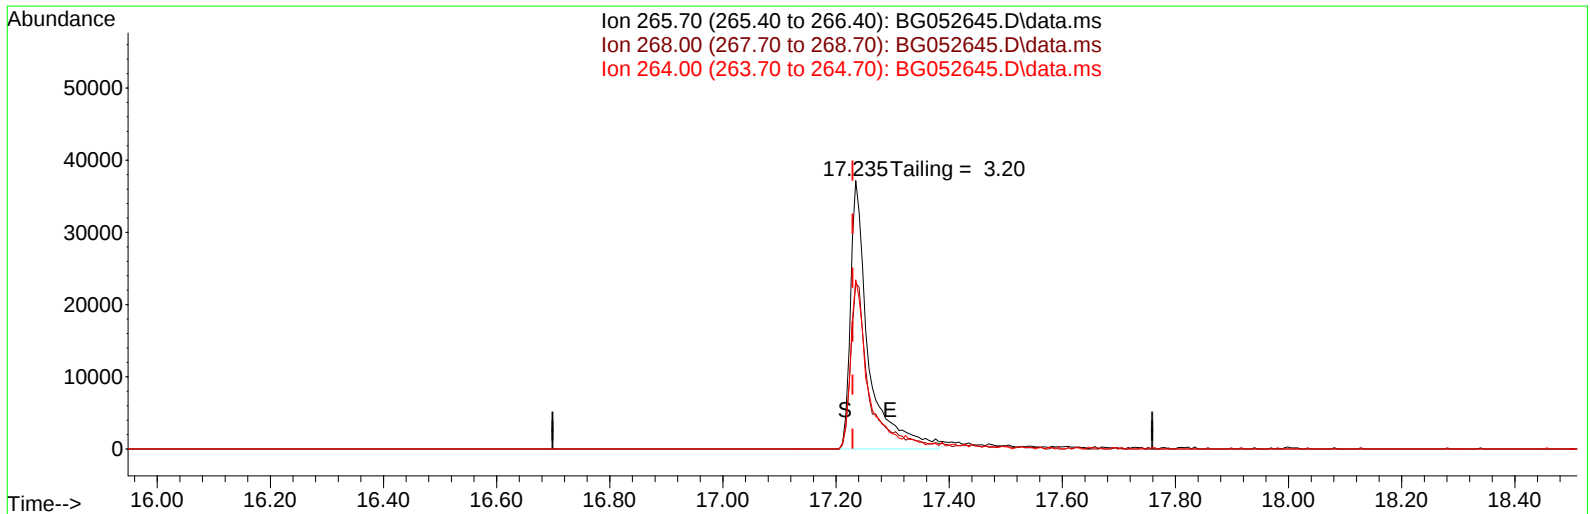

TIC: BG052645.D\data.ms

(70) Pentachlorophenol (C)

17.235min (+ 0.006) 194681.34 ng




response 81987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.76
264.00	56.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031122\
Data File : BG052645.D
Acq On : 11 Mar 2022 13:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 11 14:02:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

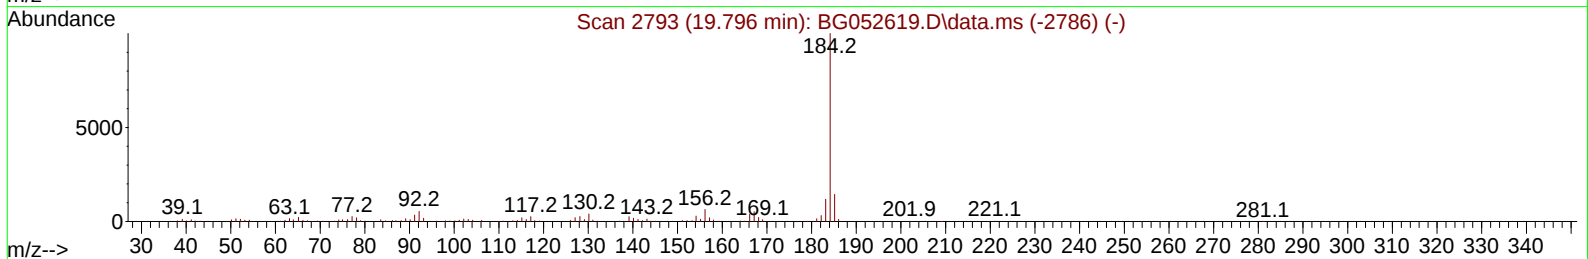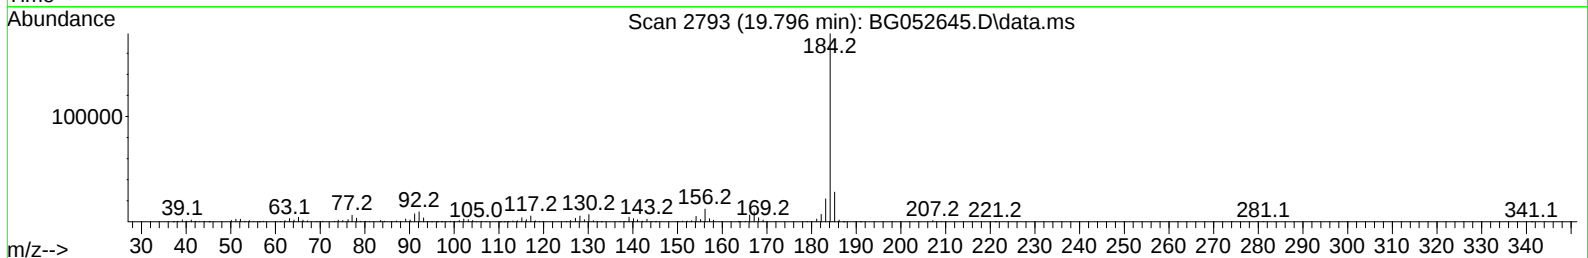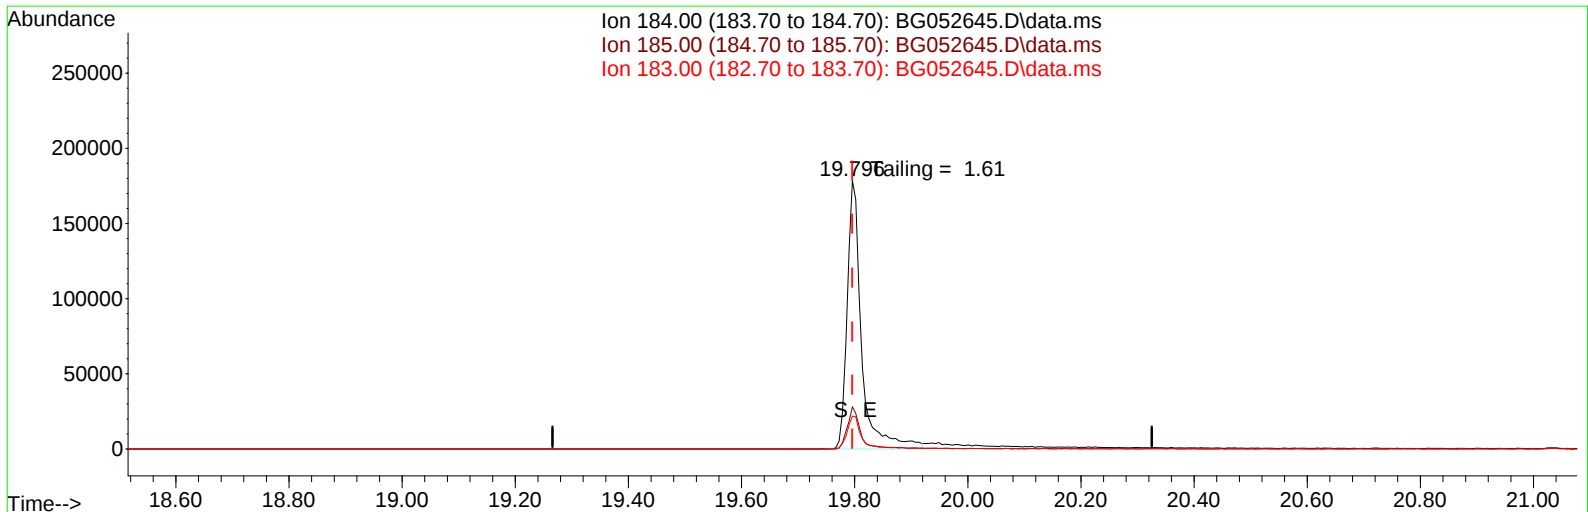

TIC: BG052645.D\data.ms

(77) Benzidine

19.796min (+ 0.000) 275781.70 ng

response 308932

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.78
183.00	11.80	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/11/2022	BNA_G	<u>BG052645.D</u>
Compound Name	Response	Retention Time
DDT	183278	21.036
DDD	2294	20.63
DDE	0	20.025
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2294	185572	1.24

Instrument :
BNA_G
ClientSampleId :
DFTPP