


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031519\
 Data File : BG039936.D
 Acq On : 15 Mar 2019 11:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

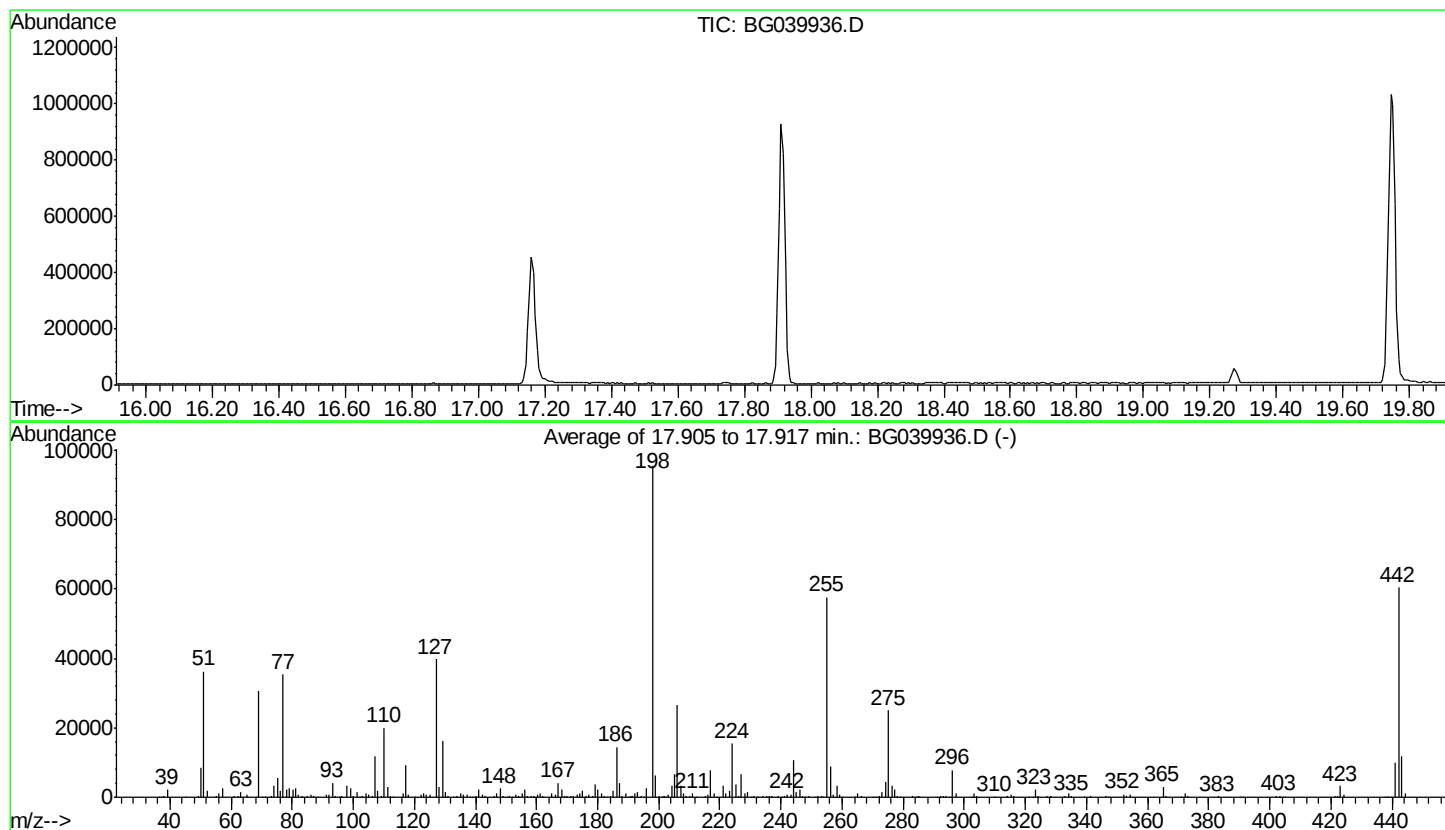

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	36298	PASS
68	69	0.00	2	0.5	166	PASS
69	198	0.00	100	32.1	30696	PASS
70	69	0.00	2	0.2	67	PASS
127	198	10	80	41.5	39685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95528	PASS
199	198	5	9	6.7	6389	PASS
275	198	10	60	26.2	25018	PASS
365	198	1	100	3.2	3081	PASS
441	198	0.01	100	10.3	9855	PASS
442	198	50	100	63.3	60429	PASS
443	442	15	24	19.8	11995	PASS