


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031519\
 Data File : BG039955.D
 Acq On : 16 Mar 2019 00:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

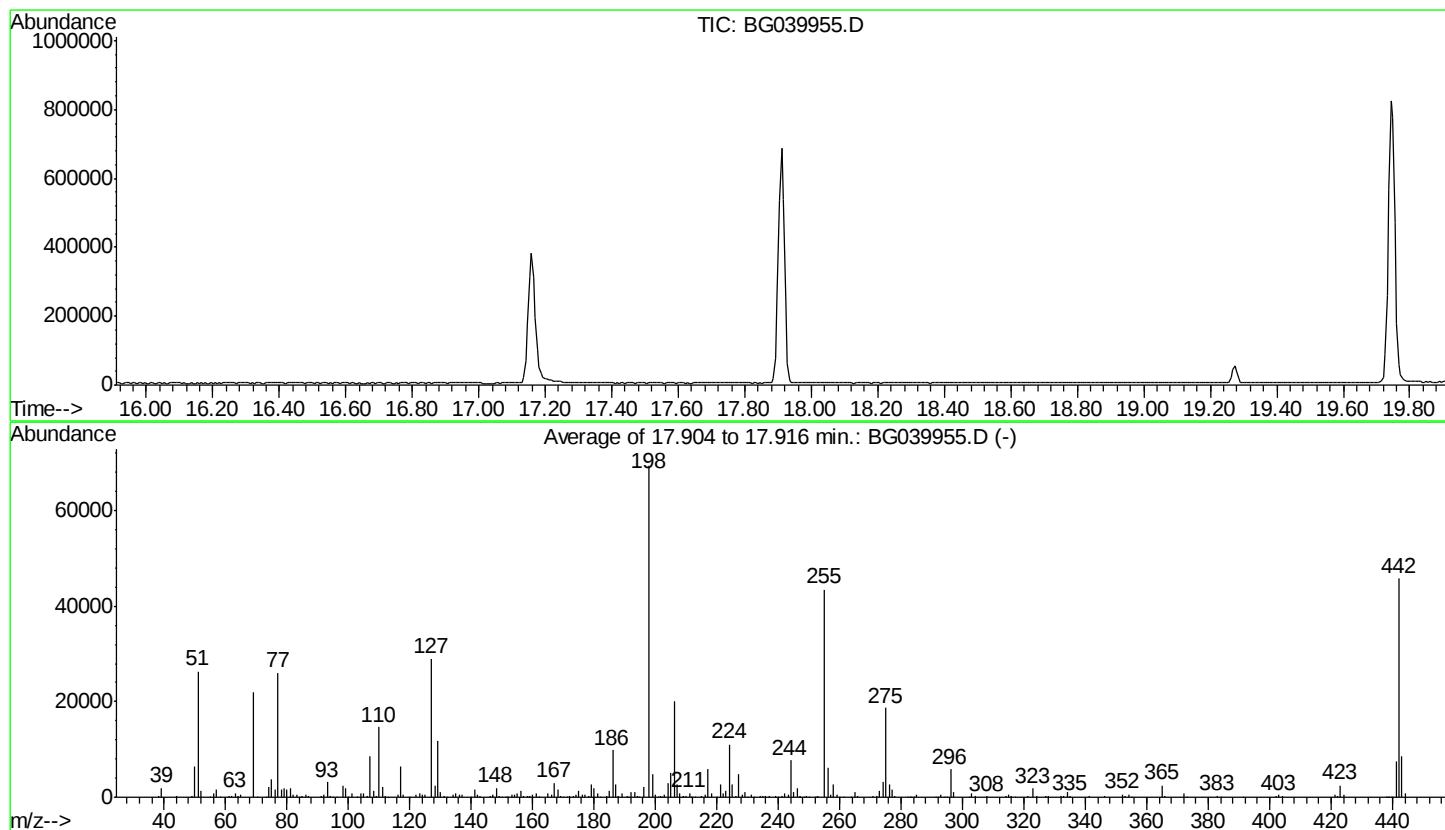

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	26360	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.8	22048	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	41.8	29016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69424	PASS
199	198	5	9	7.0	4881	PASS
275	198	10	60	26.9	18706	PASS
365	198	1	100	3.6	2518	PASS
441	198	0.01	100	10.8	7475	PASS
442	198	50	100	65.8	45714	PASS
443	442	15	24	18.6	8490	PASS