
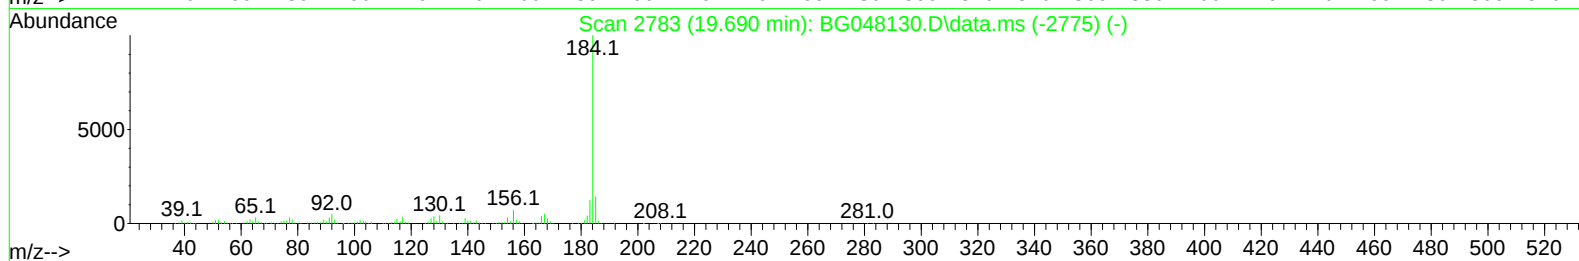
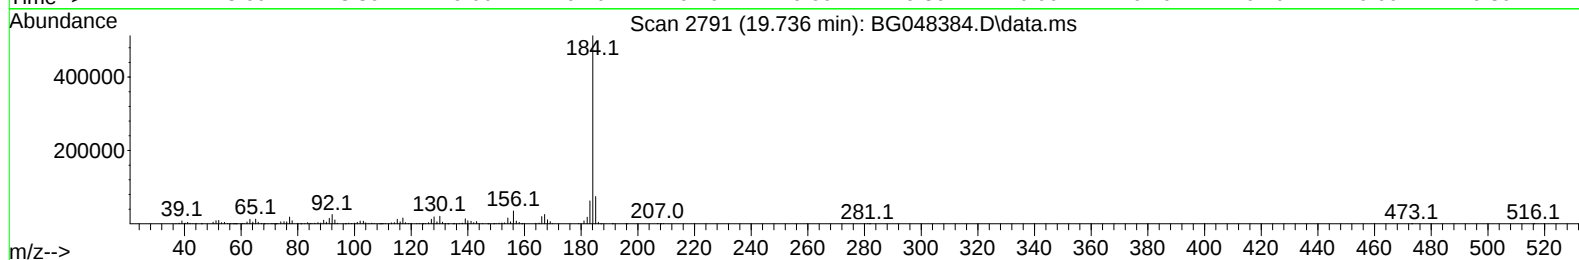


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031621\
Data File : BG048384.D
Acq On : 16 Mar 2021 8:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 10:55:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 16 10:42:19 2021
Response via : Initial Calibration

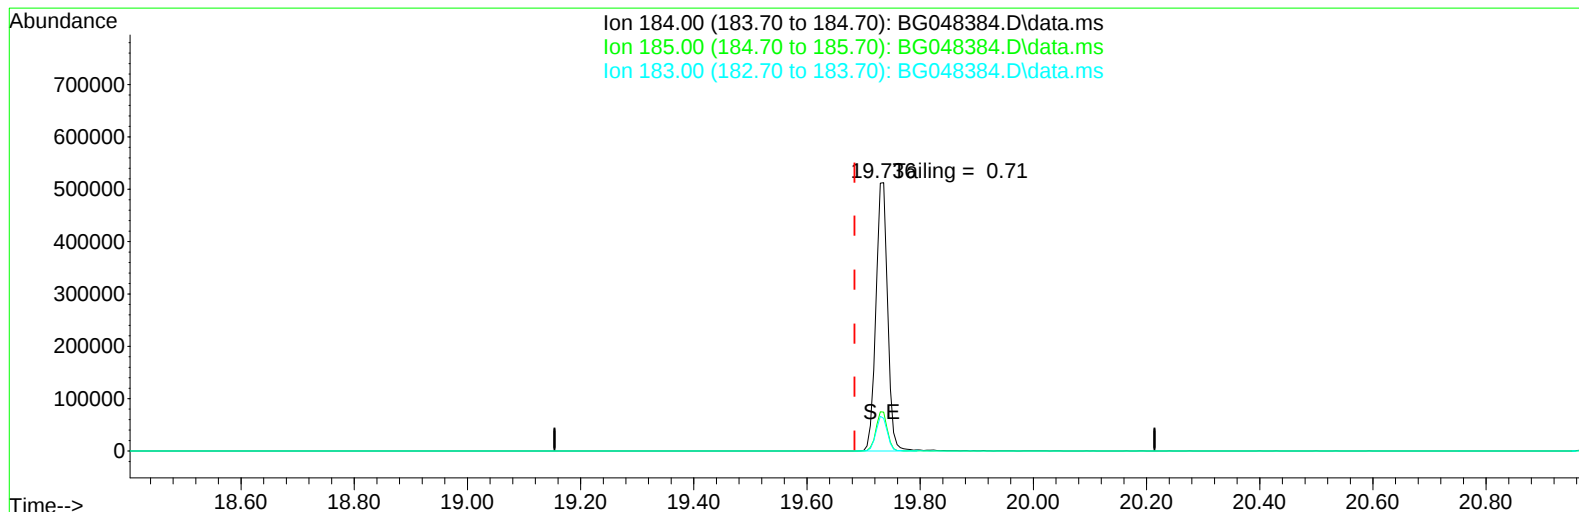




TIC: BG048384.D\data.ms

(77) Benzidine**19.736min (+ 0.052) 342296.28 ng****response 738164**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031621\
 Data File : BG048384.D
 Acq On : 16 Mar 2021 8:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 10:55:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 16 10:42:19 2021
 Response via : Initial Calibration

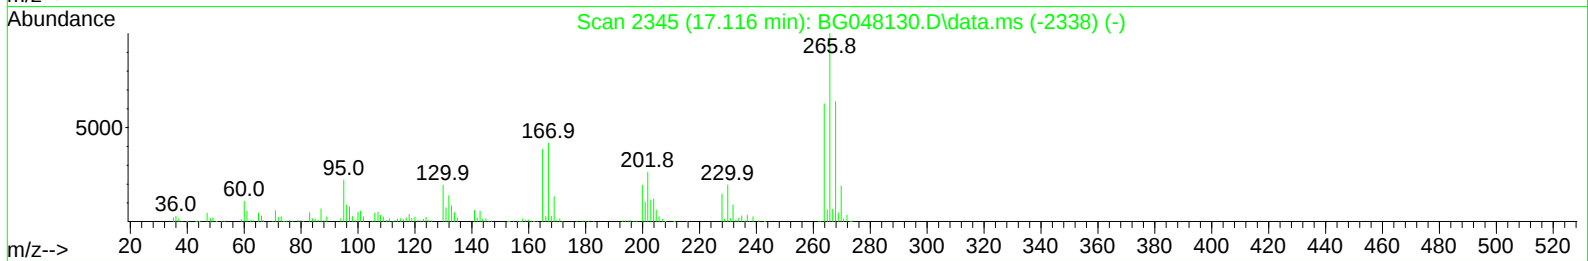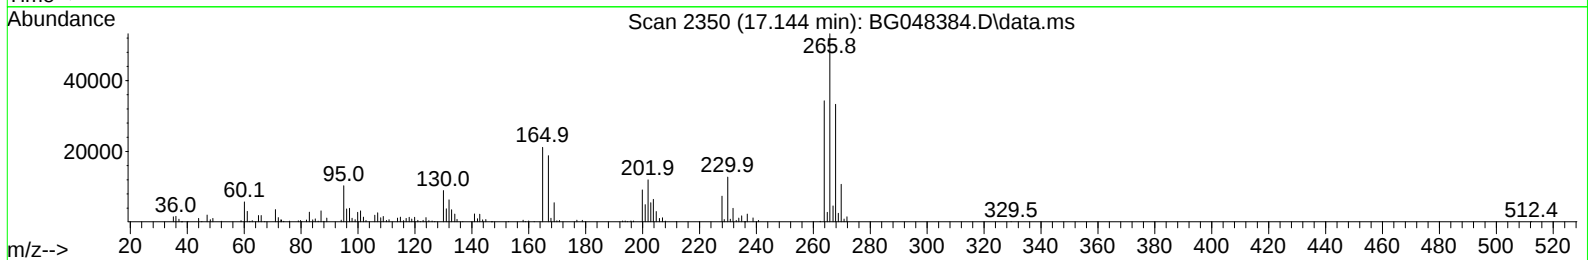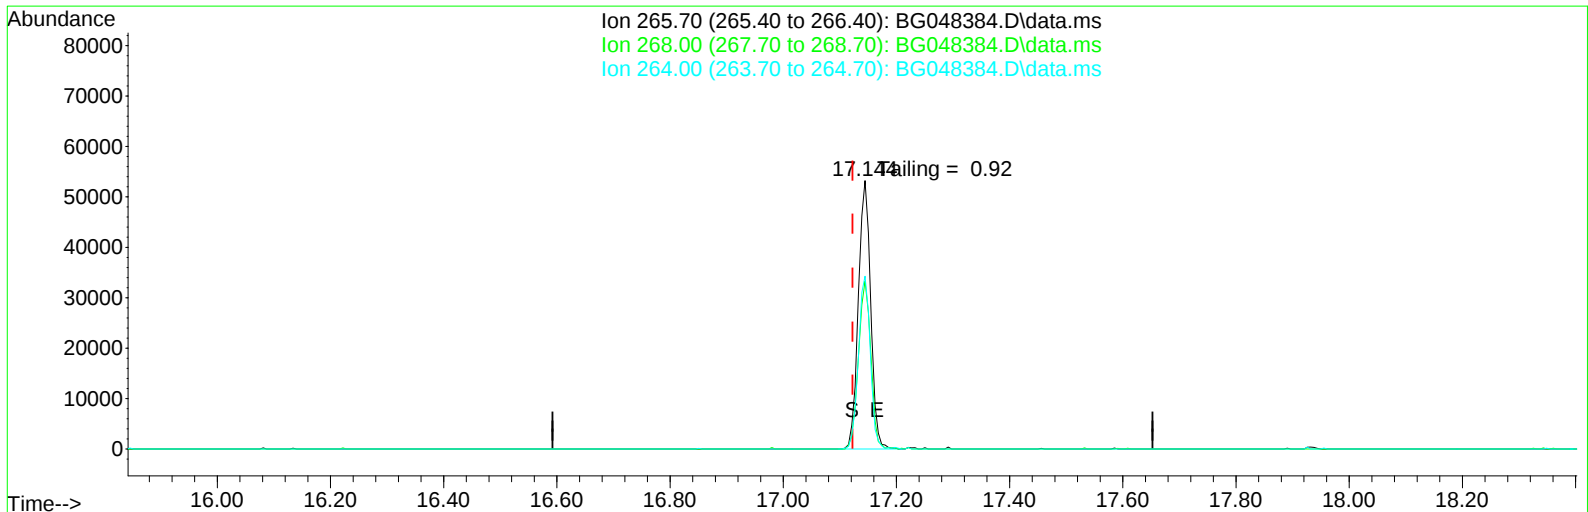

TIC: BG048384.D\data.ms

(70) Pentachlorophenol (C)

17.144min (+ 0.022) 60929.31 ng

response 80557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.57
264.00	61.60	64.41
0.00	0.00	0.00