
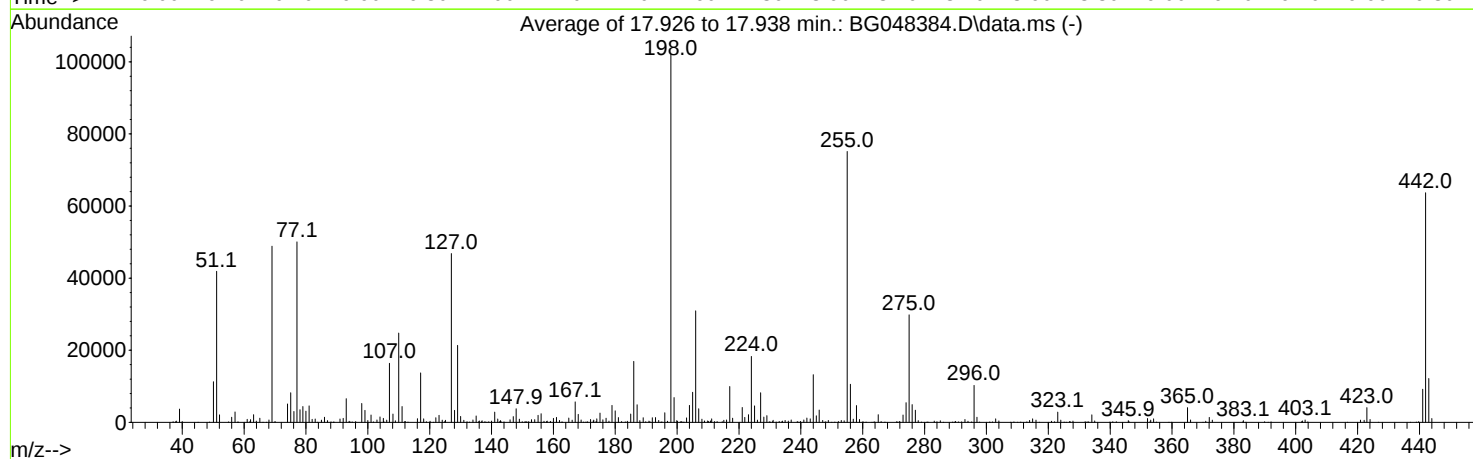


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031621\
 Data File : BG048384.D
 Acq On : 16 Mar 2021 8:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 16 16:05:10 2021

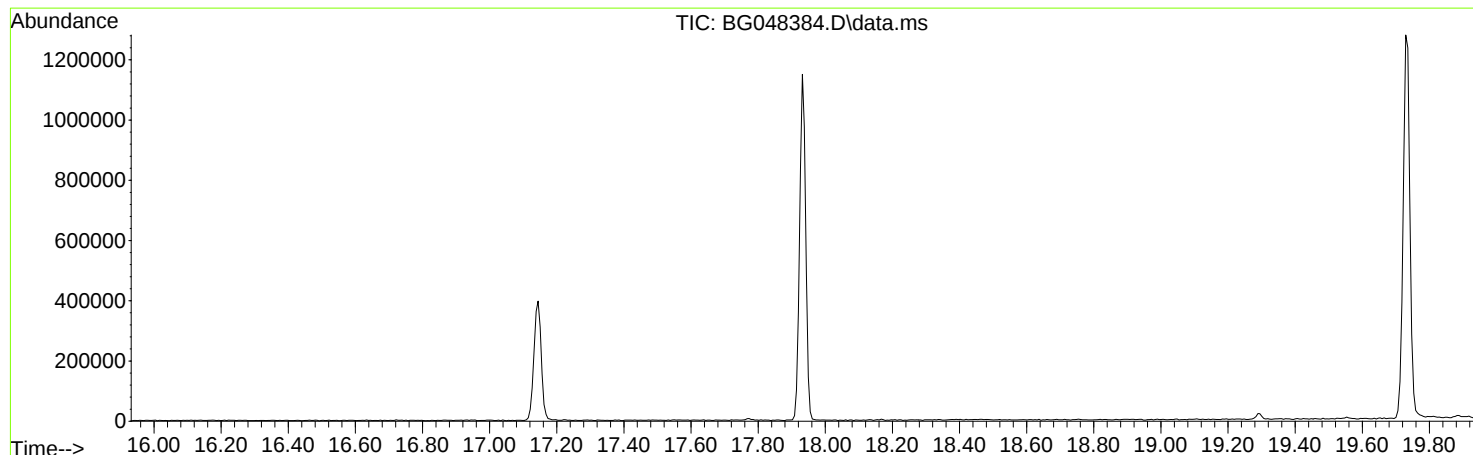

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	41877	PASS
68	69	0.00	2	1.3	658	PASS
69	198	0.00	100	47.9	48875	PASS
70	69	0.00	2	0.6	276	PASS
127	198	10	80	45.9	46837	PASS
197	198	0.00	2	0.3	318	PASS
198	198	100	100	100.0	102024	PASS
199	198	5	9	6.8	6903	PASS
275	198	10	60	29.3	29843	PASS
365	198	1	100	4.0	4070	PASS
441	198	0.01	100	9.0	9192	PASS
442	198	50	100	62.4	63691	PASS
443	442	15	24	19.1	12176	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2021	BNA_G	<u>BG048384.D</u>
Compound Name	Response	Retention Time
DDT	260129	20.96
DDD	714	20.57
DDE	630	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1344	261473	0.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031621\
Data File : BG048384.D
Acq On : 16 Mar 2021 8:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 16 10:55:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 16 10:42:19 2021
Response via : Initial Calibration

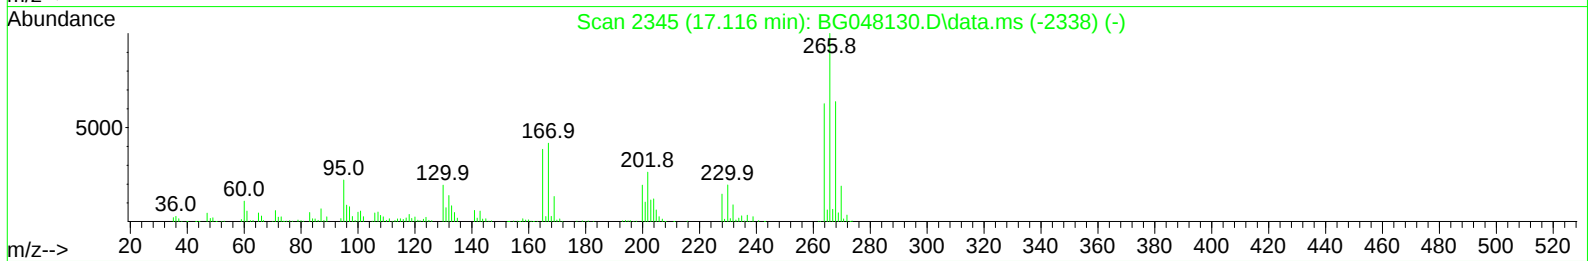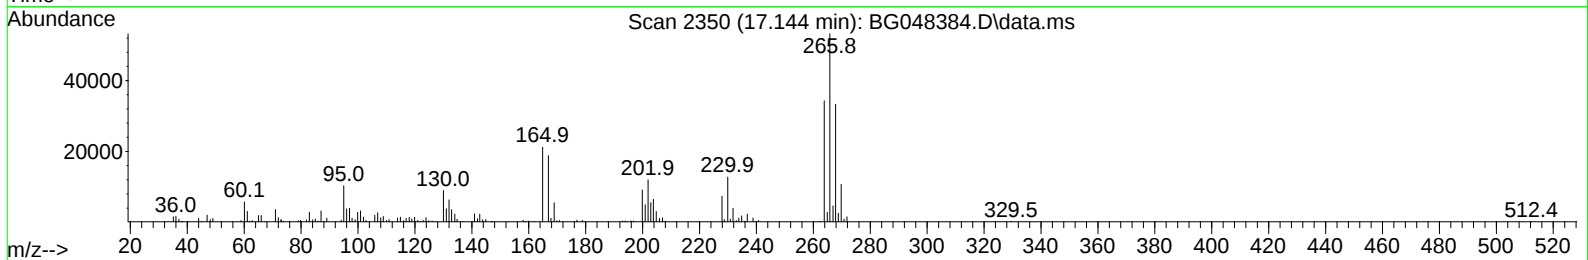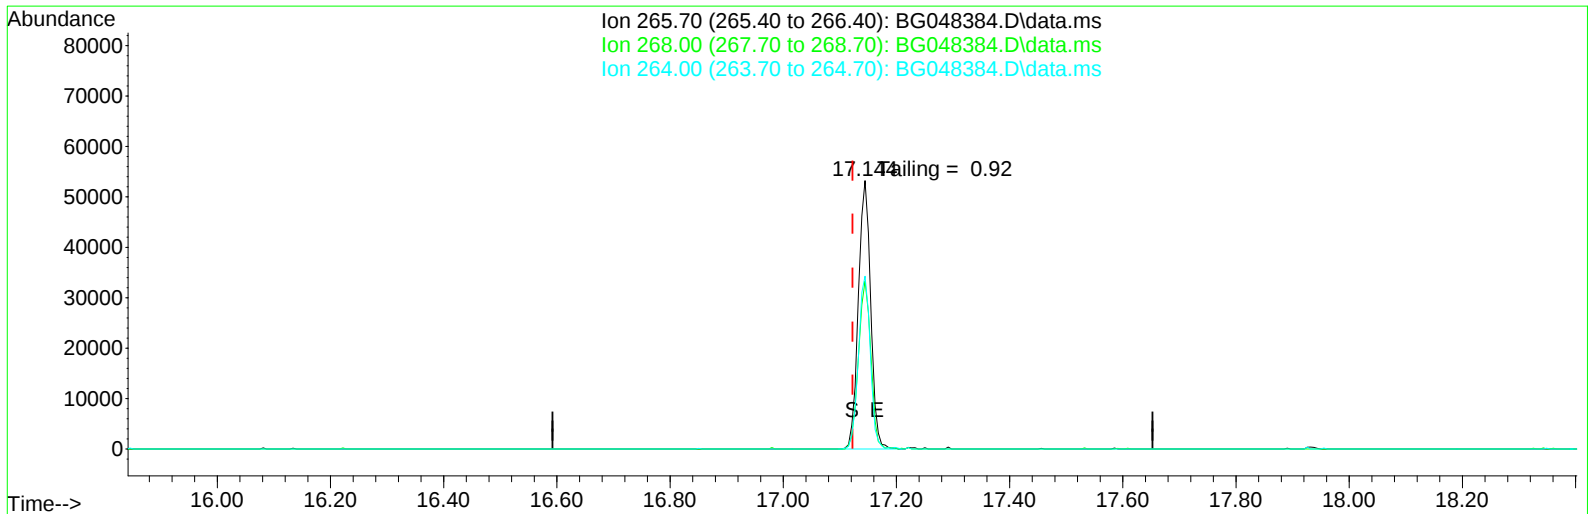

TIC: BG048384.D\data.ms

(70) Pentachlorophenol (C)

17.144min (+ 0.022) 60929.31 ng




response 80557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.57
264.00	61.60	64.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031621\
Data File : BG048384.D
Acq On : 16 Mar 2021 8:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 16 10:55:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 16 10:42:19 2021
Response via : Initial Calibration

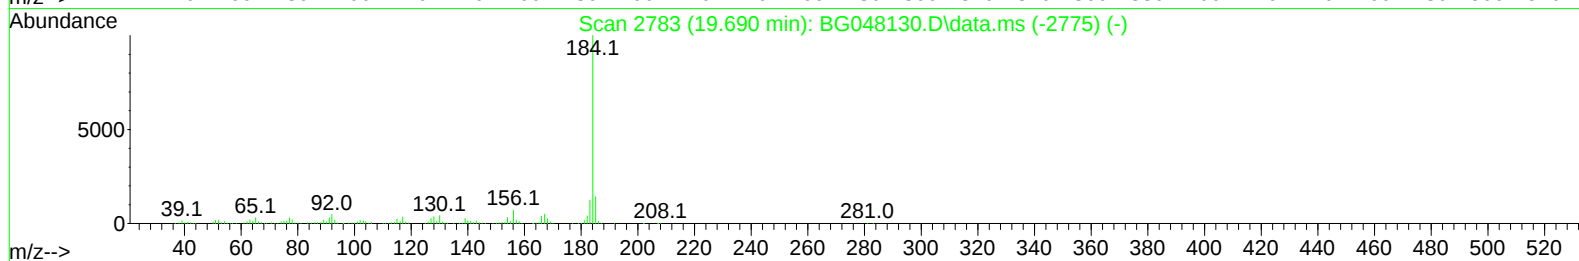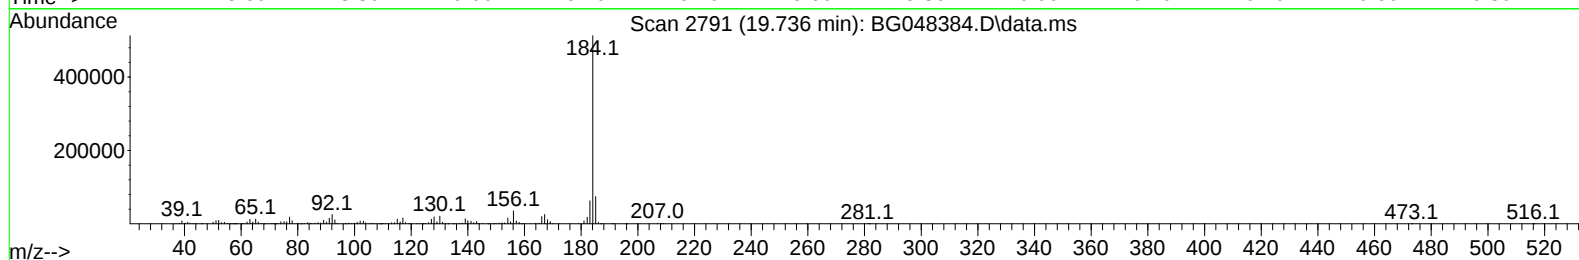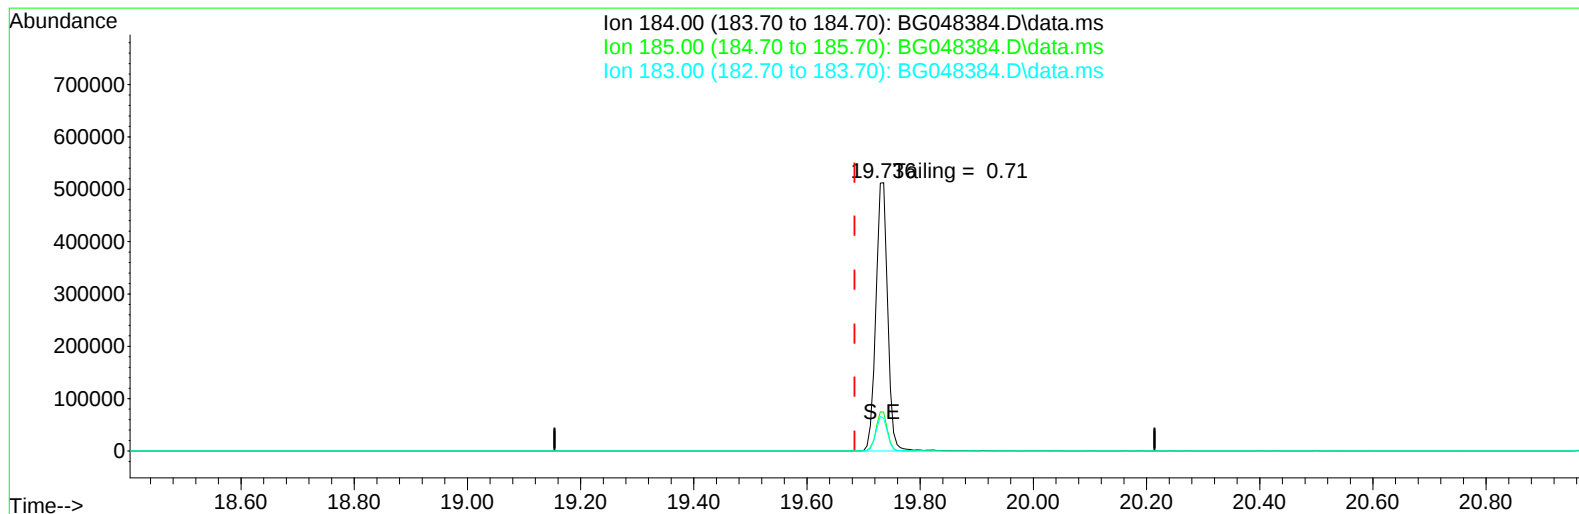

TIC: BG048384.D\data.ms

(77) Benzidine

19.736min (+ 0.052) 342296.28 ng

response 738164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.19
0.00	0.00	0.00