
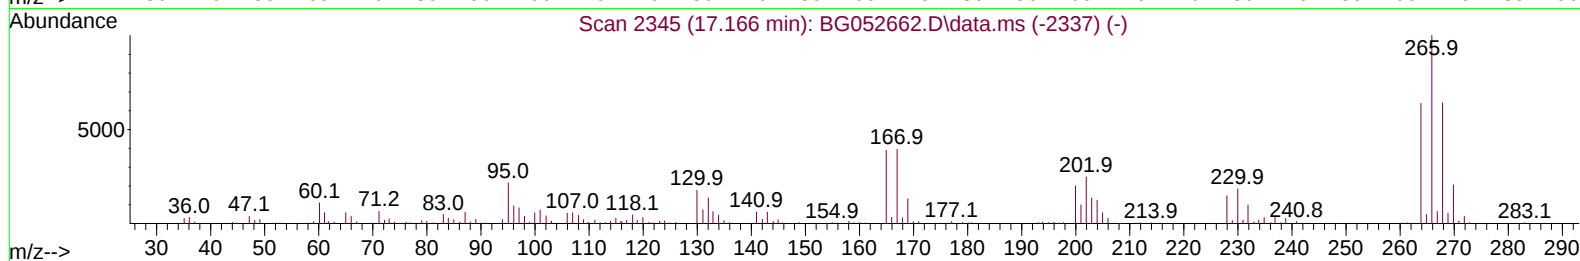
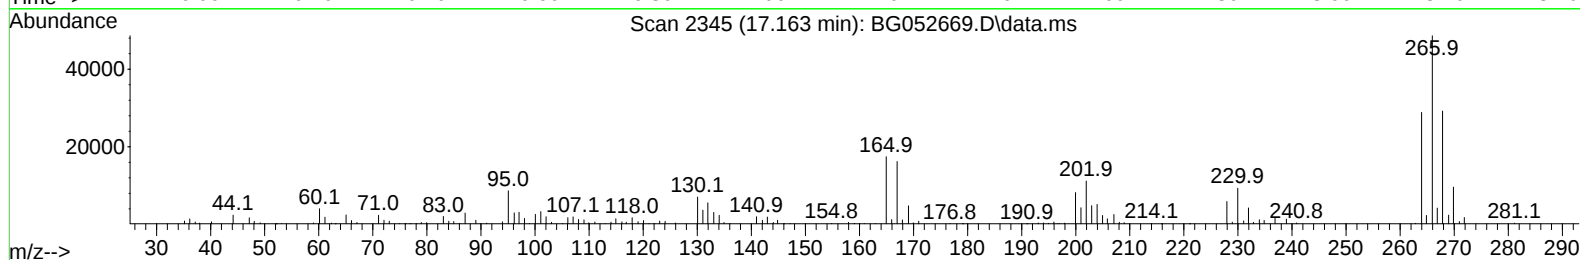


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031622\
 Data File : BG052669.D
 Acq On : 16 Mar 2022 7:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 11:40:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

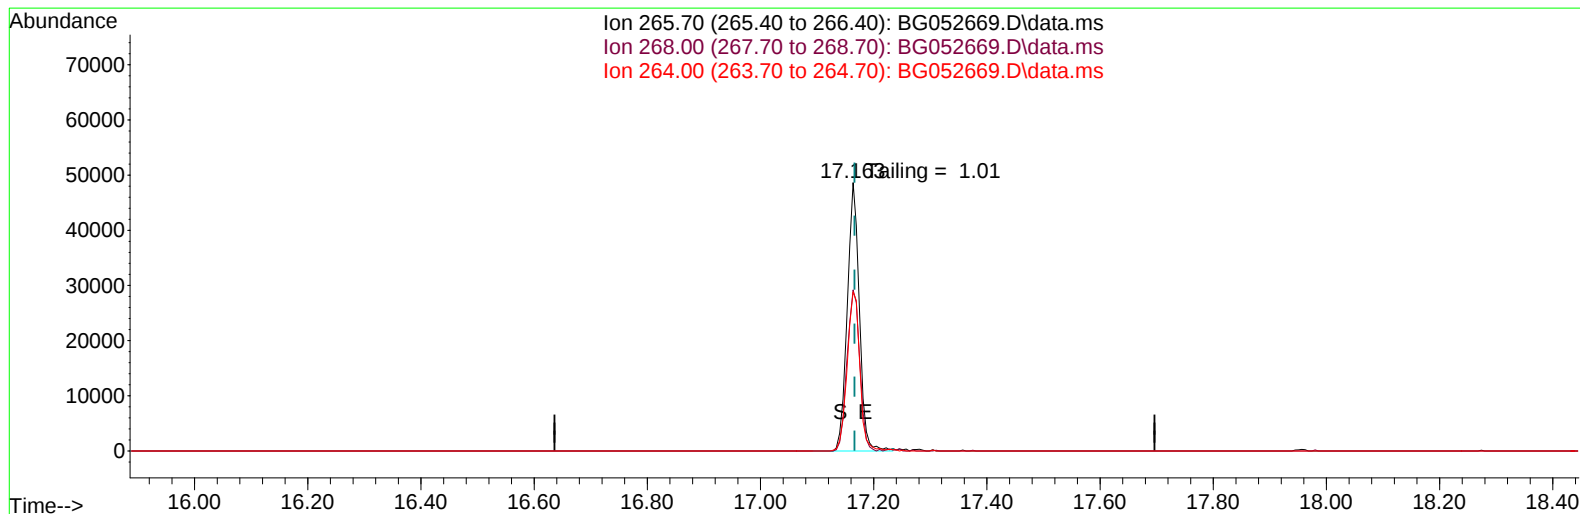

TIC: BG052669.D\data.ms

(70) Pentachlorophenol (C)




17.163min (-0.003) 15189.67 ng

response 72294

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	60.04
264.00	56.60	59.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031622\
 Data File : BG052669.D
 Acq On : 16 Mar 2022 7:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 11:40:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

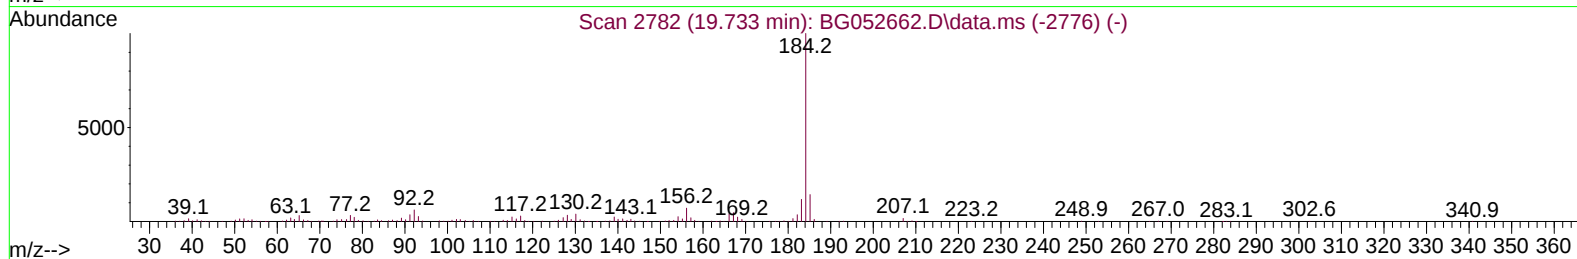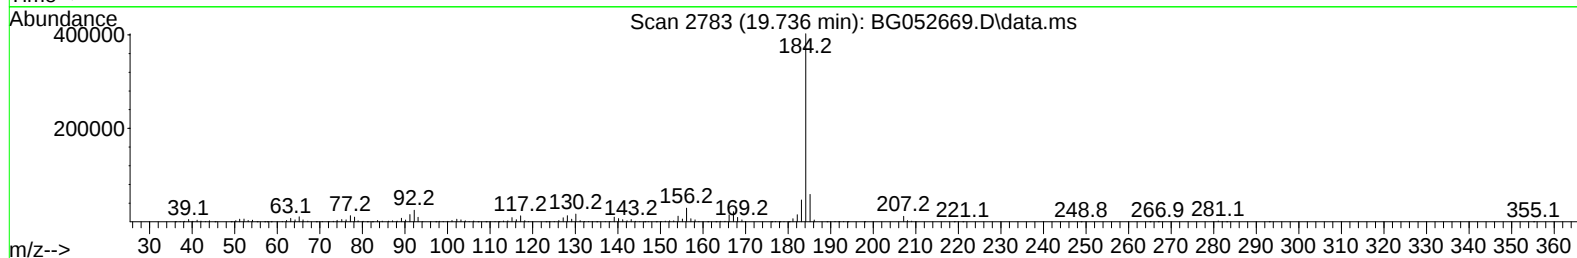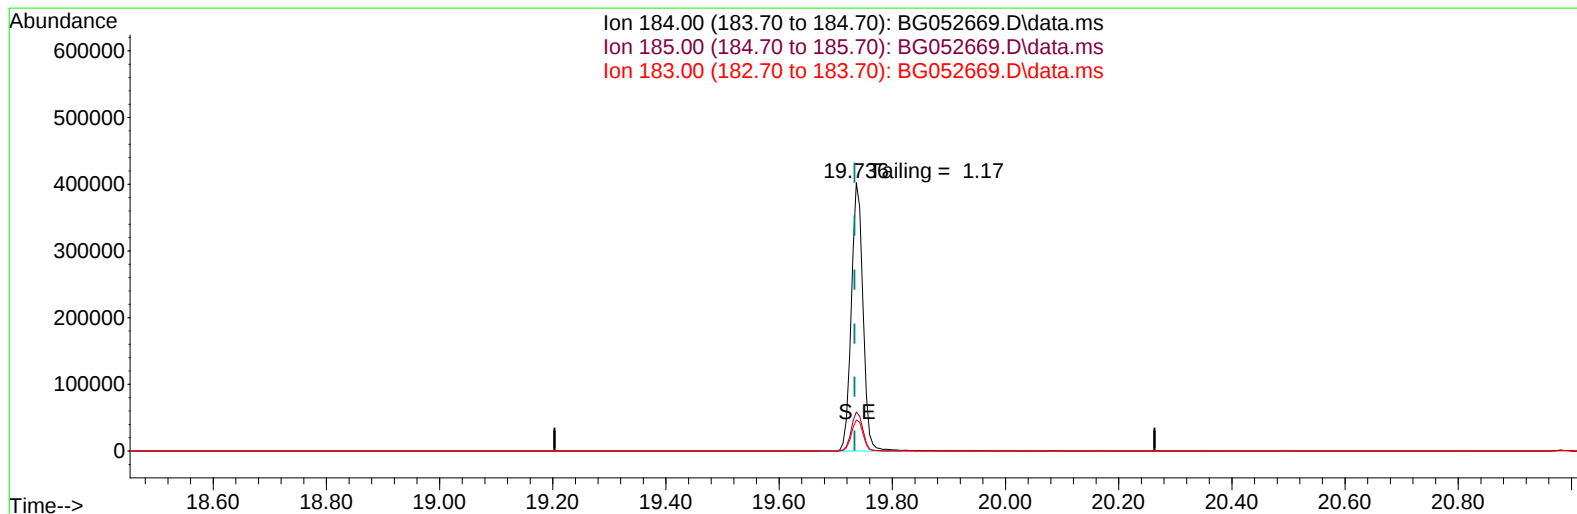

TIC: BG052669.D\data.ms

(77) Benzidine**19.736min (+ 0.003) 399593.66 ng****response 577154**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.59
183.00	11.80	11.59
0.00	0.00	0.00