

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031622\
 Data File : BG052671.D
 Acq On : 16 Mar 2022 9:05
 Operator : CG/JU
 Sample : PB143161BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143161BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.709	387	395	407	rBV	757346	1204032	32.80%	9.158%
2	7.301	658	666	680	rBV	739830	1303544	35.51%	9.915%
3	8.152	805	811	819	rVB	137101	236426	6.44%	1.798%
4	9.310	999	1008	1021	rBV	428624	788291	21.47%	5.996%
5	10.966	1283	1290	1298	rVB	178605	325120	8.86%	2.473%
6	13.404	1697	1705	1712	rBV	1199196	1888906	51.46%	14.368%
7	14.773	1931	1938	1948	rBV	287946	452432	12.33%	3.441%
8	16.253	2181	2190	2200	rBV	804119	1226101	33.40%	9.326%
9	17.516	2398	2405	2416	rBV	381201	580052	15.80%	4.412%
10	20.119	2842	2848	2854	rVB	2707280	3670757	100.00%	27.921%
11	21.805	3129	3135	3141	rVB	467850	761150	20.74%	5.790%
12	25.129	3691	3701	3711	rVB2	243129	710082	19.34%	5.401%




Sum of corrected areas: 13146893

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031622\
Data File : BG052671.D
Acq On : 16 Mar 2022 9:05
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

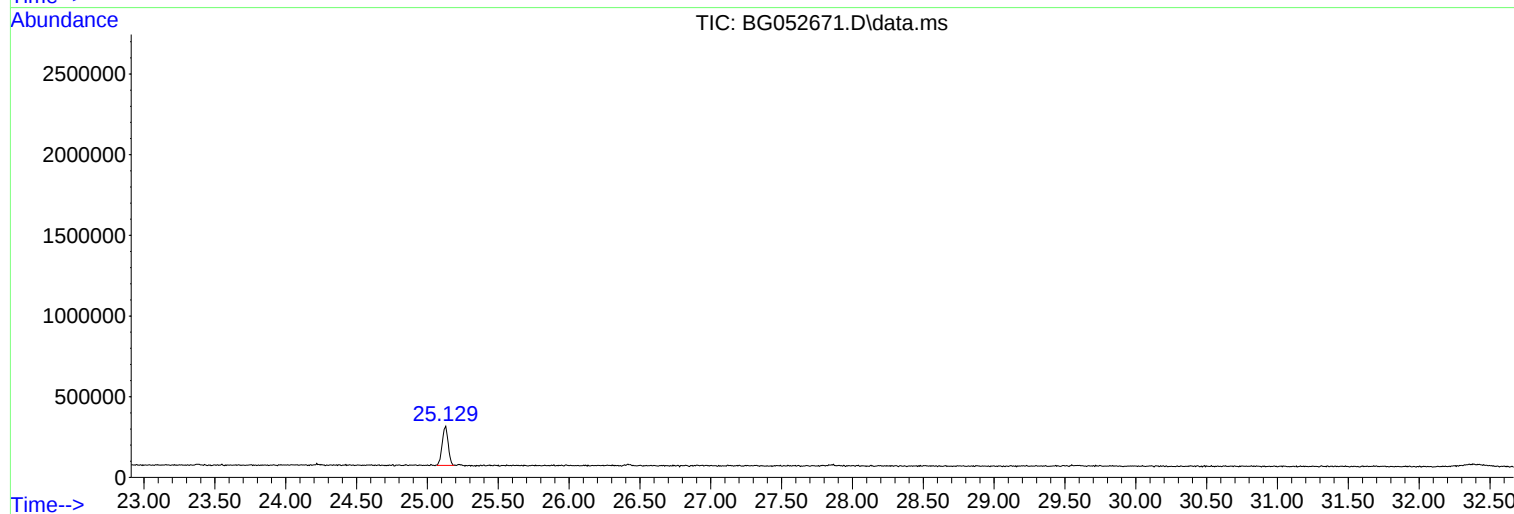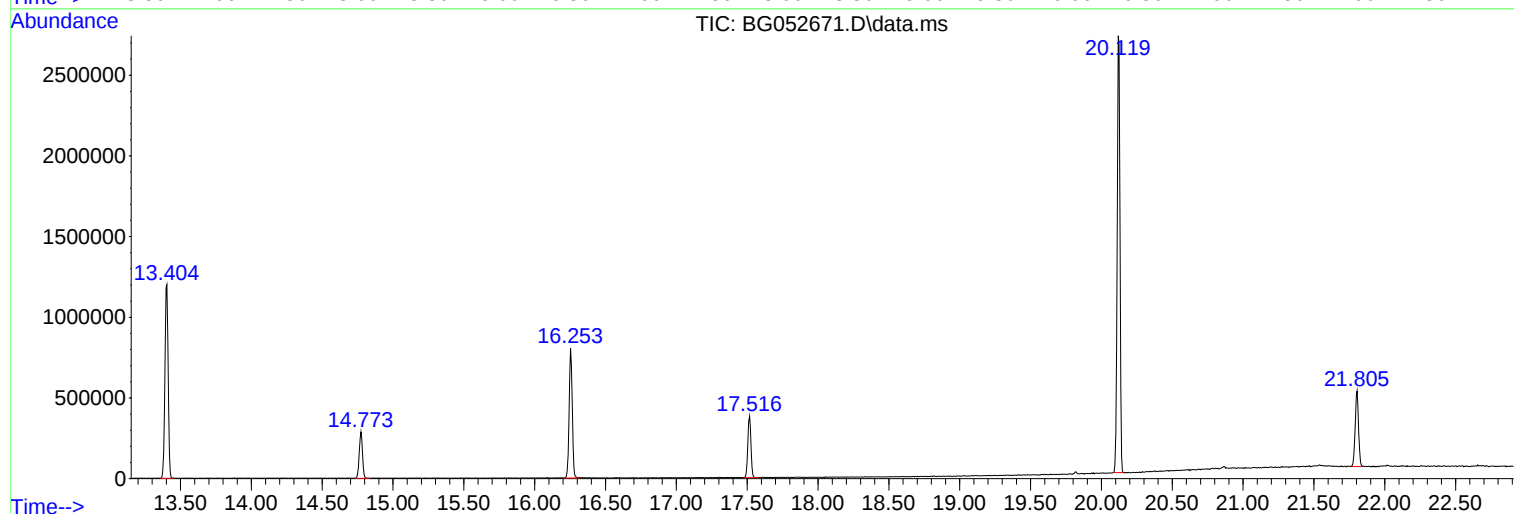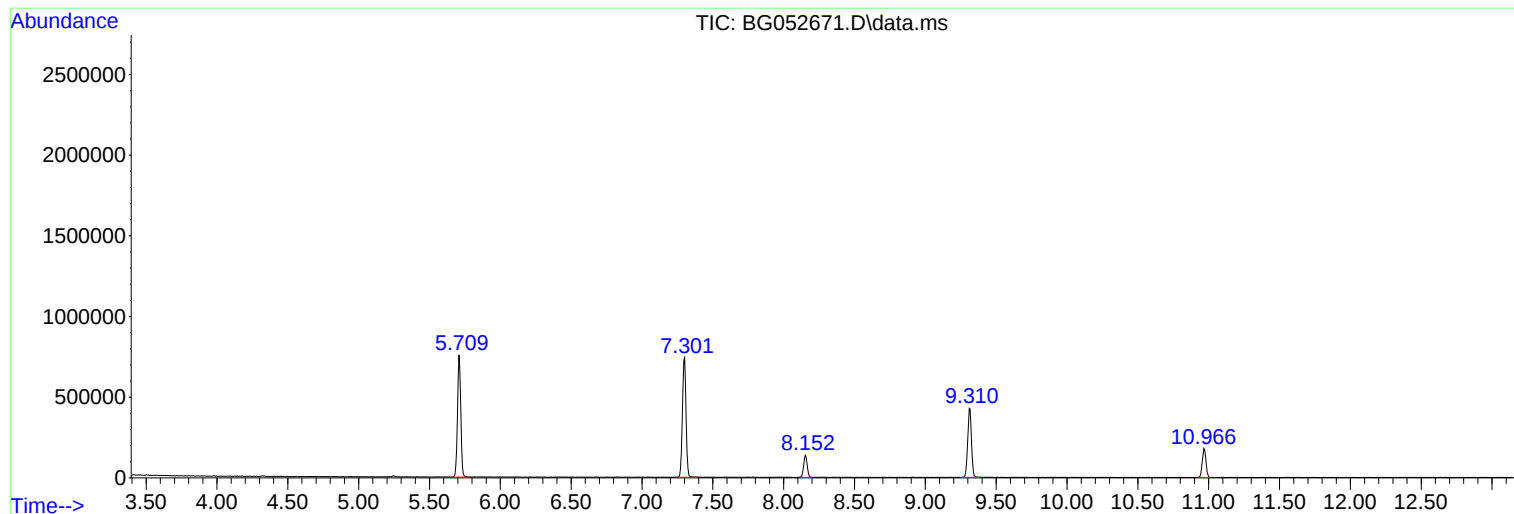

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031622\
Data File : BG052671.D
Acq On : 16 Mar 2022 9:05
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031622\
Data File : BG052671.D
Acq On : 16 Mar 2022 9:05
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------