
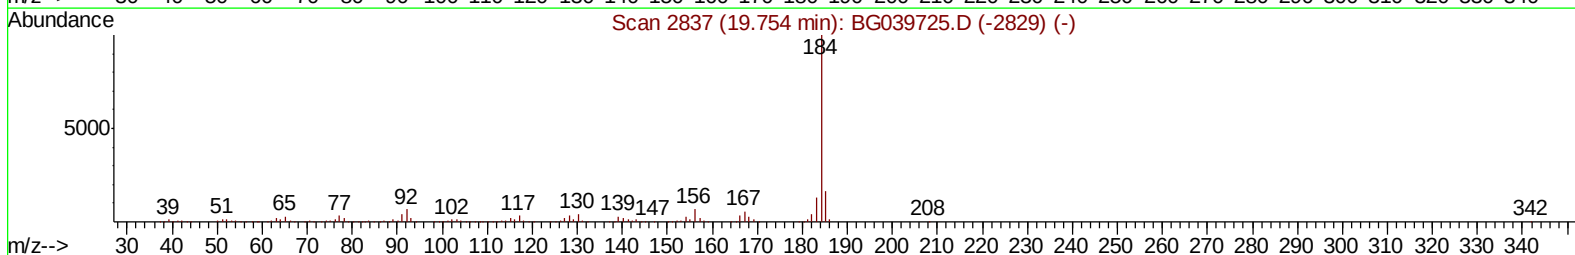
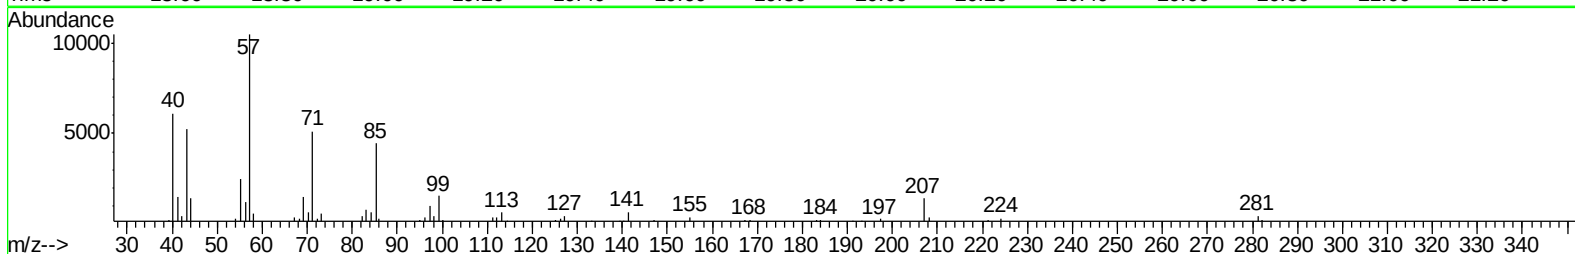


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031819\
 Data File : BG039972.D
 Acq On : 18 Mar 2019 16:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:21:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

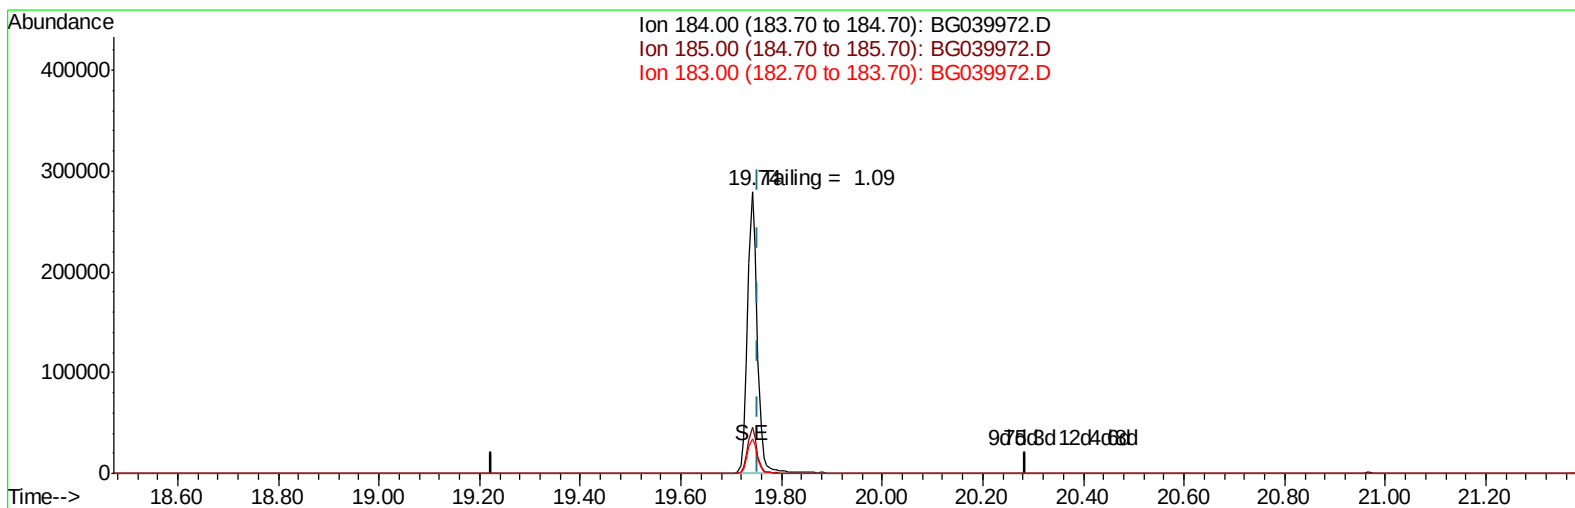

TIC: BG039972.D

(77) Benzidine




20.364min (+0.610) 167.69ng

response 298

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	0.00#
183.00	13.20	91.24#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031819\
Data File : BG039972.D
Acq On : 18 Mar 2019 16:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:21:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

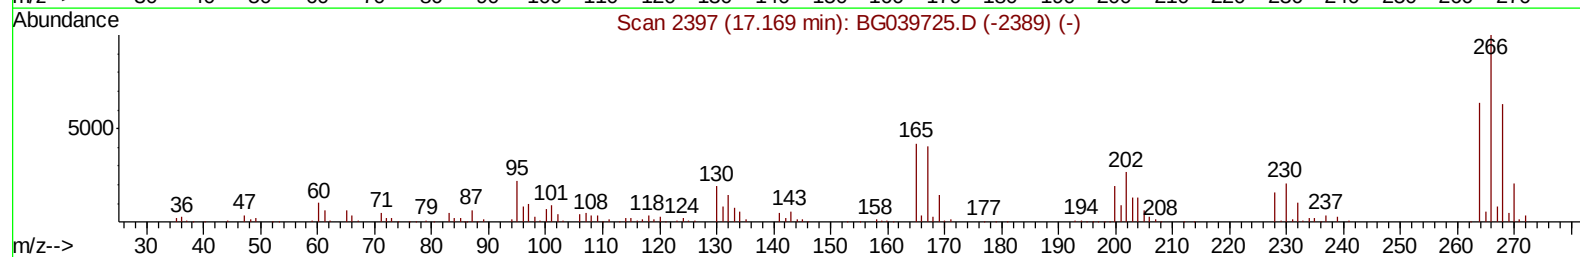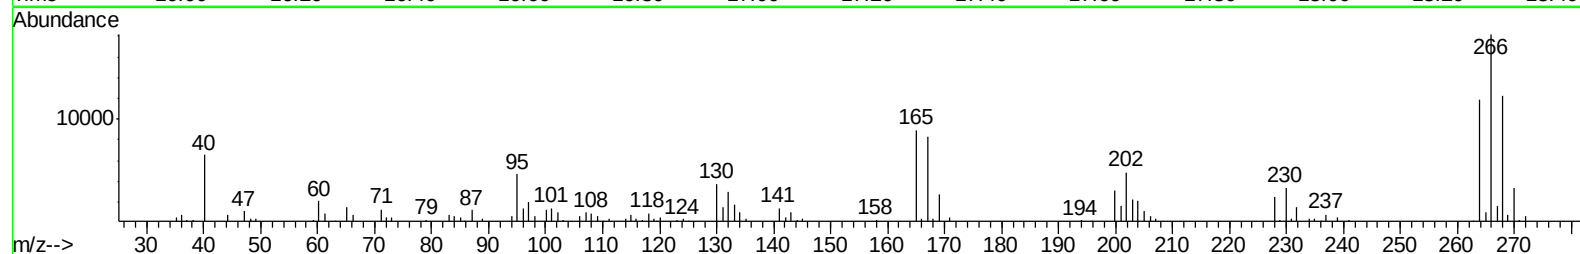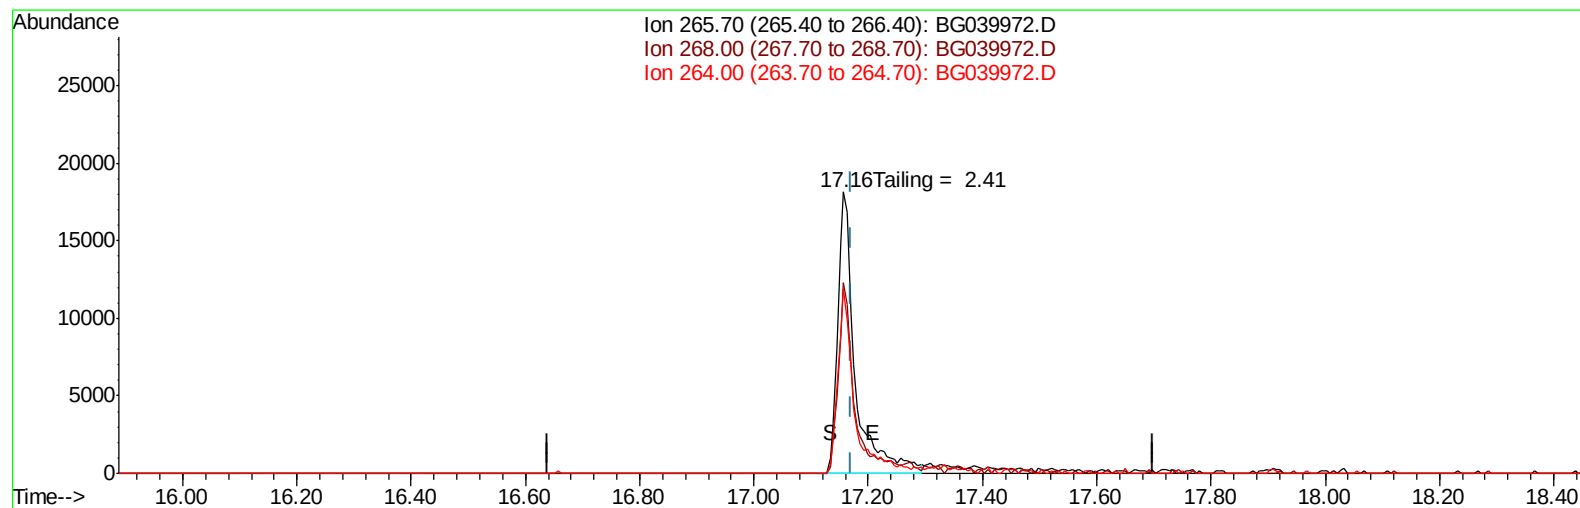

TIC: BG039972.D

(70) Pentachlorophenol (C)

17.157min (-0.013) 19923.36ng

response 36644

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.63
264.00	65.10	65.58
0.00	0.00	0.00