


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031819\
 Data File : BG039990.D
 Acq On : 19 Mar 2019 4:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

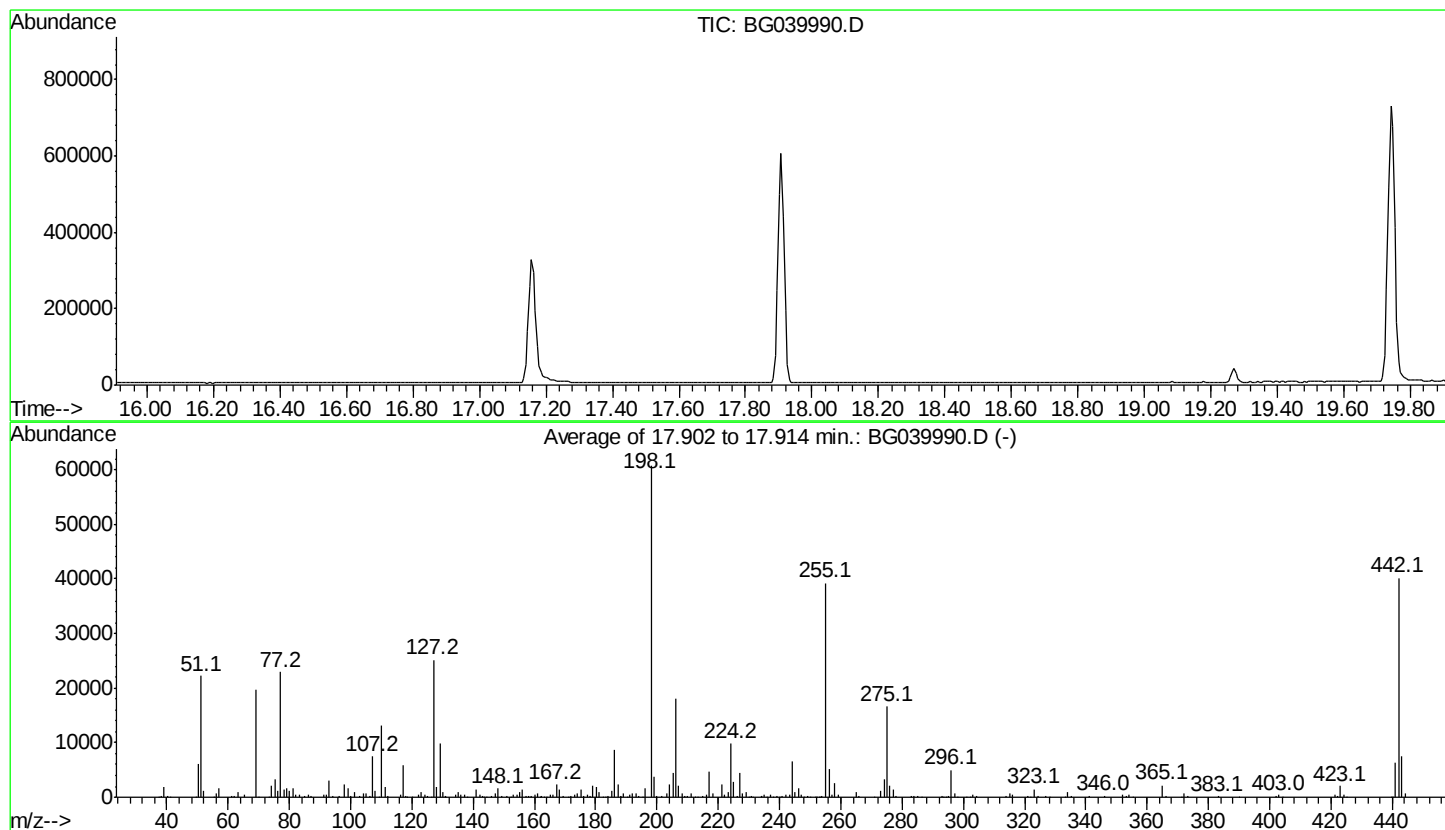

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	22231	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.3	19625	PASS
70	69	0.00	2	0.3	63	PASS
127	198	10	80	41.4	25146	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60757	PASS
199	198	5	9	6.3	3846	PASS
275	198	10	60	27.3	16563	PASS
365	198	1	100	3.6	2170	PASS
441	198	0.01	100	10.5	6404	PASS
442	198	50	100	66.0	40122	PASS
443	442	15	24	18.7	7486	PASS