
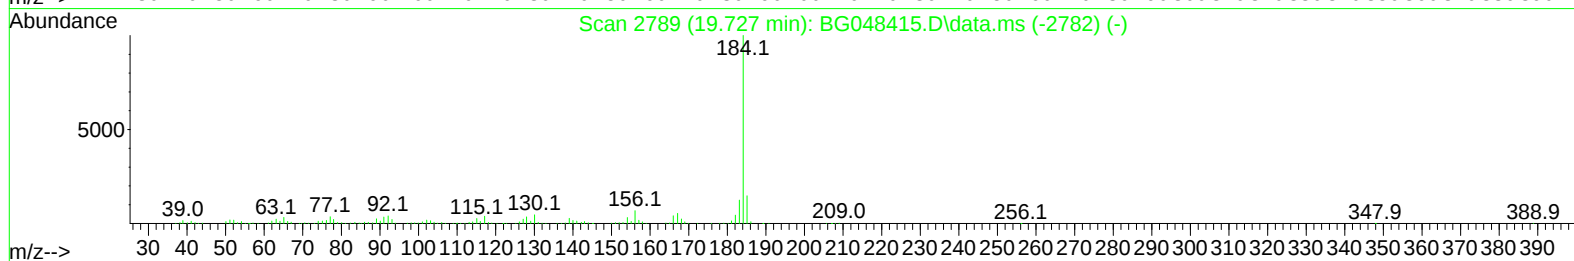
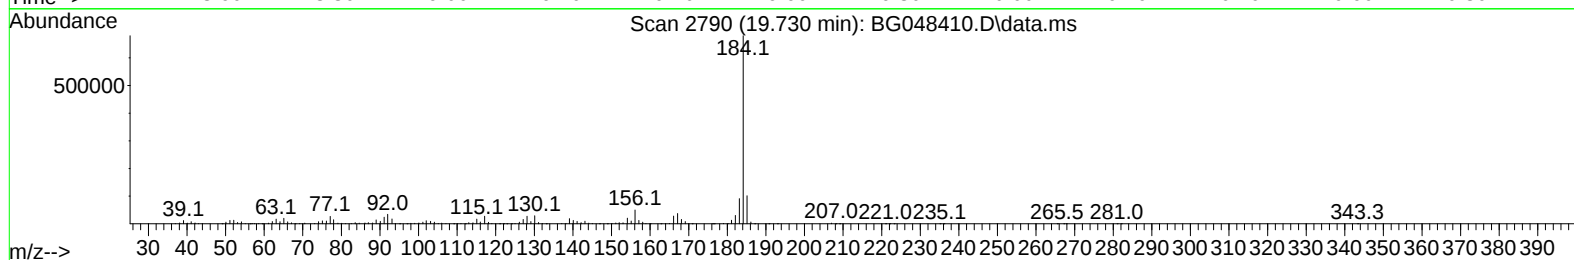


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031821\
 Data File : BG048410.D
 Acq On : 18 Mar 2021 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 16:41:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 18 16:38:55 2021
 Response via : Initial Calibration

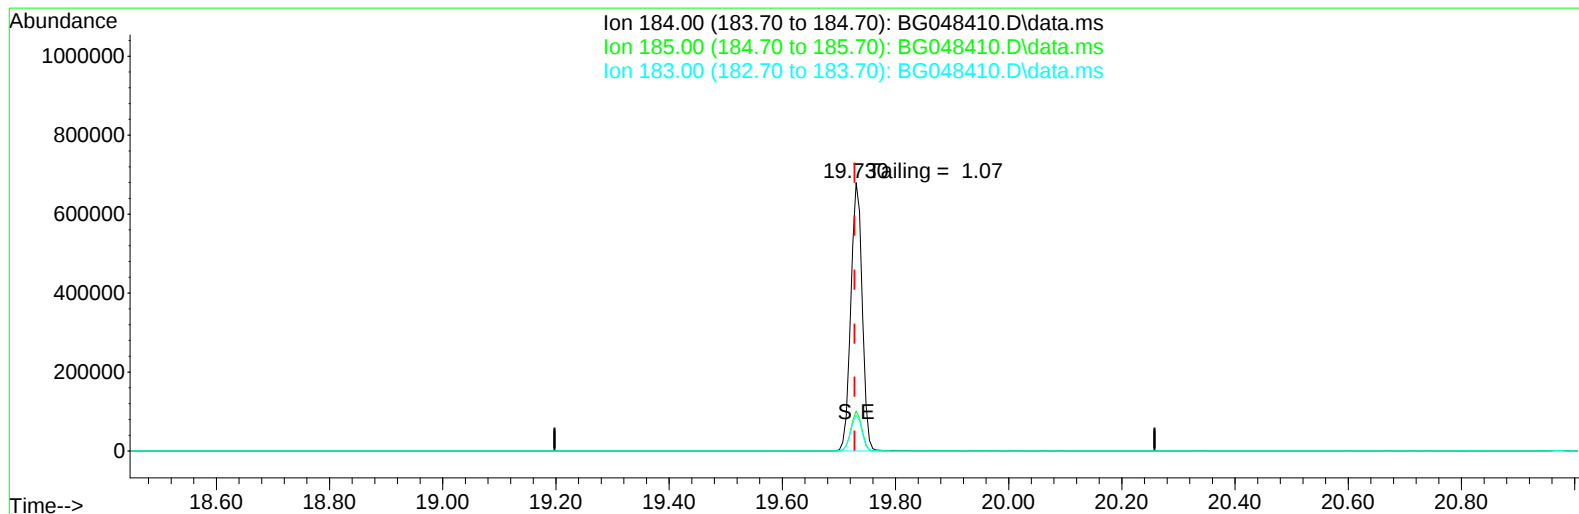




TIC: BG048410.D\data.ms

(77) Benzidine**19.730min (+ 0.003) 454028.63 ng****response 952024**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	13.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031821\
Data File : BG048410.D
Acq On : 18 Mar 2021 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 16:41:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

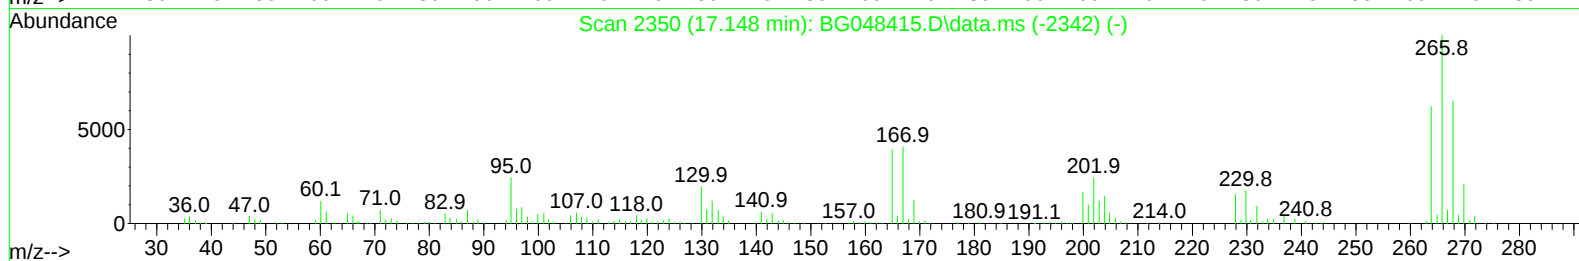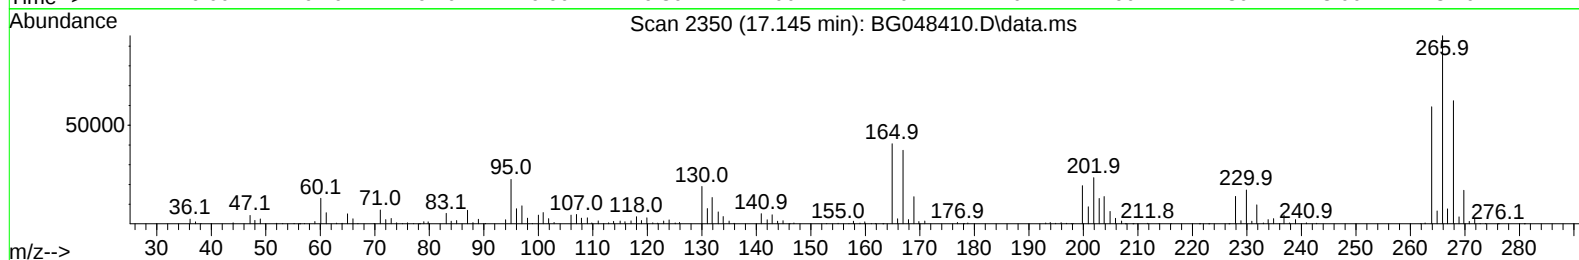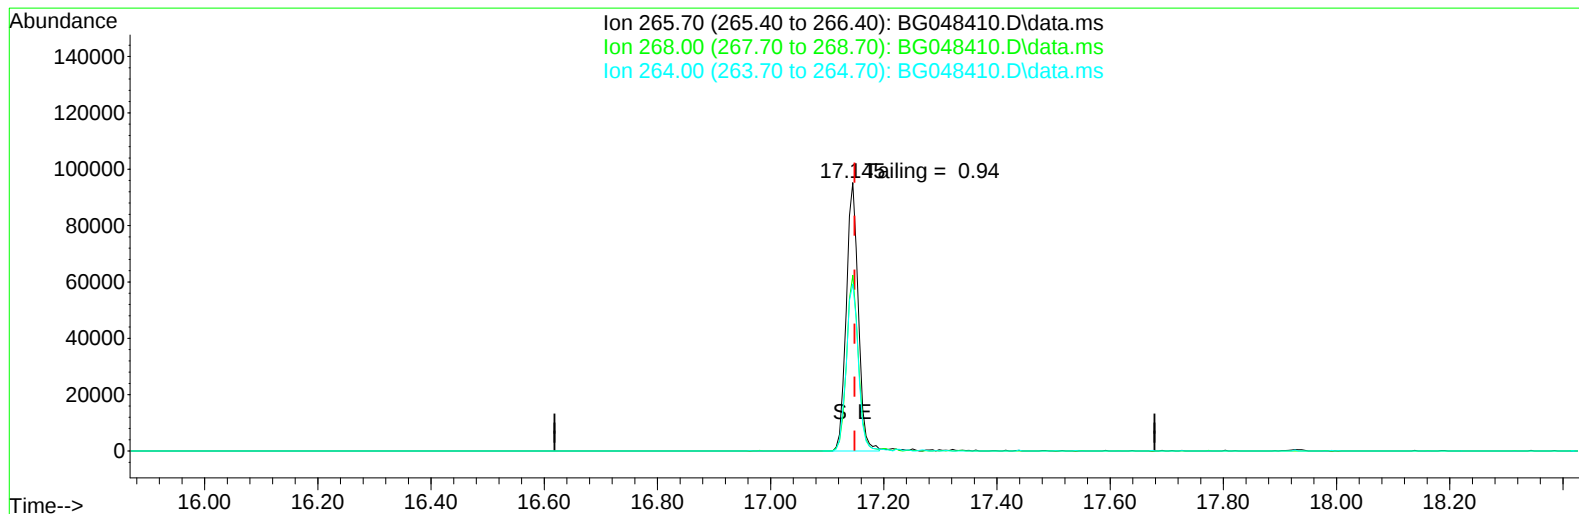

TIC: BG048410.D\data.ms

(70) Pentachlorophenol (C)

17.145min (-0.003) 280394.09 ng

response 140868

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.48
264.00	61.60	62.27
0.00	0.00	0.00