
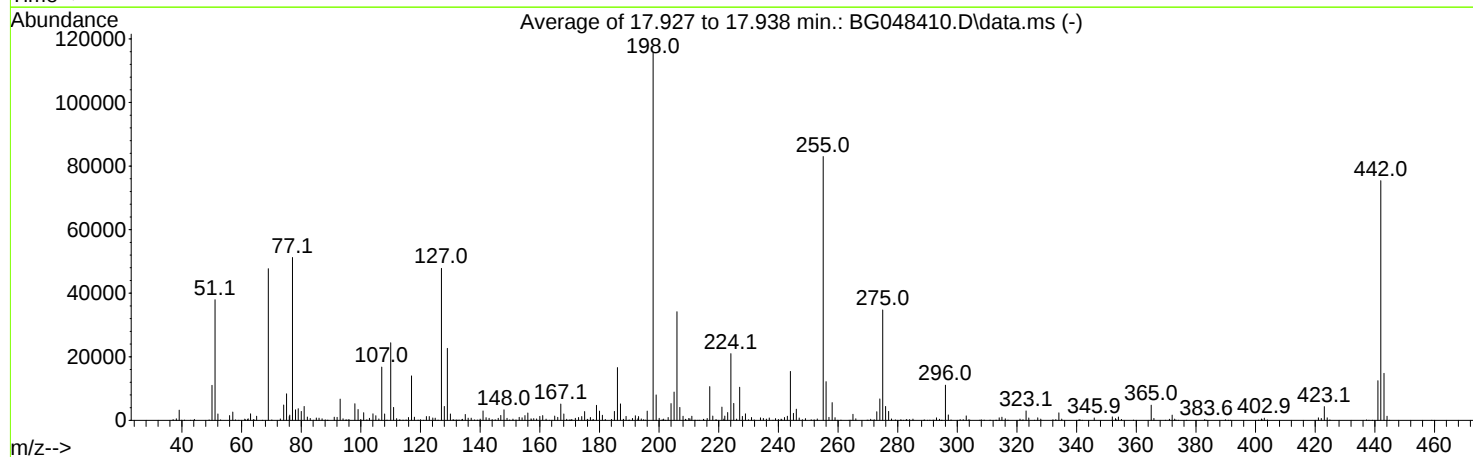


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031821\
 Data File : BG048410.D
 Acq On : 18 Mar 2021 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 18 16:38:55 2021

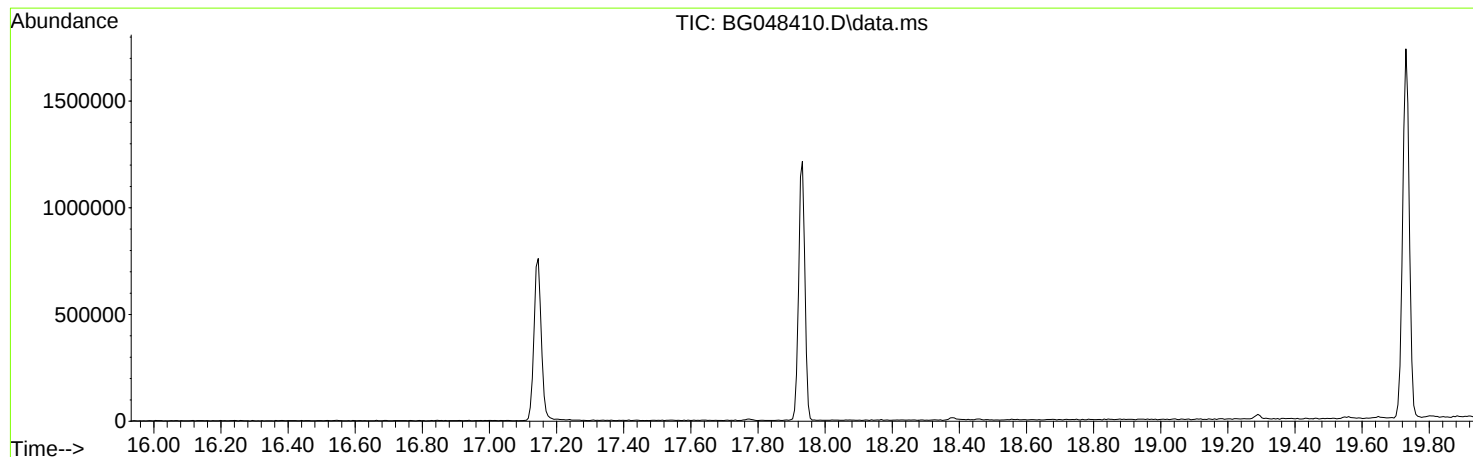

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	37941	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.2	47715	PASS
70	69	0.00	2	0.3	163	PASS
127	198	10	80	41.3	47835	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115731	PASS
199	198	5	9	6.9	8015	PASS
275	198	10	60	30.0	34747	PASS
365	198	1	100	4.1	4798	PASS
441	198	0.01	100	10.8	12486	PASS
442	198	50	100	65.2	75405	PASS
443	442	15	24	19.7	14827	PASS

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2021	BNA_G	<u>BG048410.D</u>
Compound Name	Response	Retention Time
DDT	442517	20.97
DDD	2959	20.52
DDE	788	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3747	446264	0.84

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031821\
 Data File : BG048410.D
 Acq On : 18 Mar 2021 10:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 18 16:41:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 18 16:38:55 2021
 Response via : Initial Calibration

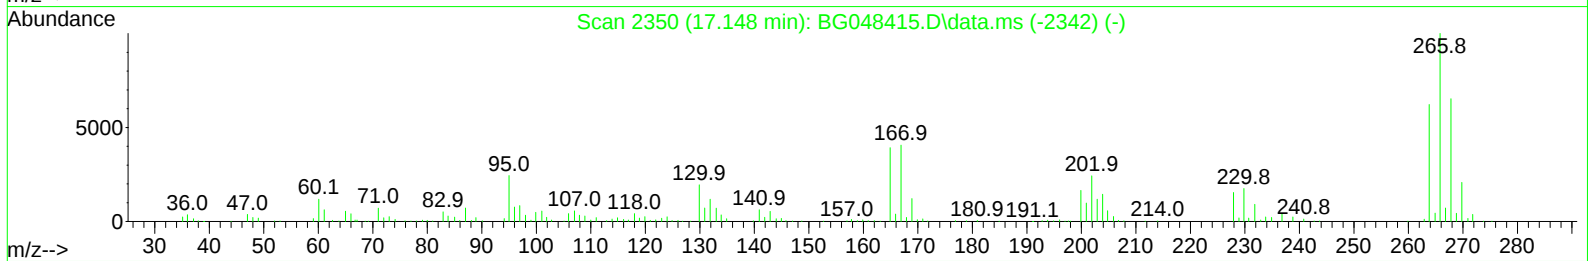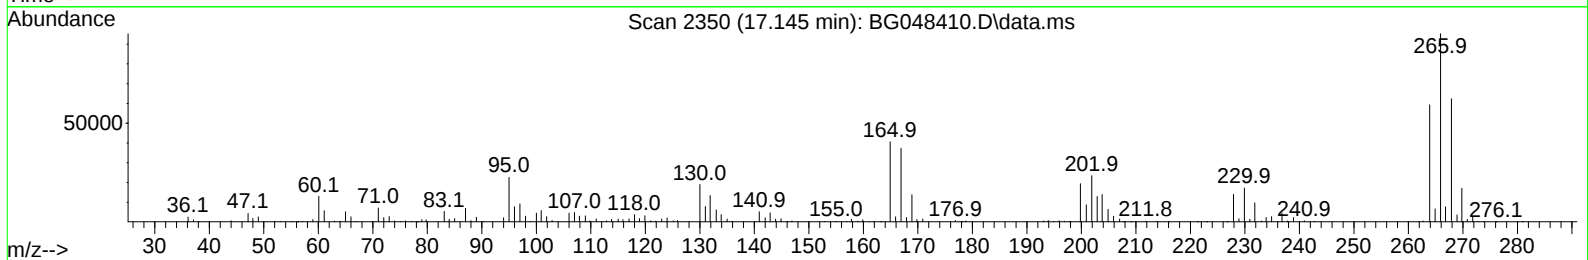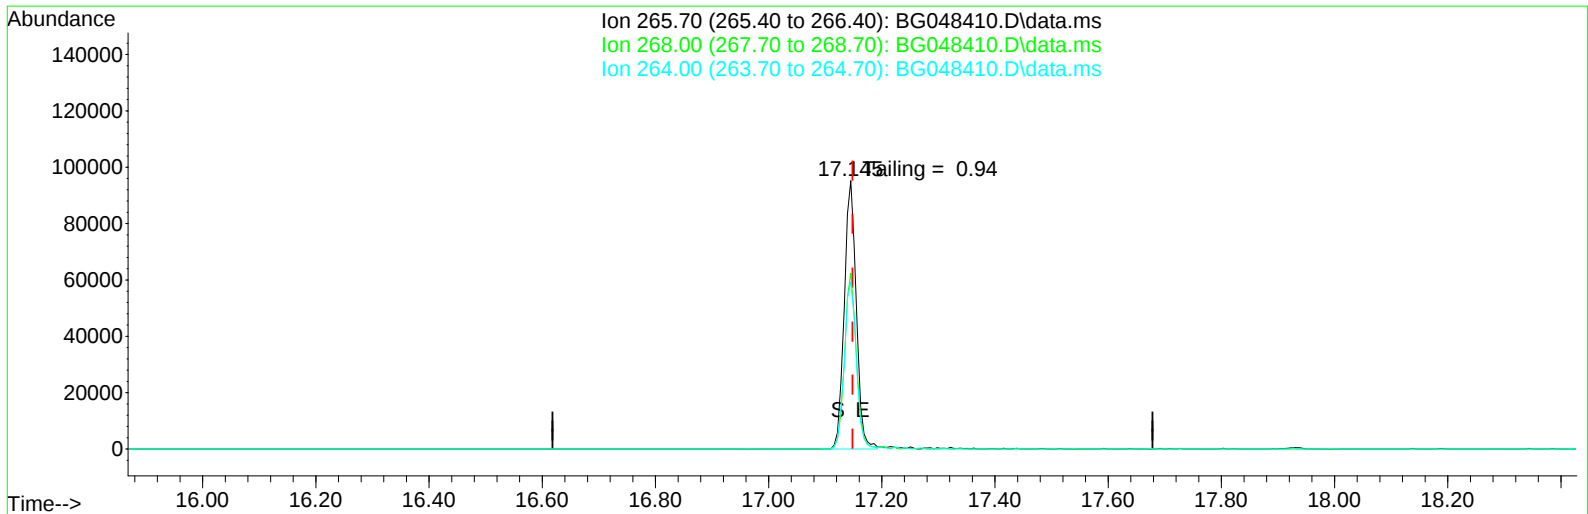

TIC: BG048410.D\data.ms

(70) Pentachlorophenol (C)

17.145min (-0.003) 280394.09 ng




response 140868

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.48
264.00	61.60	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031821\
Data File : BG048410.D
Acq On : 18 Mar 2021 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 18 16:41:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

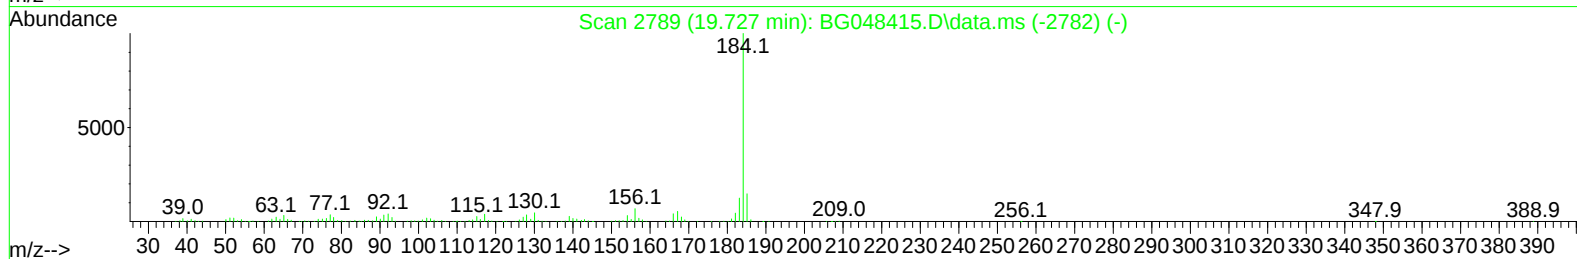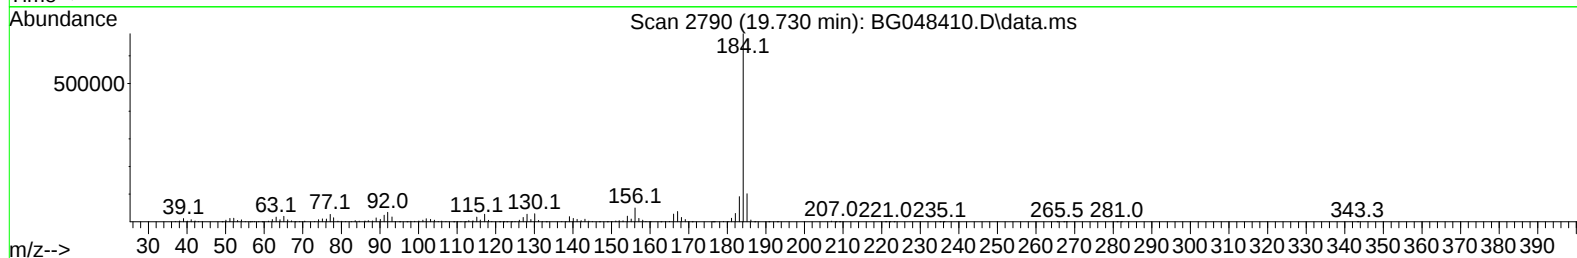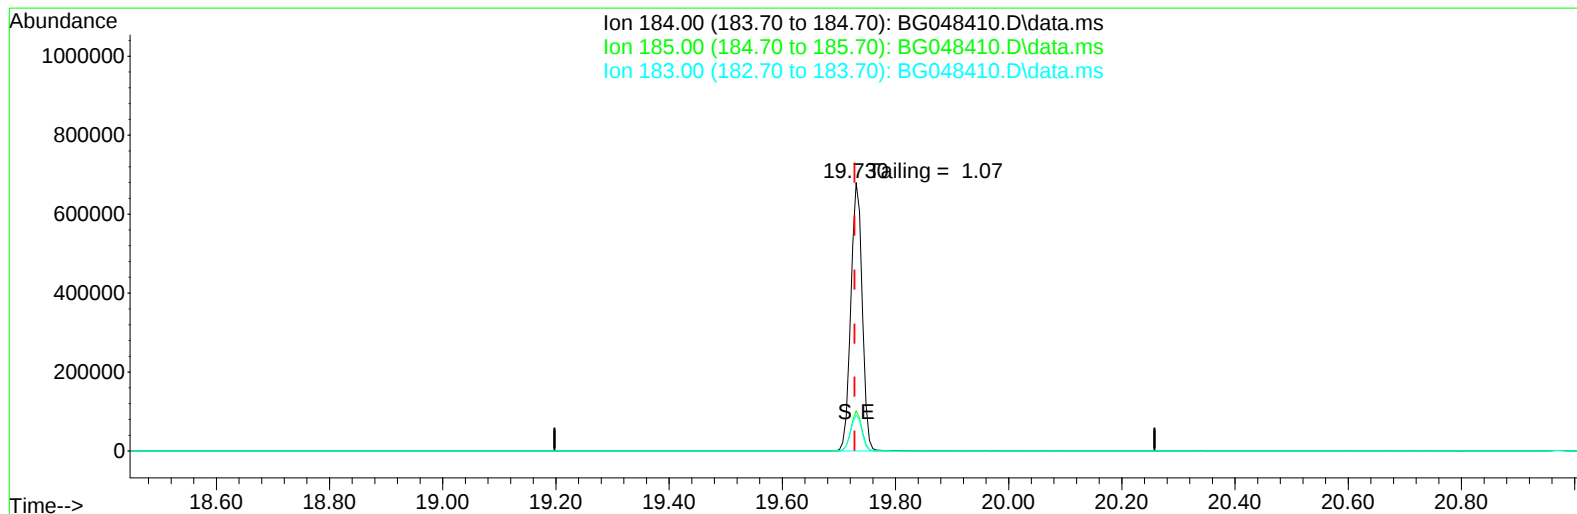

TIC: BG048410.D\data.ms

(77) Benzidine

19.730min (+ 0.003) 454028.63 ng

response 952024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	13.36
0.00	0.00	0.00