
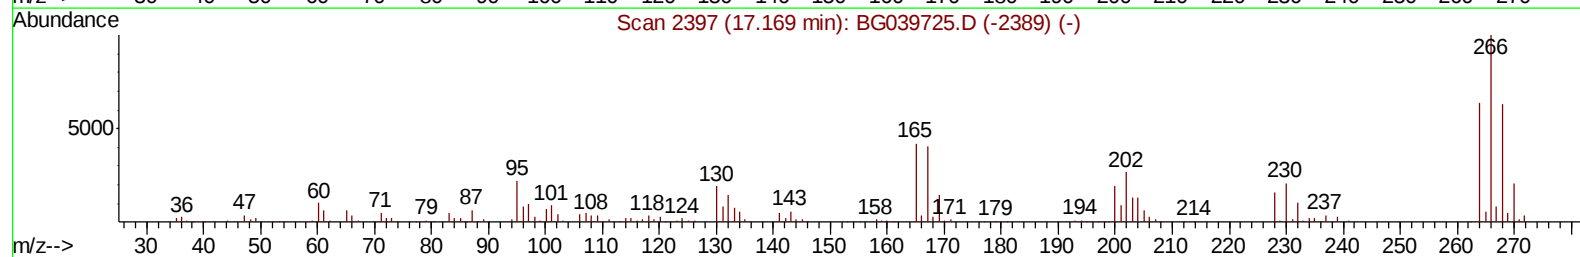
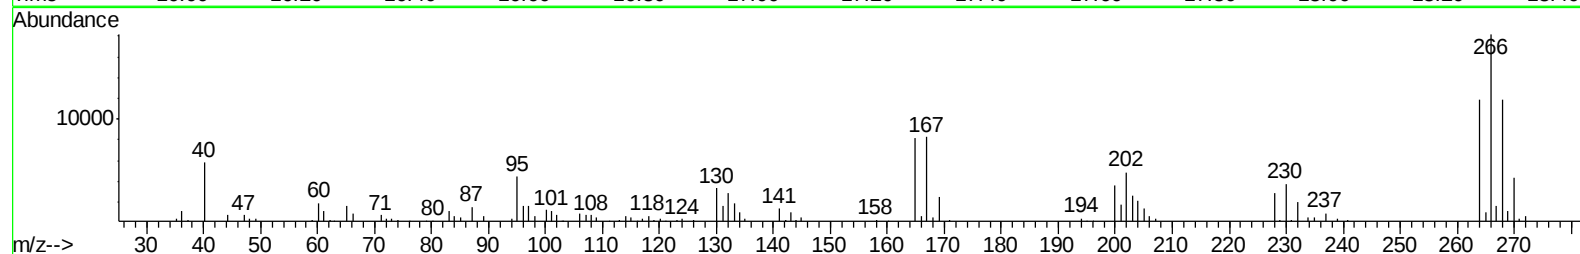


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG031919\  
Data File : BG040001.D  
Acq On : 19 Mar 2019 13:23  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 09:04:52 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 14:38:15 2019  
Response via : Initial Calibration

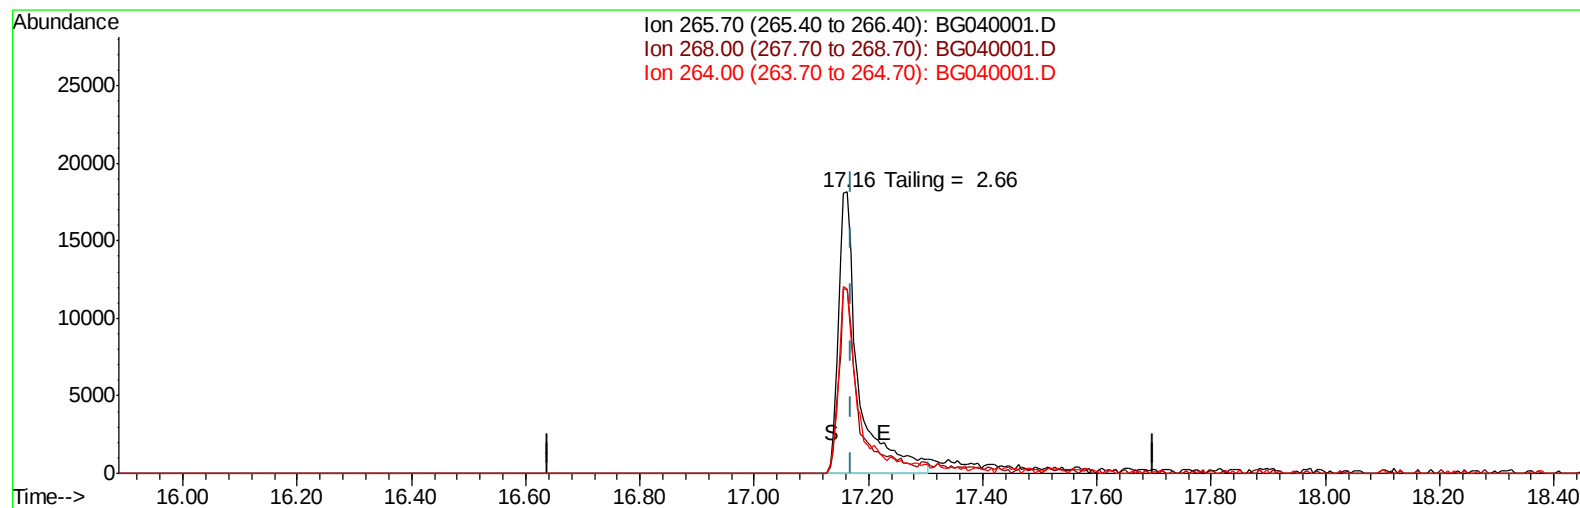

TIC: BG040001.D

(70) Pentachlorophenol (C)




17.162min (-0.008) 9371.22ng

response 43399

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 65.31 |
| 264.00 | 65.10 | 65.56 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG031919\  
Data File : BG040001.D  
Acq On : 19 Mar 2019 13:23  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 09:04:52 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 14:38:15 2019  
Response via : Initial Calibration

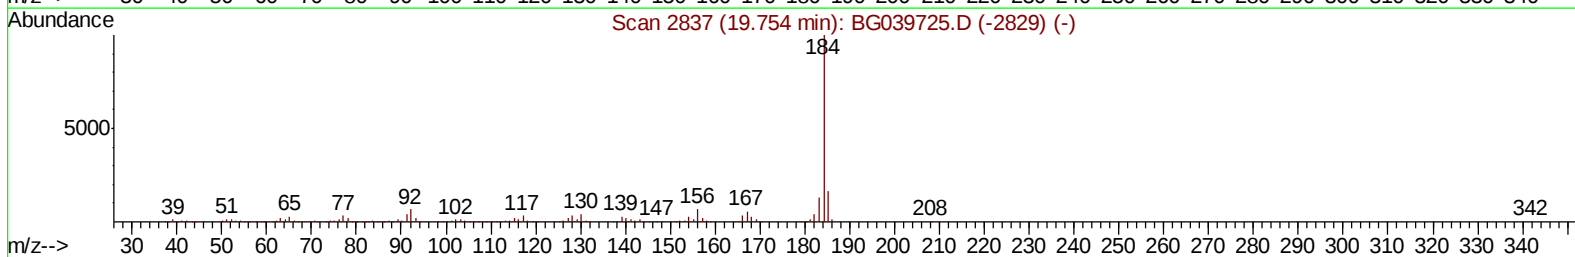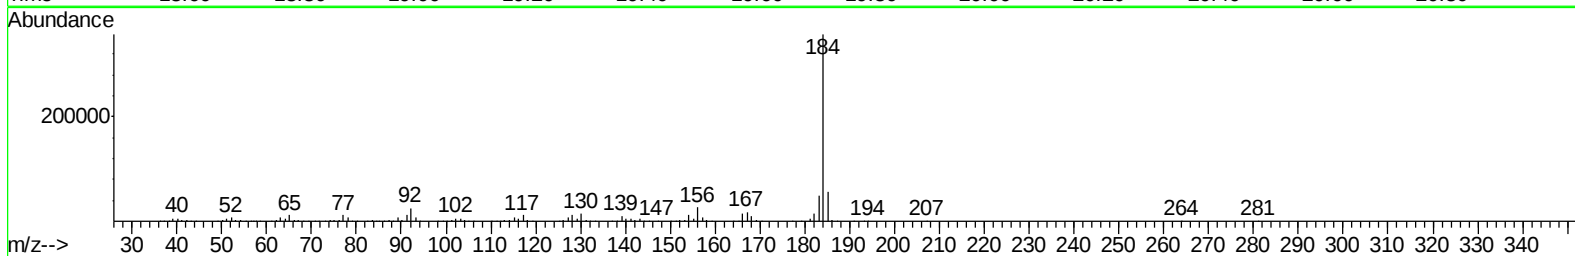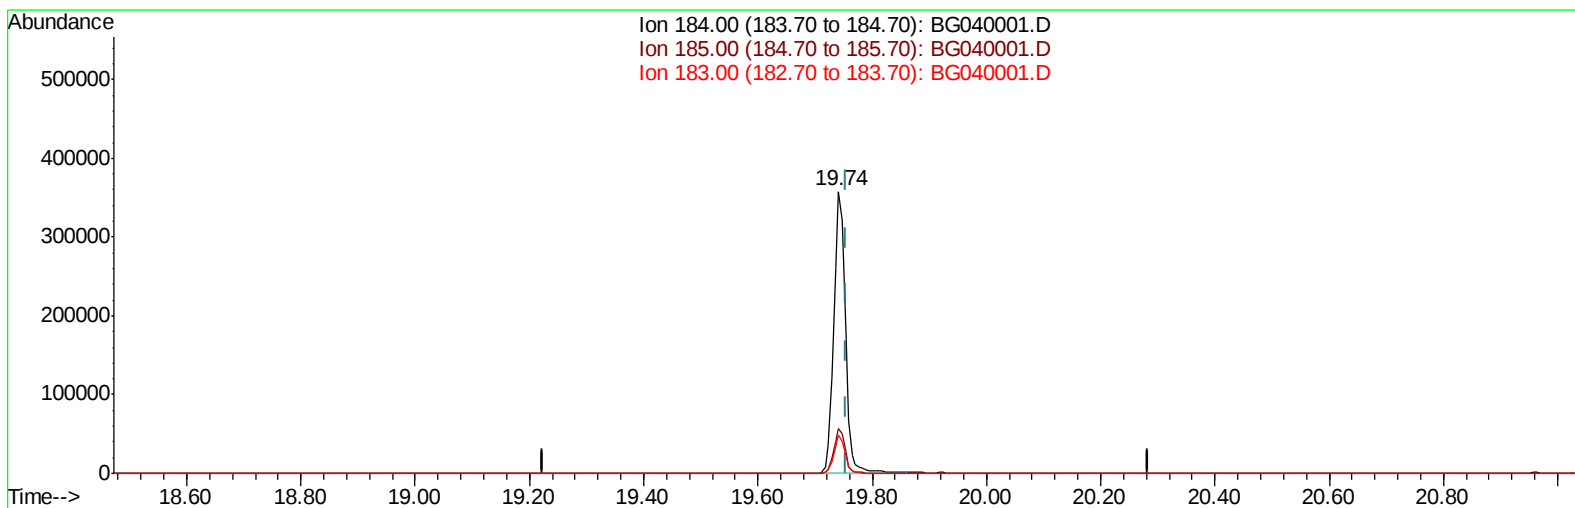

TIC: BG040001.D

(77) Benzidine




19.741min (-0.013) 0.00ng

response 504344

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 15.83 |
| 183.00 | 13.20 | 13.54 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG031919\  
Data File : BG040001.D  
Acq On : 19 Mar 2019 13:23  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 09:04:52 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 14:38:15 2019  
Response via : Initial Calibration

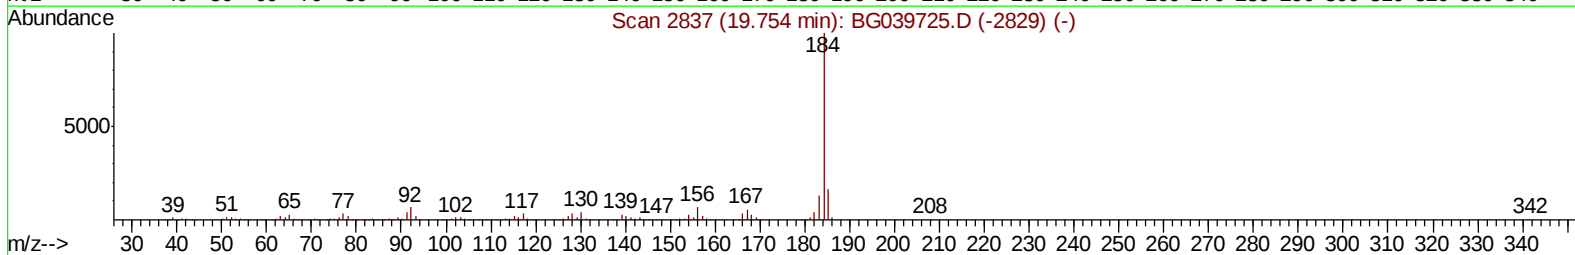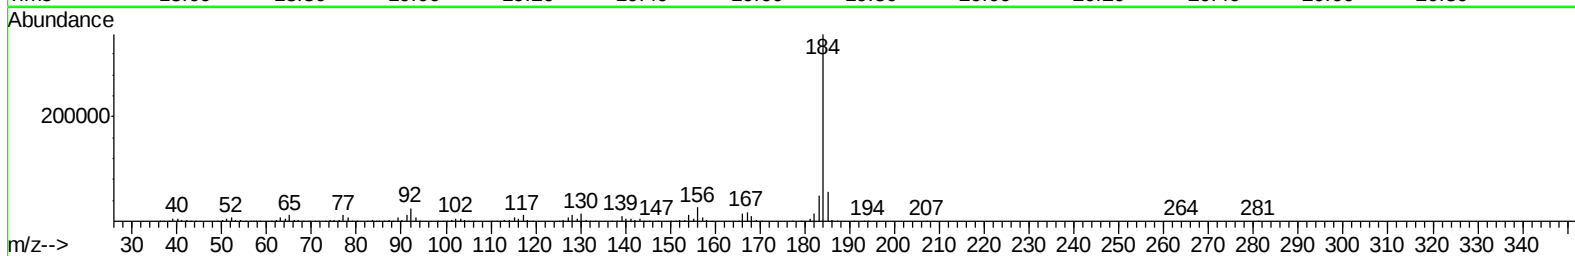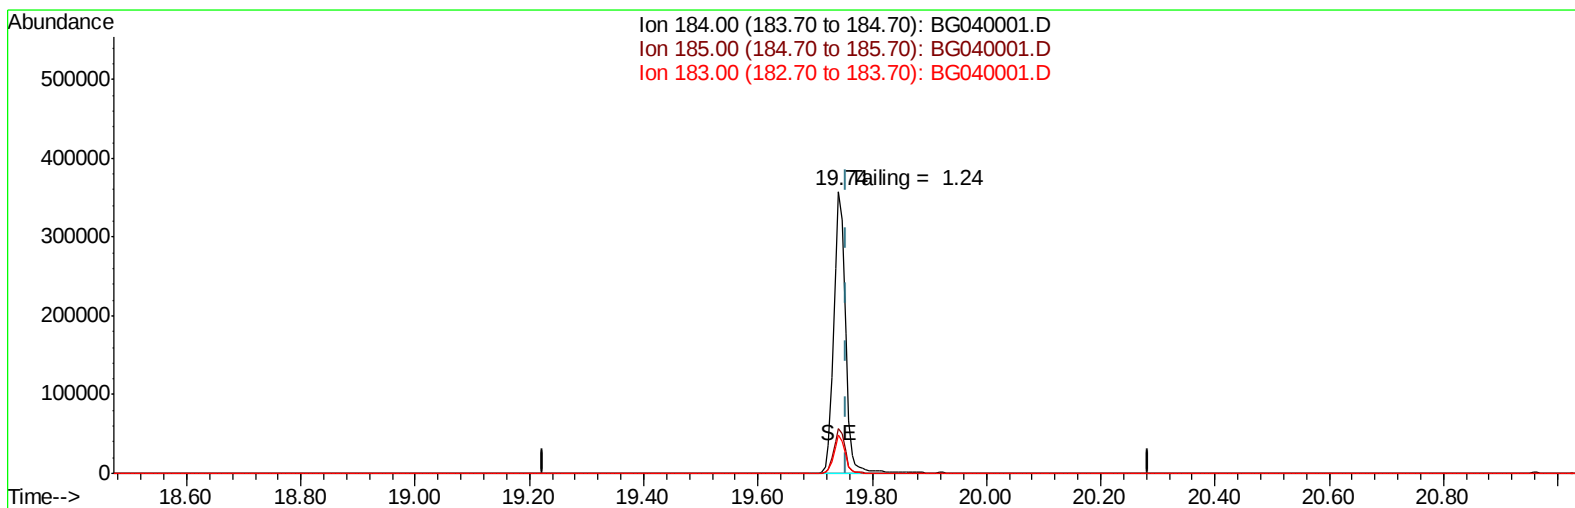

TIC: BG040001.D

(77) Benzidine




19.741min (-0.013) 0.00ng

response 504344

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 15.83 |
| 183.00 | 13.20 | 13.54 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG031919\  
Data File : BG040001.D  
Acq On : 19 Mar 2019 13:23  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 09:04:52 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 04 14:38:15 2019  
Response via : Initial Calibration

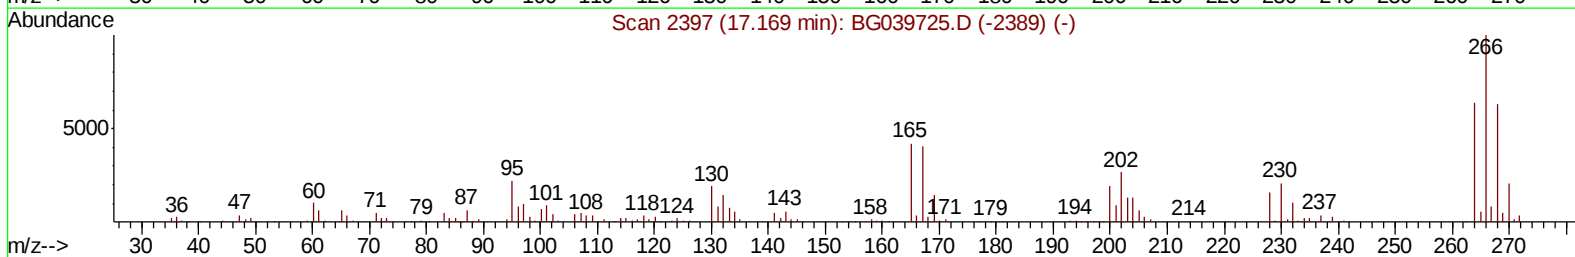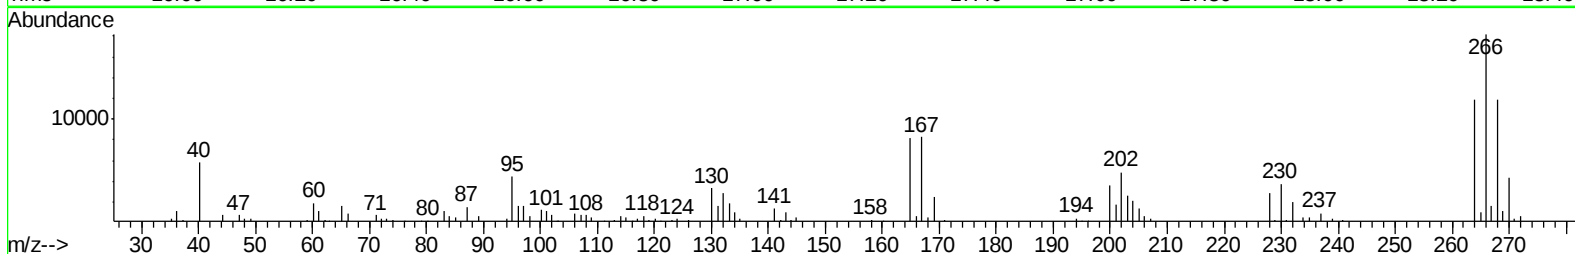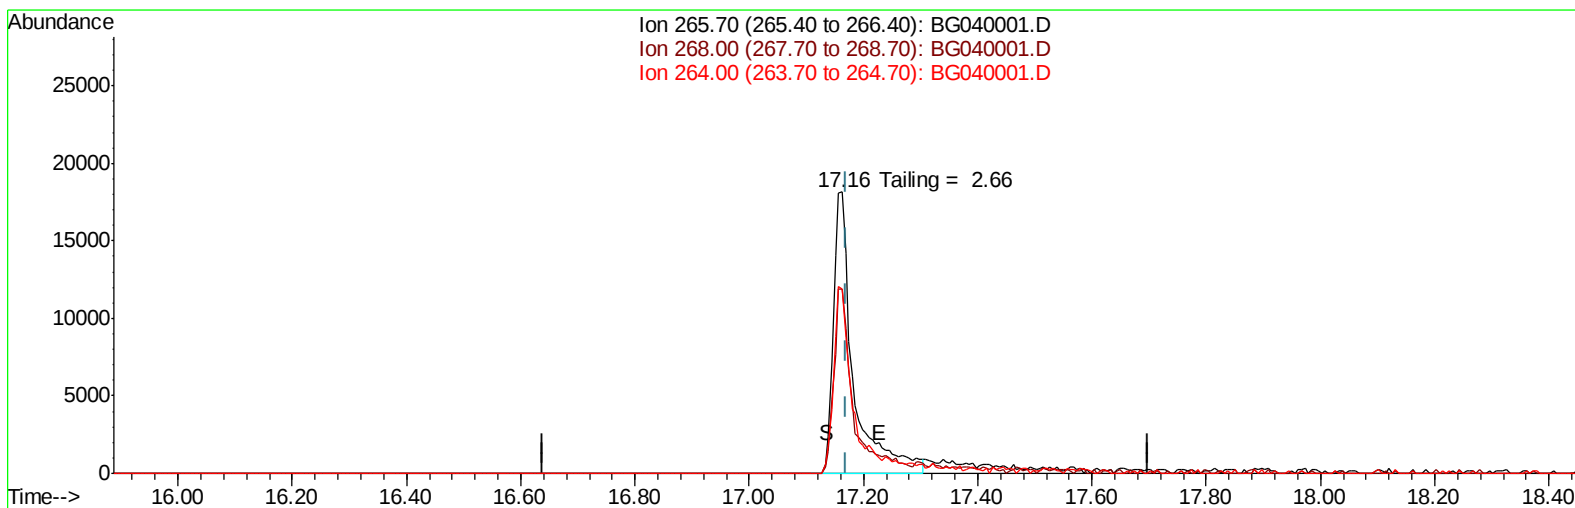

TIC: BG040001.D

(70) Pentachlorophenol (C)

17.162min (-0.008) 9371.22ng

response 43399

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 65.31 |
| 264.00 | 65.10 | 65.56 |
| 0.00   | 0.00  | 0.00  |