
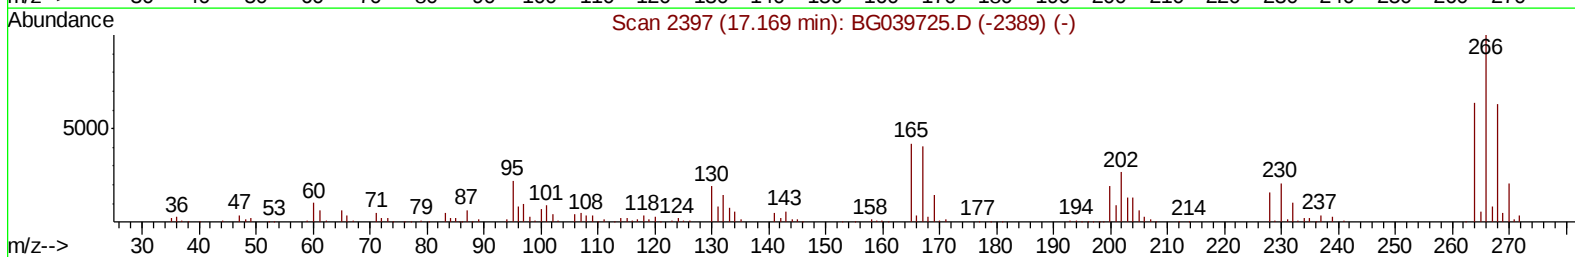
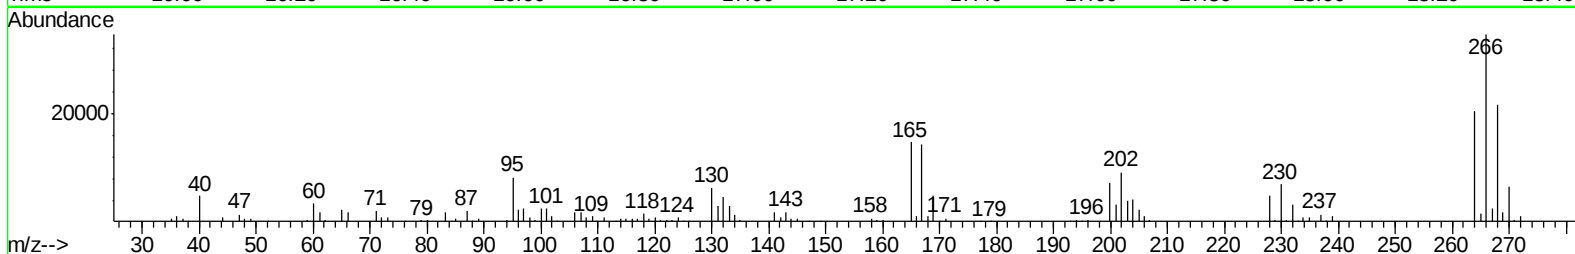


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031919\
 Data File : BG040019.D
 Acq On : 20 Mar 2019 1:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 05:12:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

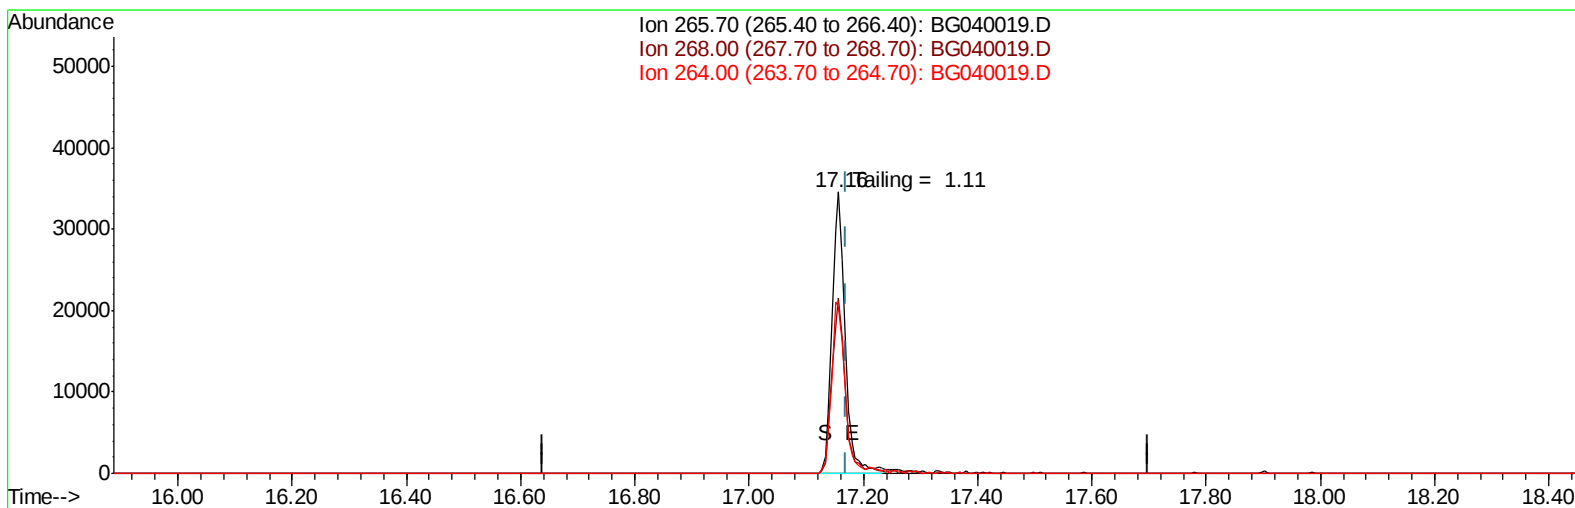

TIC: BG040019.D

(70) Pentachlorophenol (C)




17.157min (-0.013) 0.00ng

response 53753

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.44
264.00	65.10	59.30
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031919\
Data File : BG040019.D
Acq On : 20 Mar 2019 1:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 05:12:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

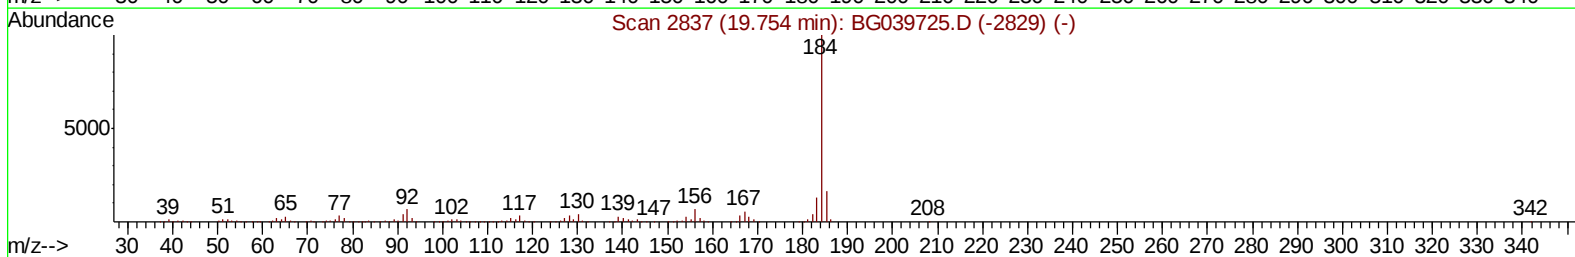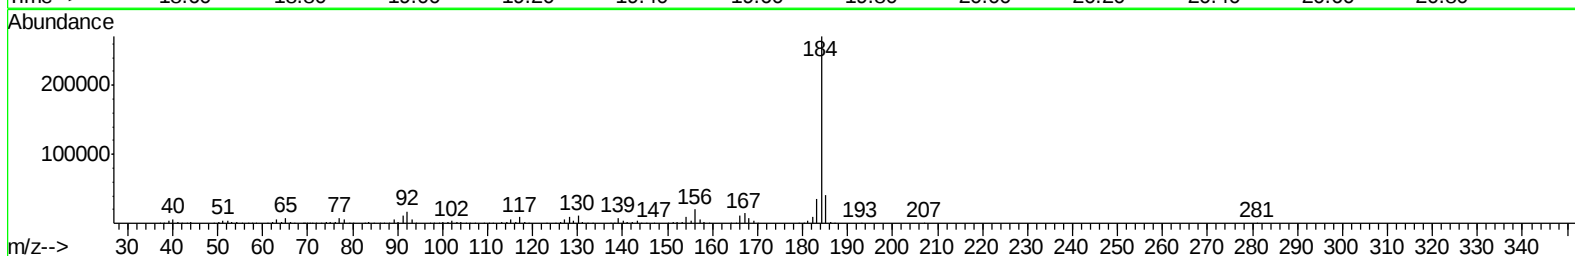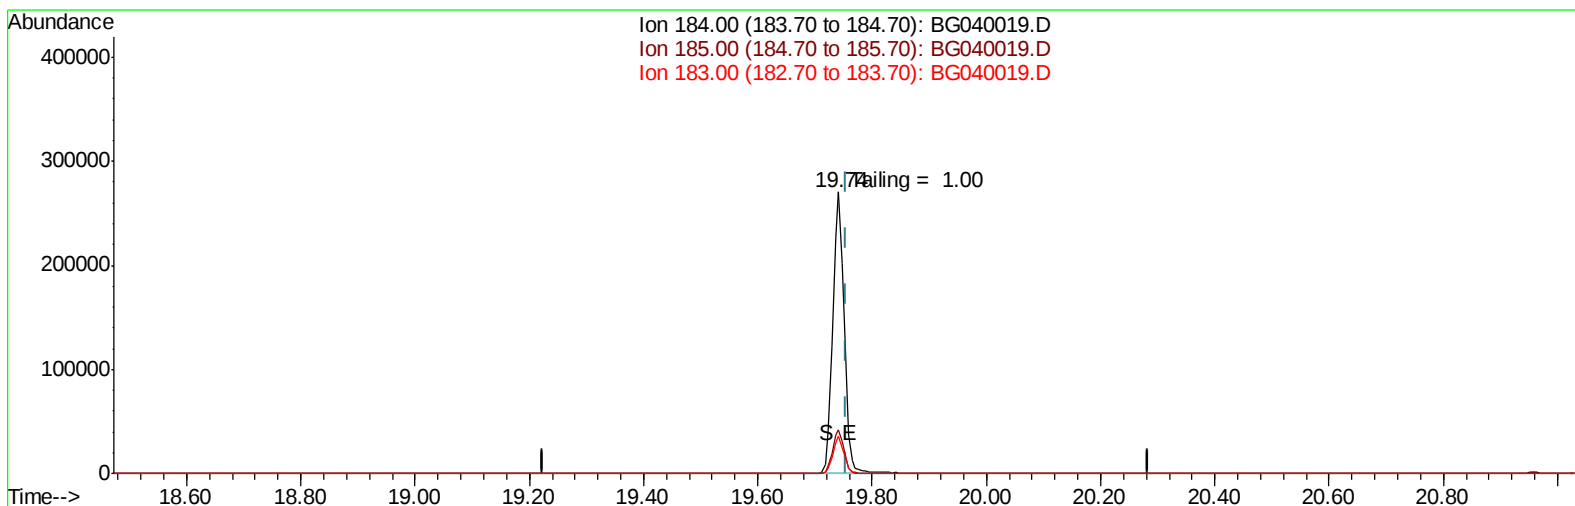

TIC: BG040019.D

(77) Benzidine

19.741min (-0.013) 0.00ng

response 370052

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.47
183.00	13.20	13.06
0.00	0.00	0.00