


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031919\  
 Data File : BG040001.D  
 Acq On : 19 Mar 2019 13:23  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG030419.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Mar 04 14:38:15 2019

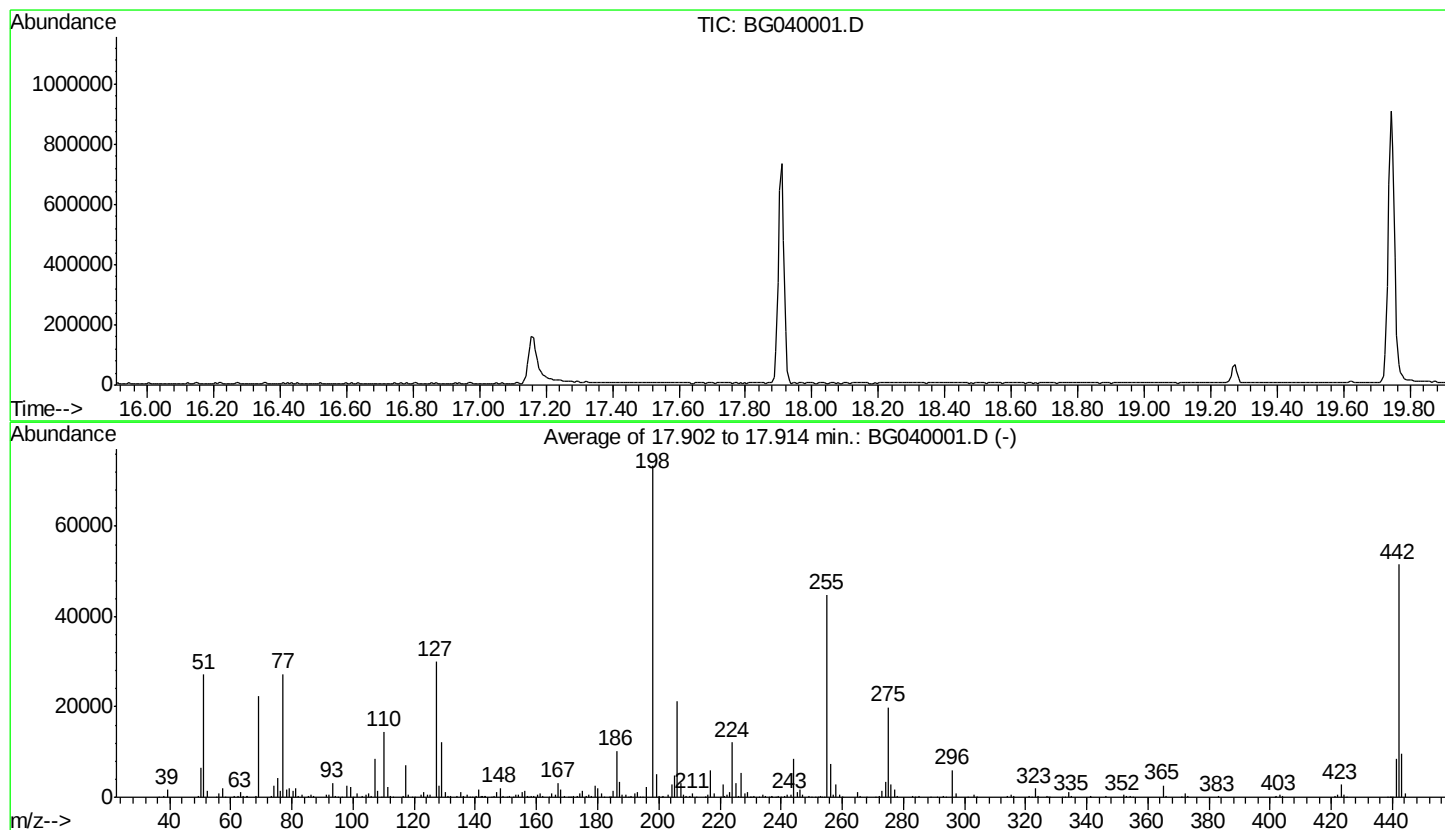

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.0      | 27165   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.7       | 153     | PASS             |
| 69          | 198          | 0.00         | 100          | 30.7      | 22524   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 40.8      | 29986   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 73442   | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 5180    | PASS             |
| 275         | 198          | 10           | 60           | 27.0      | 19864   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 2613    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.4      | 8405    | PASS             |
| 442         | 198          | 50           | 100          | 70.1      | 51504   | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 9760    | PASS             |