

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032019\
 Data File : BG040039.D
 Acq On : 20 Mar 2019 17:03
 Operator : JU/SJ
 Sample : PB118051BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB118051BL

Quant Time: Mar 21 10:41:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	37933	20.00	ng	-0.03
21) Naphthalene-d8	10.96	136	157760	20.00	ng	-0.03
39) Acenaphthene-d10	14.77	164	107530	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	281806	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	320091	20.00	ng	-0.03
87) Perylene-d12	25.15	264	312785	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	229400	103.17	ng	-0.02
7) Phenol-d6	7.29	99	324438	97.86	ng	-0.02
23) Nitrobenzene-d5	9.32	82	192572	66.02	ng	-0.03
42) 2,4,6-Tribromophenol	16.25	330	130539	104.15	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	499368	66.12	ng	-0.02
79) Terphenyl-d14	20.11	244	960116	66.04	ng	-0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032019\
Data File : BG040039.D
Acq On : 20 Mar 2019 17:03
Operator : JU/SJ
Sample : PB118051BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118051BL

Quant Time: Mar 21 10:41:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

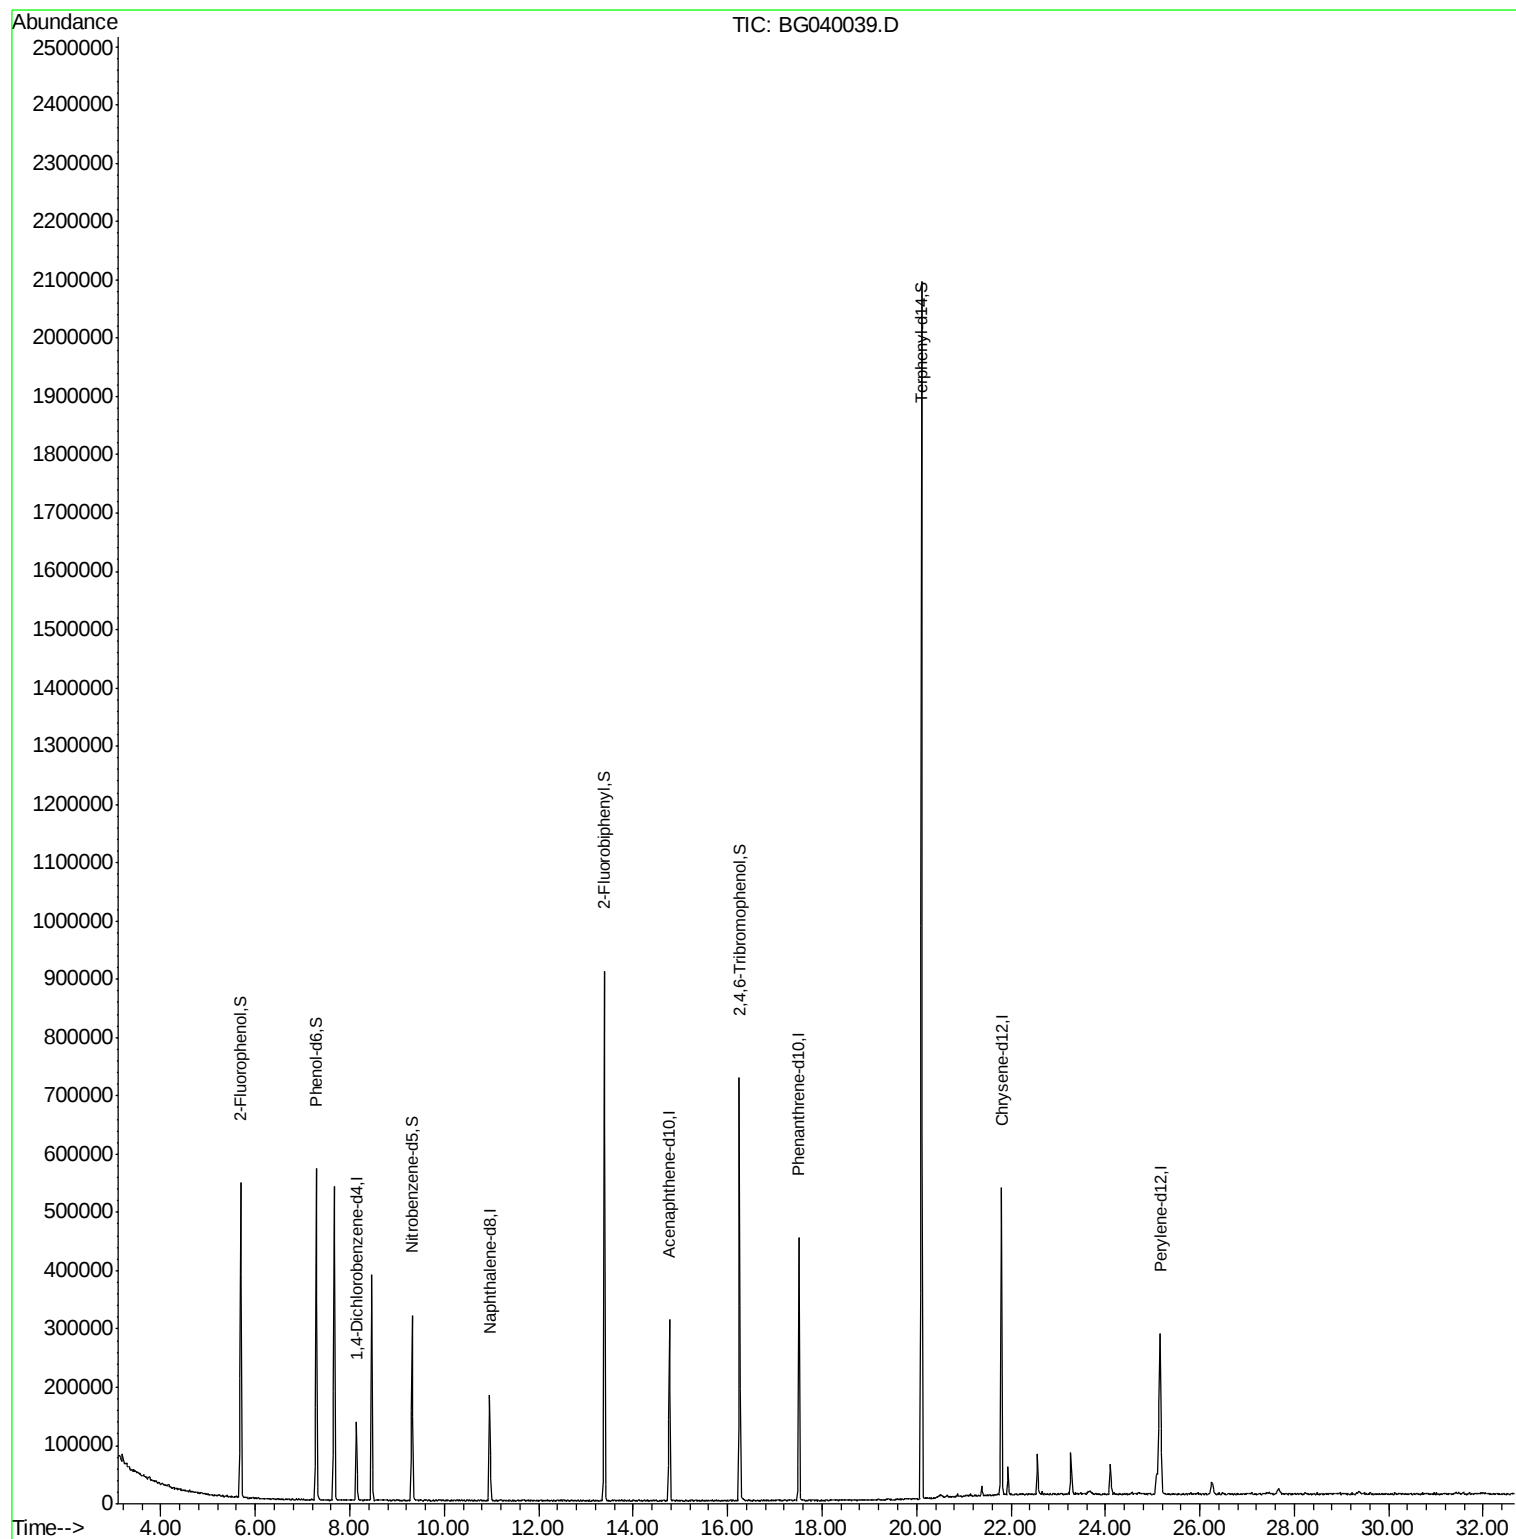



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.14 min Scan# 860

Delta R.T. -0.03 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03

Instrument :

BNA_G

ClientSampleId :

PB118051BL


Tgt Ion:152 Resp: 37933

Ion Ratio Lower Upper

152 100

150 147.7 123.7 185.5




115 55.8 45.9 68.9

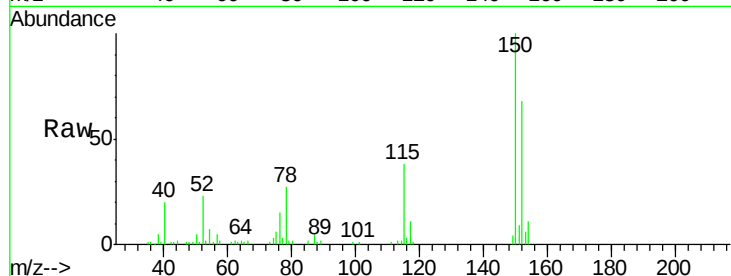

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

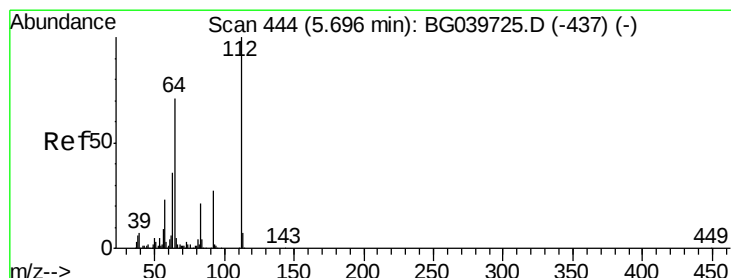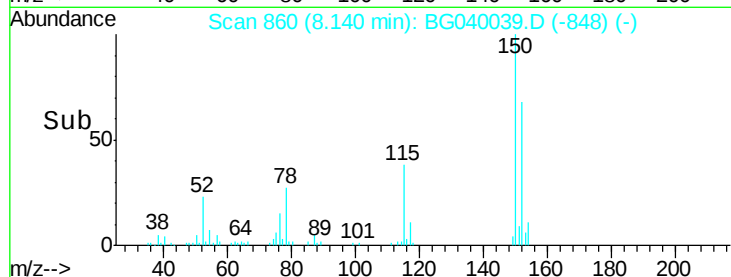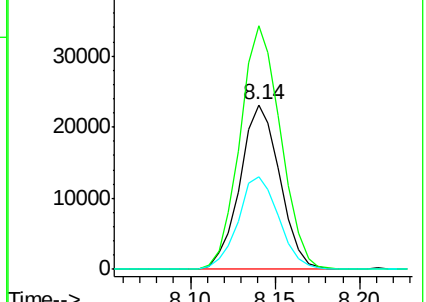

#5

2-Fluorophenol

Concen: 103.171 ng

RT: 5.69 min Scan# 443

Delta R.T. -0.02 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03


Tgt Ion:112 Resp: 229400

Ion Ratio Lower Upper

112 100

64 68.6 57.8 86.8



63 35.7 29.8 44.6

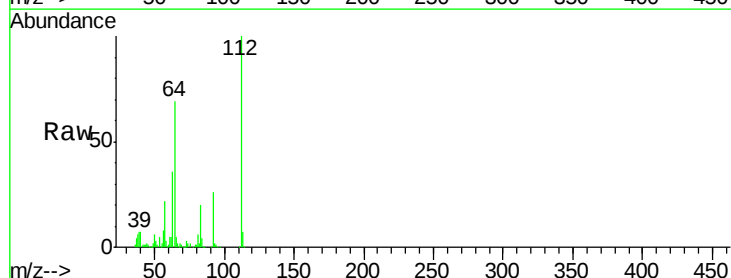

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

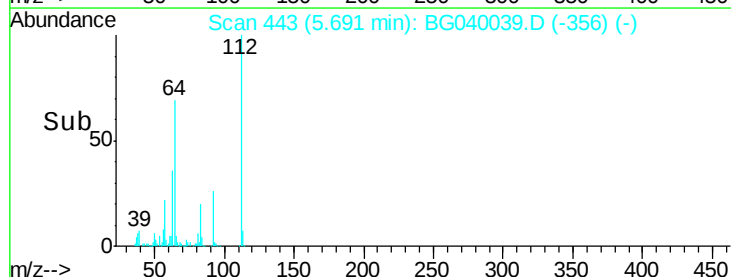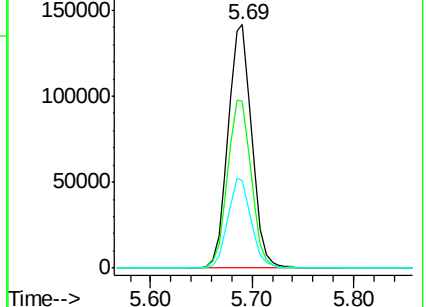



#7

Phenol-d6

Concen: 97.859 ng

RT: 7.29 min Scan# 715

Delta R.T. -0.02 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03

Instrument :

BNA_G

ClientSampleId :

PB118051BL


Tgt Ion: 99 Resp: 324438

Ion Ratio Lower Upper



99 100

42 19.8 18.2 27.2

71 34.9 28.0 42.0

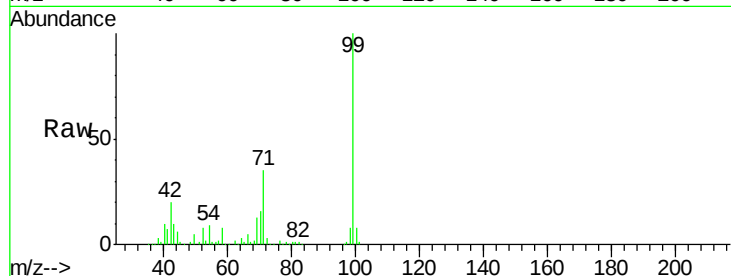

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

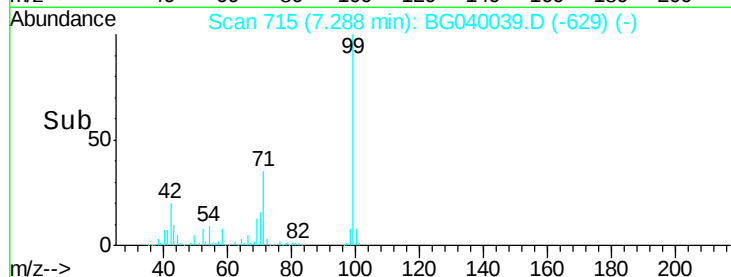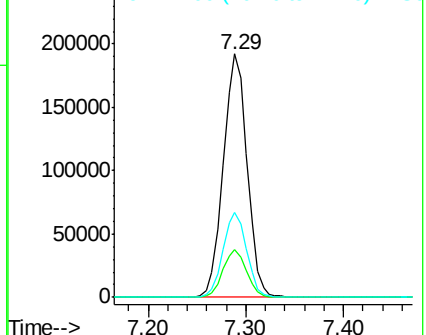

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.96 min Scan# 1340

Delta R.T. -0.03 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03

Tgt Ion: 136 Resp: 157760


Ion Ratio Lower Upper

136 100



137 10.7 9.1 13.7


54 9.5 9.4 14.2

68 5.4 4.2 6.4

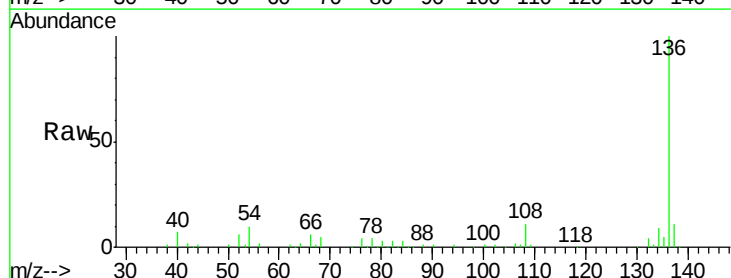

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

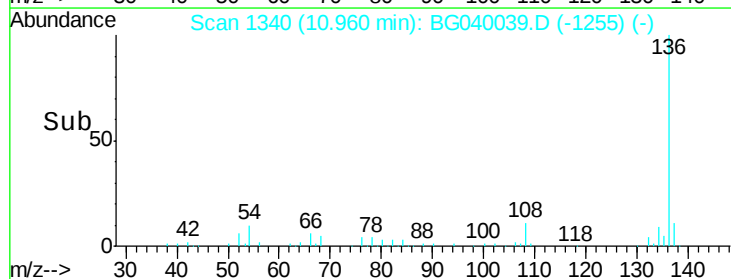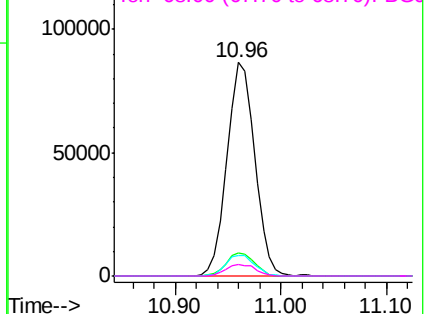


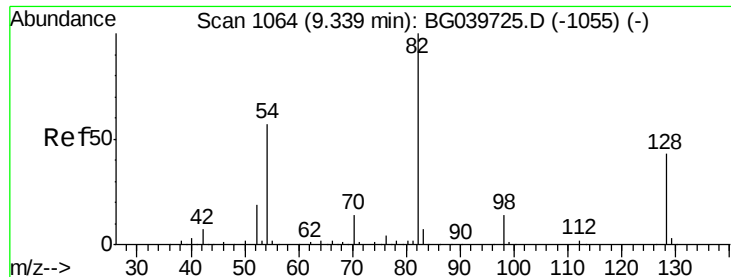




#23
 Nitrobenzene-d5
 Concen: 66.018 ng
 RT: 9.32 min Scan# 1060
 Delta R.T. -0.03 min
 Lab File: BG040039.D
 Acq: 20 Mar 2019 17:03

Instrument :
 BNA_G
 ClientSampleId :
 PB118051BL

Tgt Ion: 82 Resp: 192572
 Ion Ratio Lower Upper
 82 100
 128 41.2 31.3 46.9
 54 58.0 50.9 76.3

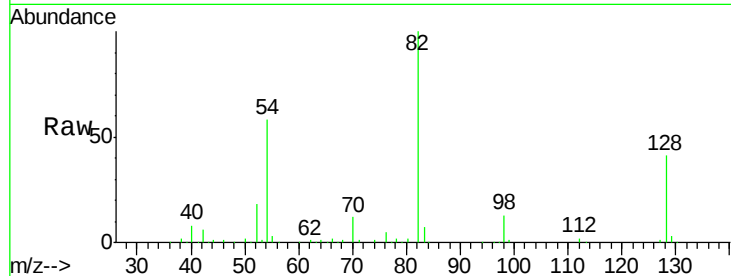


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

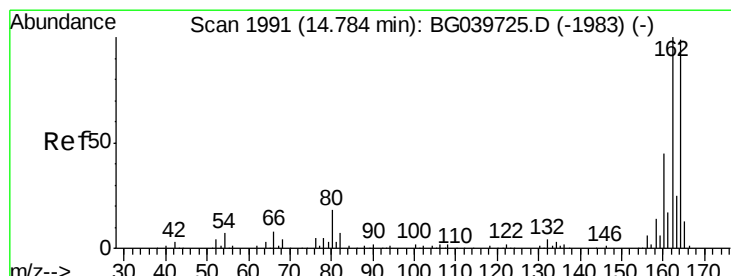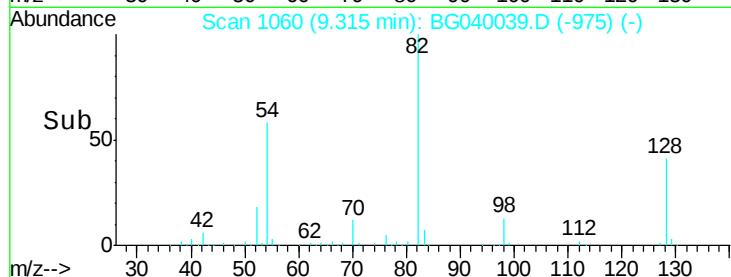
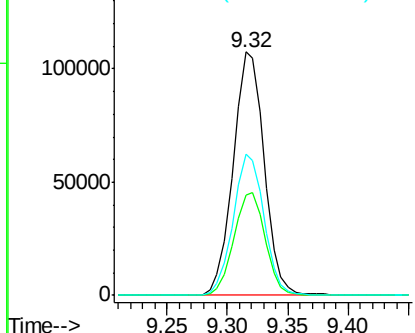



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.77 min Scan# 1988
 Delta R.T. -0.02 min
 Lab File: BG040039.D
 Acq: 20 Mar 2019 17:03

Tgt Ion: 164 Resp: 107530
 Ion Ratio Lower Upper
 164 100
 162 103.3 81.6 122.4
 160 44.3 34.2 51.2

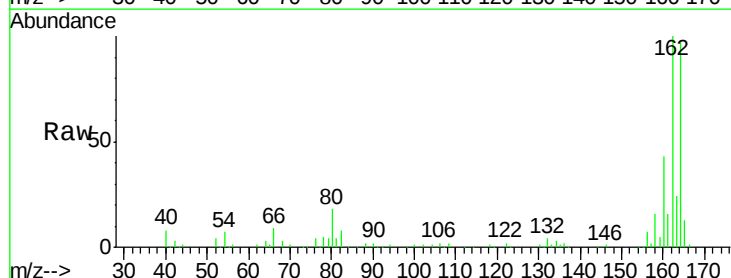

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

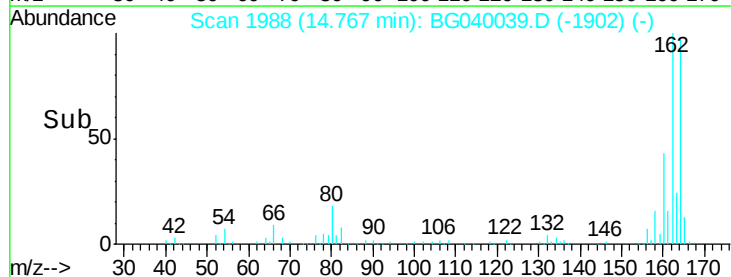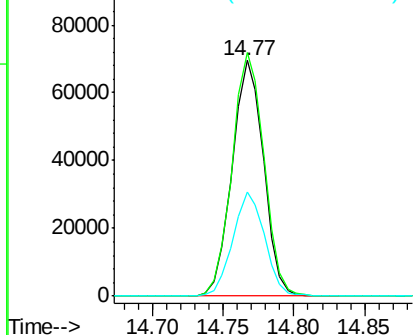


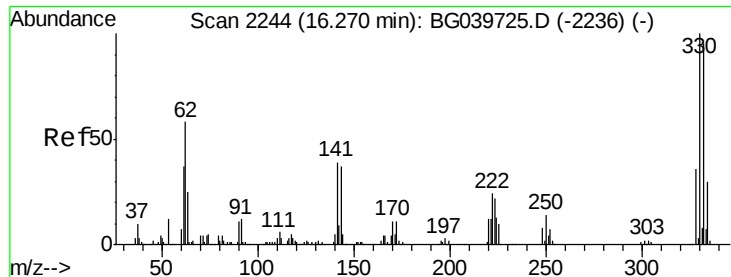




#42
 2,4,6-Tribromophenol
 Concen: 104.153 ng
 RT: 16.25 min Scan# 2241
 Delta R.T. -0.02 min
 Lab File: BG040039.D
 Acq: 20 Mar 2019 17:03

Instrument :
 BNA_G
 ClientSampleID :
 PB118051BL

Tgt Ion:330 Resp: 130539
 Ion Ratio Lower Upper
 330 100
 332 95.3 75.7 113.5
 141 40.8 35.6 53.4

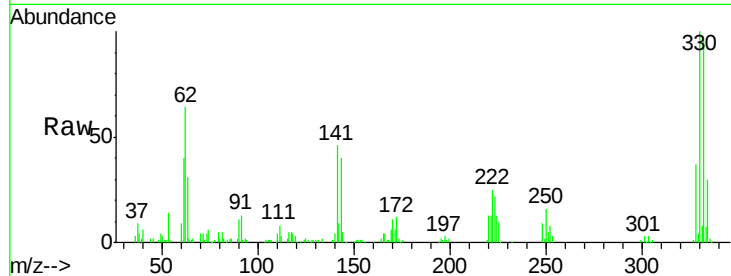


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

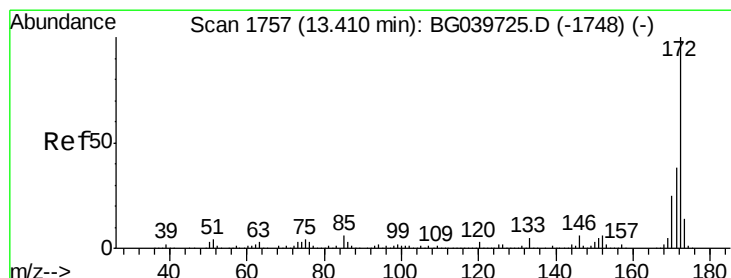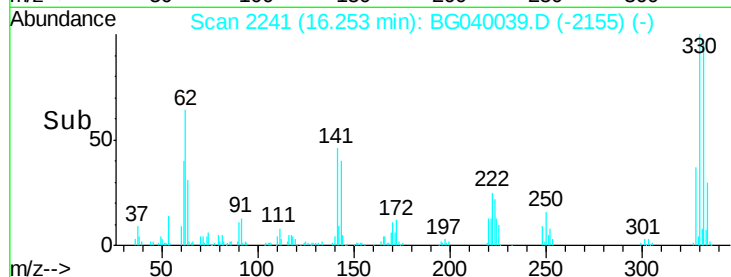
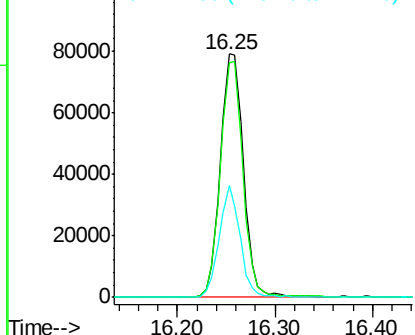



#45
 2-Fluorobiphenyl
 Concen: 66.122 ng
 RT: 13.39 min Scan# 1754
 Delta R.T. -0.02 min
 Lab File: BG040039.D
 Acq: 20 Mar 2019 17:03

Tgt Ion:172 Resp: 499368
 Ion Ratio Lower Upper
 172 100
 171 36.2 30.8 46.2
 170 24.3 20.2 30.4

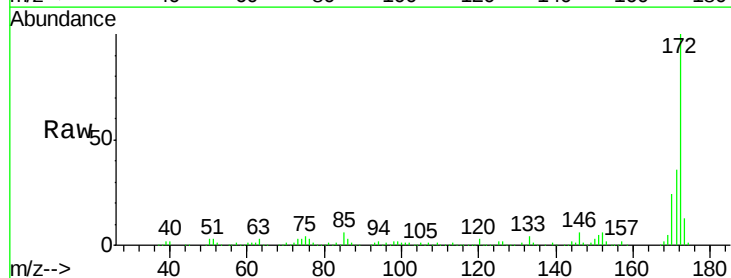

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

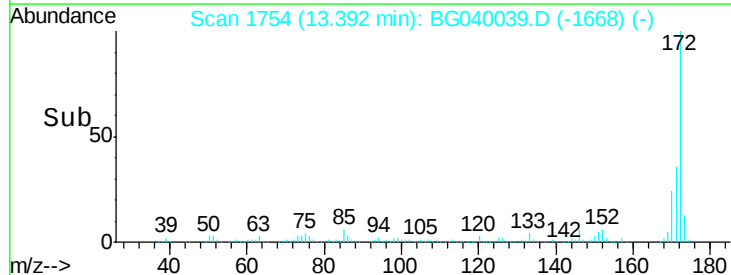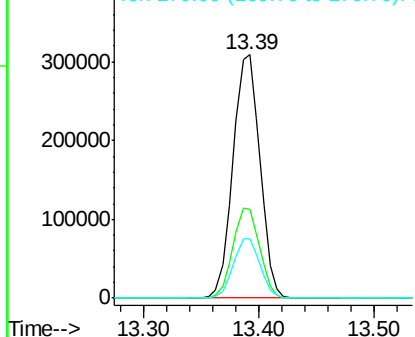

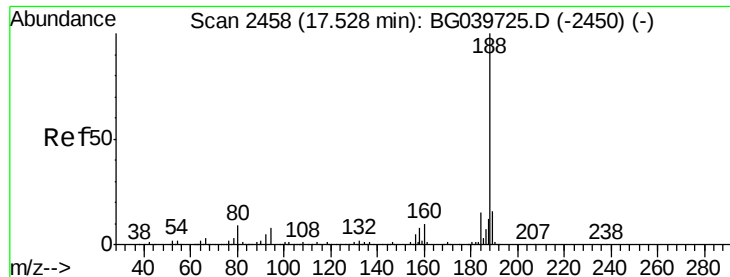

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.51 min Scan# 2455

Delta R.T. -0.02 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03

Instrument :

BNA_G

ClientSampleId :

PB118051BL


Tgt Ion:188 Resp: 281806

Ion Ratio Lower Upper

188 100

94 8.7 6.9 10.3




80 9.1 8.1 12.1

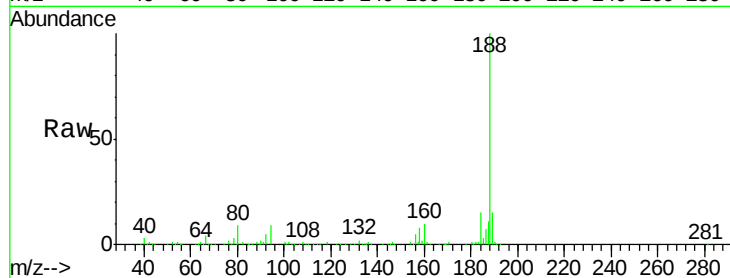

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

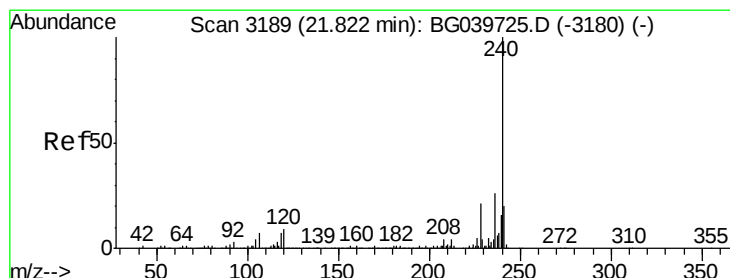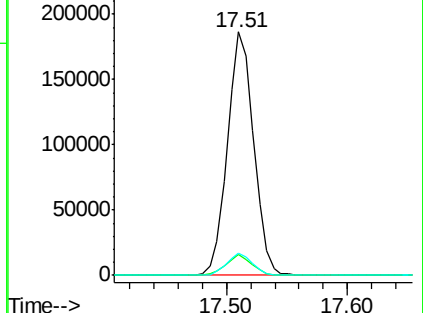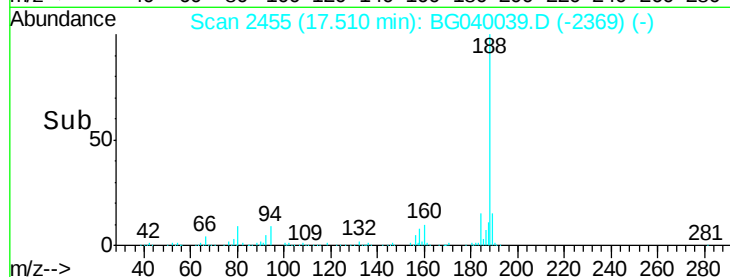

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3185

Delta R.T. -0.03 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03


Tgt Ion:240 Resp: 320091

Ion Ratio Lower Upper

240 100

120 8.8 7.0 10.6



236 26.1 21.0 31.4

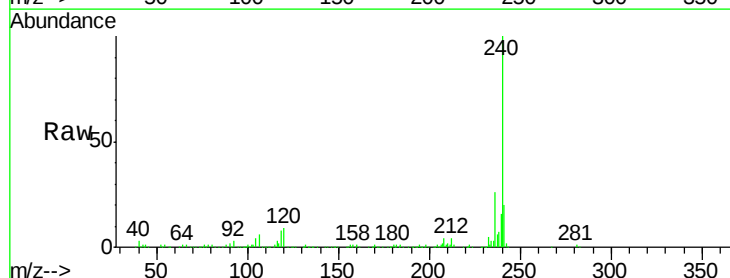


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

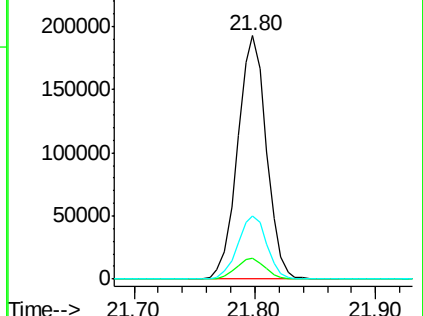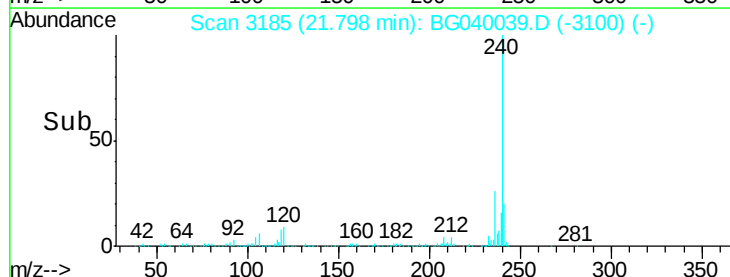

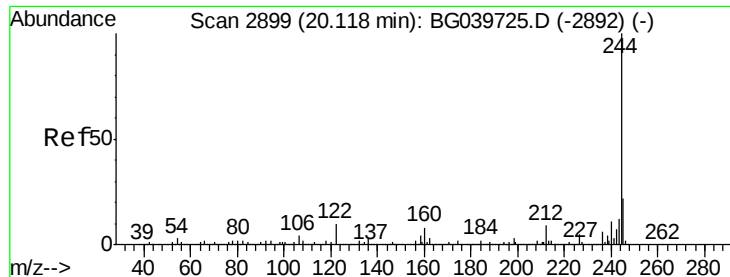

#79

Terphenyl-d14

Concen: 66.043 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03

Instrument :

BNA_G

ClientSampleId :

PB118051BL


Tgt Ion:244 Resp: 960116

Ion Ratio Lower Upper

244 100

212 9.0 7.3 10.9




122 8.9 8.4 12.6

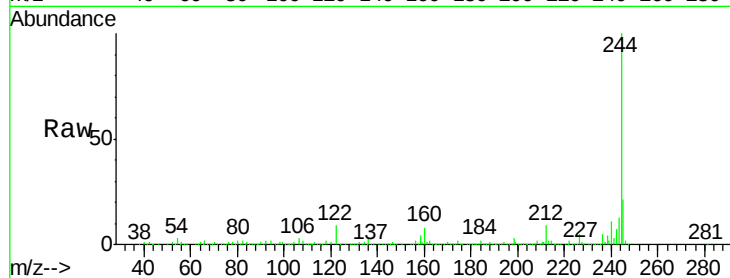

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

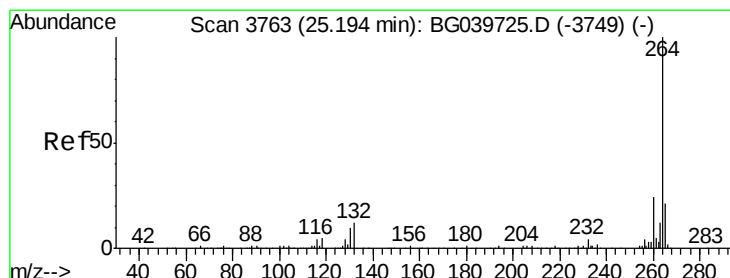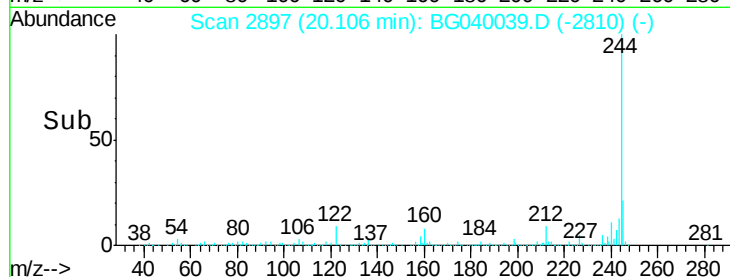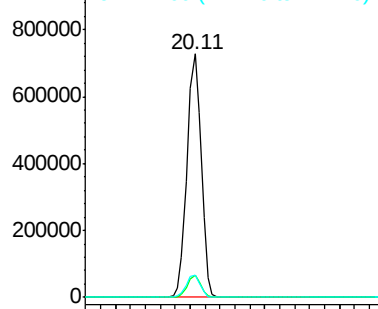

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.15 min Scan# 3756

Delta R.T. -0.05 min

Lab File: BG040039.D

Acq: 20 Mar 2019 17:03


Tgt Ion:264 Resp: 312785

Ion Ratio Lower Upper

264 100

260 23.2 18.2 27.4

265 21.6 18.5 27.7

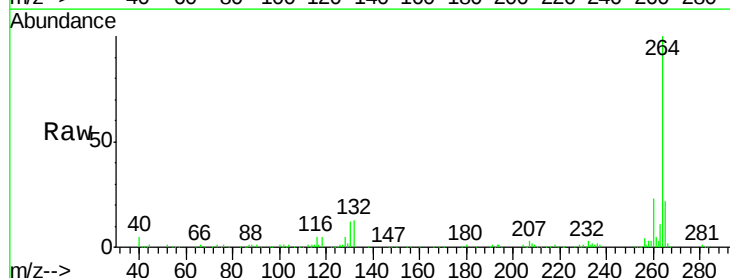

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

