

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032019\
 Data File : BG040050.D
 Acq On : 21 Mar 2019 00:26
 Operator : JU/SJ
 Sample : K1987-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20190084-FIELD-DUPLICATE

Quant Time: Mar 21 11:43:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	39701	20.00	ng	-0.03
21) Naphthalene-d8	10.96	136	176488	20.00	ng	-0.03
39) Acenaphthene-d10	14.77	164	120959	20.00	ng	-0.03
64) Phenanthrene-d10	17.51	188	287843	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	278180	20.00	ng	-0.03
87) Perylene-d12	25.16	264	279267	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	299855	128.85	ng	-0.02
7) Phenol-d6	7.29	99	437464	126.07	ng	-0.02
23) Nitrobenzene-d5	9.32	82	267576	82.00	ng	-0.03
42) 2,4,6-Tribromophenol	16.26	330	177447	125.86	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	635791	74.84	ng	-0.03
79) Terphenyl-d14	20.11	244	926982	73.37	ng	-0.02
Target Compounds						
10) Phenol	7.32	94	26132	6.952	ng	Qvalue 94
50) Dimethylphthalate	14.21	163	51296	5.072	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032019\
Data File : BG040050.D
Acq On : 21 Mar 2019 00:26
Operator : JU/SJ
Sample : K1987-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20190084-FIELD-DUPLICATE

Quant Time: Mar 21 11:43:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

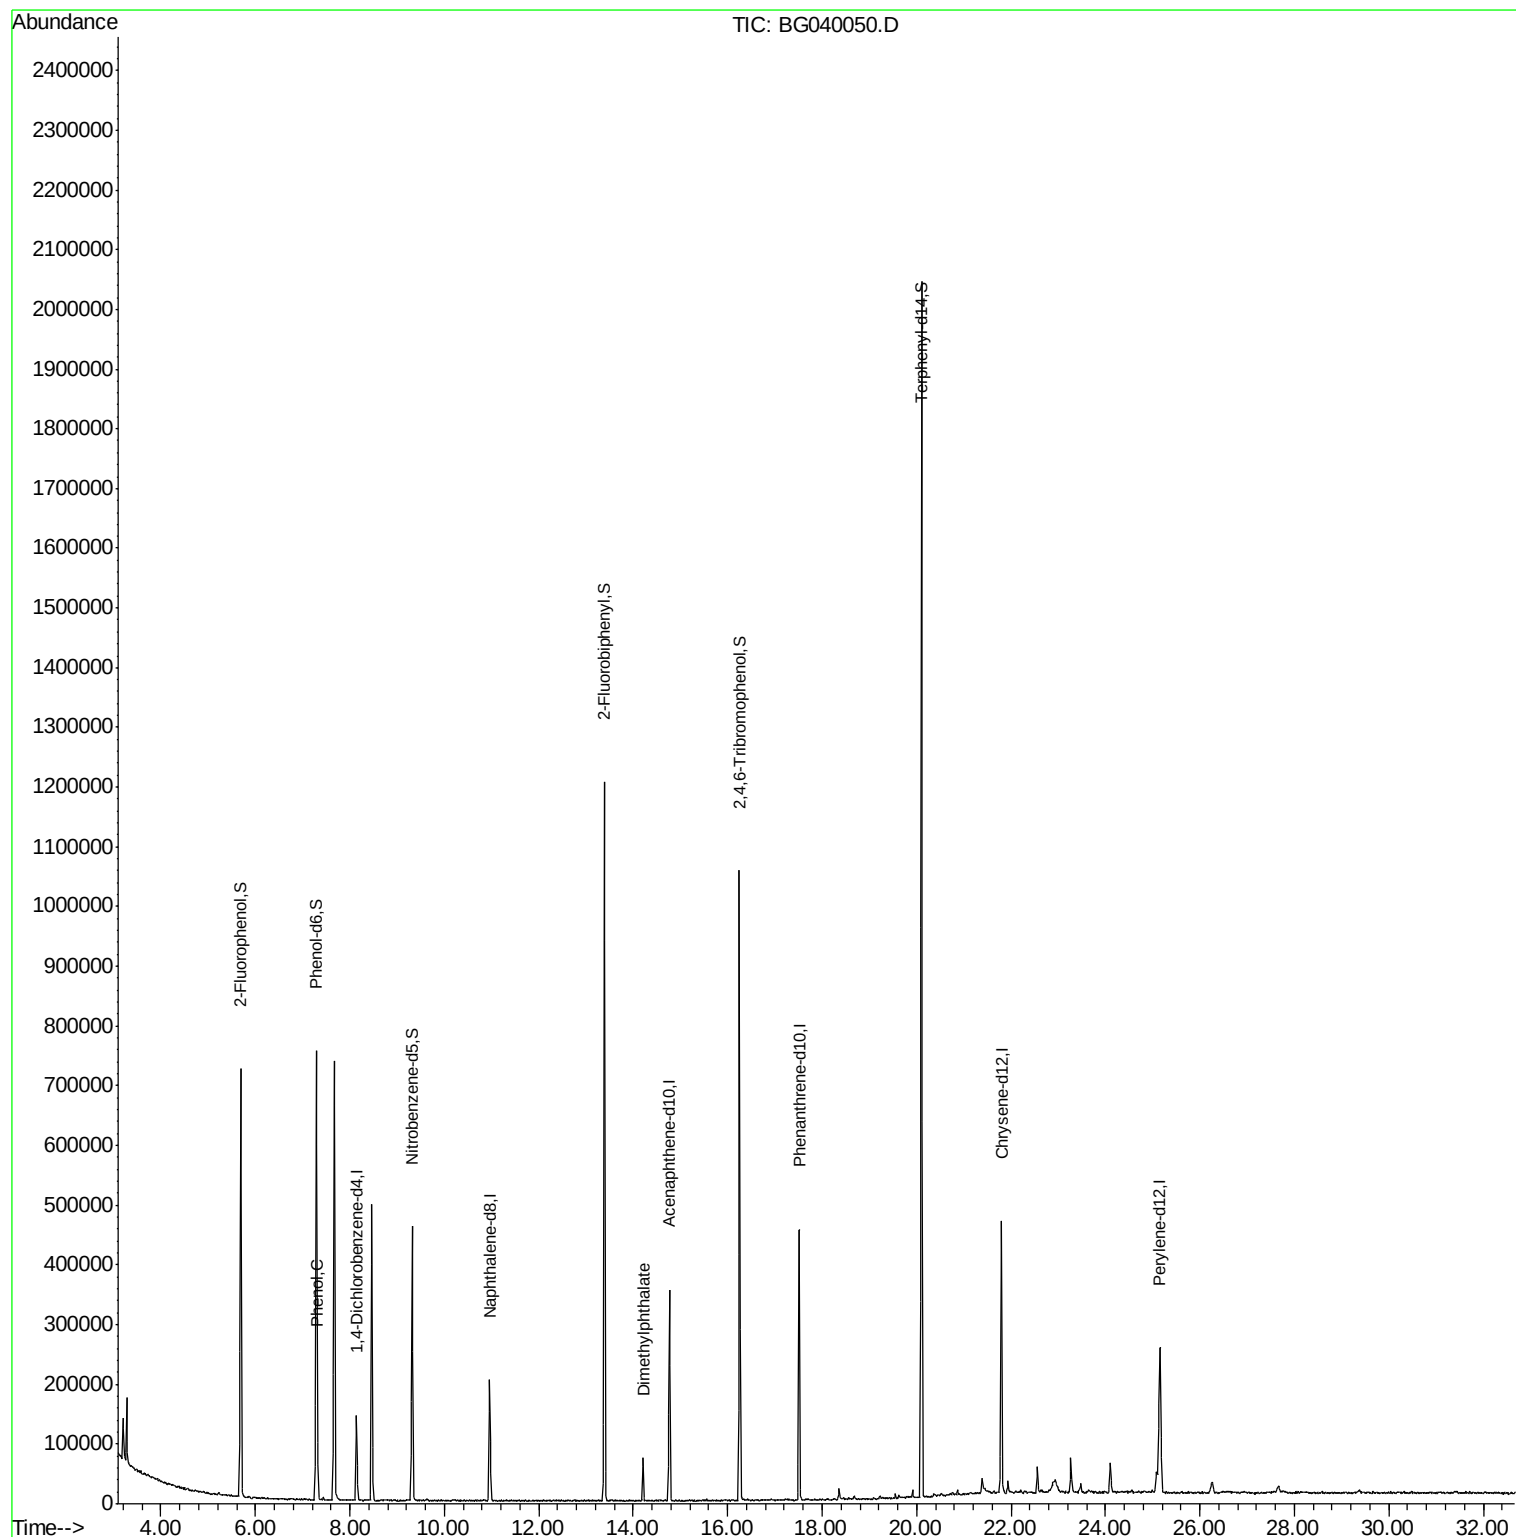

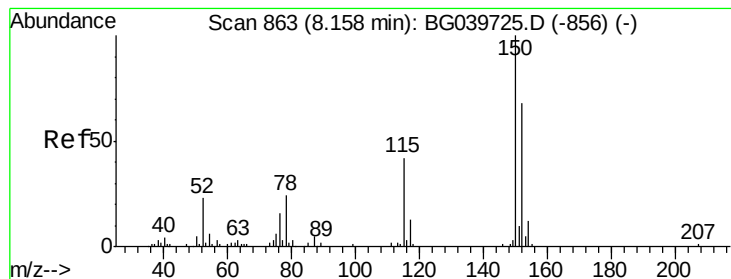

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.14 min Scan# 860

Delta R.T. -0.03 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26

Instrument :

BNA_G

ClientSampleId :

20190084-FIELD-DUPLICATE


Tgt Ion:152 Resp: 39701

Ion Ratio Lower Upper

152 100

150 156.4 123.7 185.5




115 62.4 45.9 68.9



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

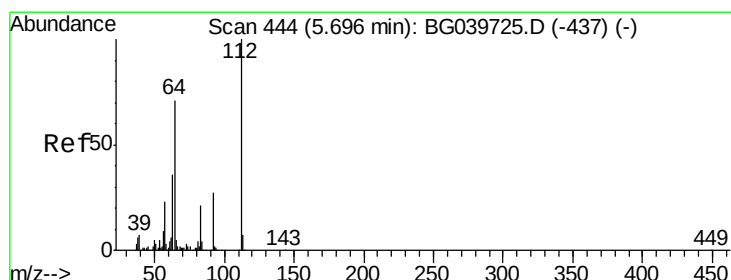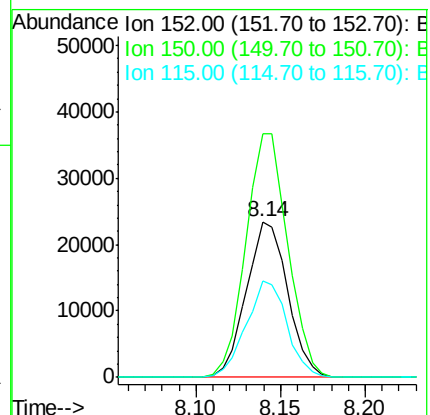

#5

2-Fluorophenol

Concen: 128.852 ng

RT: 5.69 min Scan# 443

Delta R.T. -0.02 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26


Tgt Ion:112 Resp: 299855

Ion Ratio Lower Upper

112 100

64 69.8 57.8 86.8



63 38.7 29.8 44.6






Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

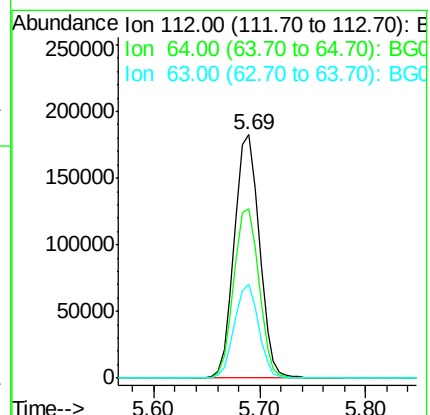

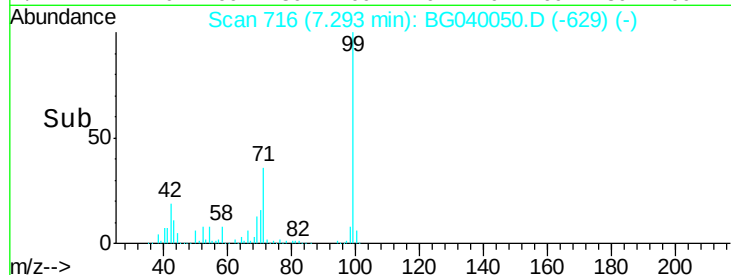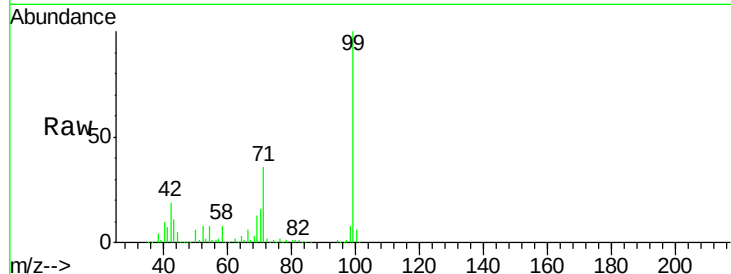

#7

Phenol-d6

Concen: 126.075 ng

RT: 7.29 min Scan# 716

Delta R.T. -0.02 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26

Instrument :

BNA_G

ClientSampleId :

20190084-FIELD-DUPLICATE





Tgt Ion: 99 Resp: 437464

Ion Ratio Lower Upper

99 100

42 19.2 18.2 27.2

71 36.0 28.0 42.0

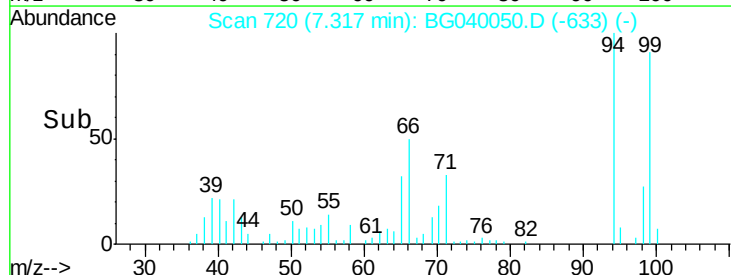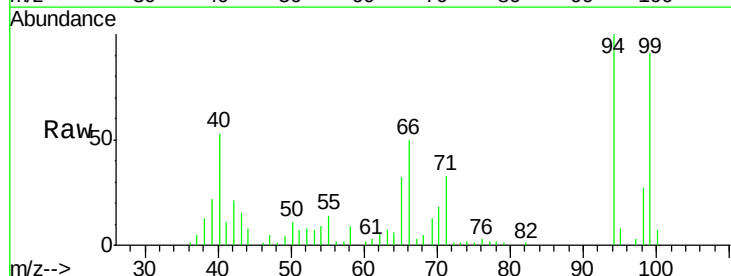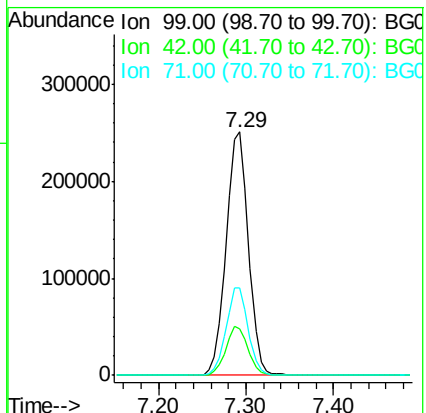

#10

Phenol

Concen: 6.952 ng

RT: 7.32 min Scan# 720

Delta R.T. -0.02 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26


Tgt Ion: 94 Resp: 26132


Ion Ratio Lower Upper

94 100

65 31.9 11.7 51.7

66 50.1 23.7 63.7

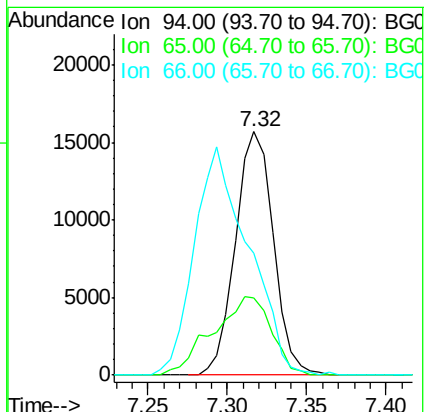


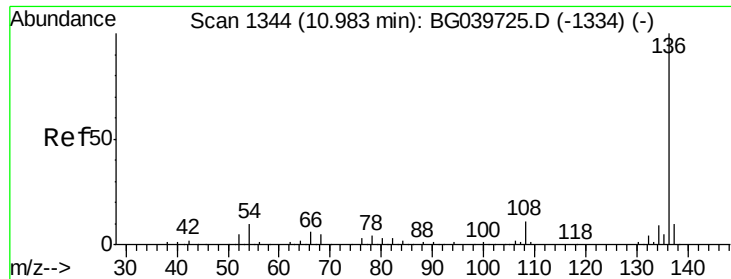




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.96 min Scan# 1341
Delta R.T. -0.03 min
Lab File: BG040050.D
Acq: 21 Mar 2019 00:26

Instrument :
BNA_G
ClientSampleId :
20190084-FIELD-DUPLICATE

Tgt Ion:	136	Resp:	176488
Ion	Ratio	Lower	Upper
136	100		
137	9.7	9.1	13.7
54	10.5	9.4	14.2
68	5.4	4.2	6.4




Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

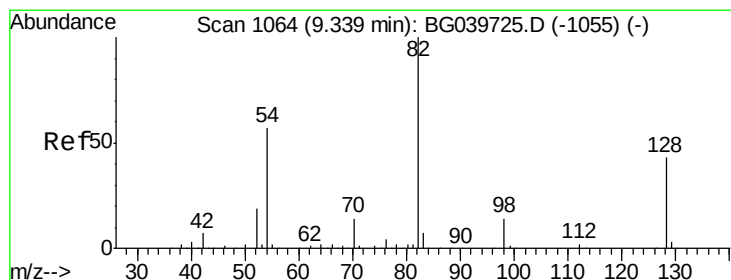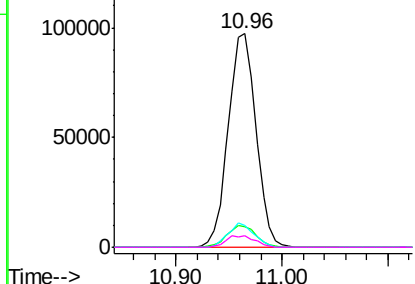




#23
Nitrobenzene-d5
Concen: 81.998 ng
RT: 9.32 min Scan# 1061
Delta R.T. -0.03 min
Lab File: BG040050.D
Acq: 21 Mar 2019 00:26

Tgt Ion:	82	Resp:	267576
Ion	Ratio	Lower	Upper
82	100		
128	41.9	31.3	46.9
54	58.8	50.9	76.3



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

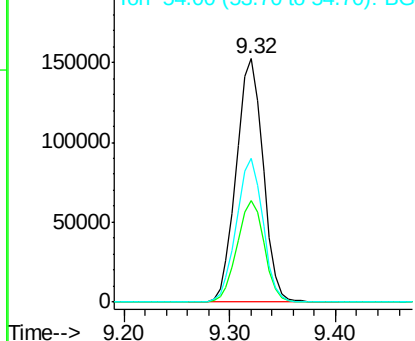



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.77 min Scan# 1988

Delta R.T. -0.03 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26

Instrument :

BNA_G

ClientSampleId :

20190084-FIELD-DUPLICATE


Tgt Ion:164 Resp: 120959

Ion Ratio Lower Upper

164 100

162 103.5 81.6 122.4




160 44.7 34.2 51.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

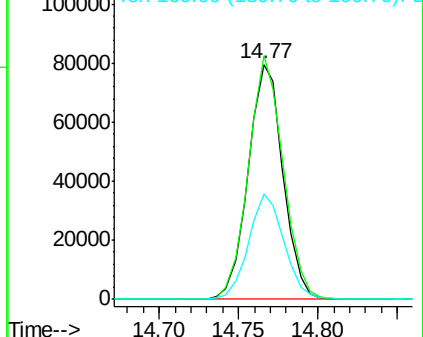

#42

2,4,6-Tribromophenol

Concen: 125.861 ng

RT: 16.26 min Scan# 2242

Delta R.T. -0.02 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26


Tgt Ion:330 Resp: 177447

Ion Ratio Lower Upper

330 100

332 96.7 75.7 113.5



141 42.6 35.6 53.4




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




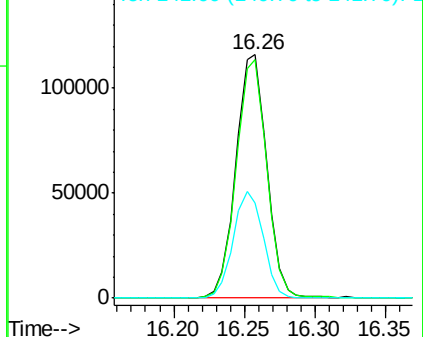




#45
2-Fluorobiphenyl
Concen: 74.840 ng
RT: 13.39 min Scan# 1754
Delta R.T. -0.03 min
Lab File: BG040050.D
Acq: 21 Mar 2019 00:26




Instrument :
BNA_G
ClientSampleId :
20190084-FIELD-DUPLICATE


Tgt Ion:172 Resp: 635791
Ion Ratio Lower Upper
172 100
171 36.9 30.8 46.2
170 25.0 20.2 30.4

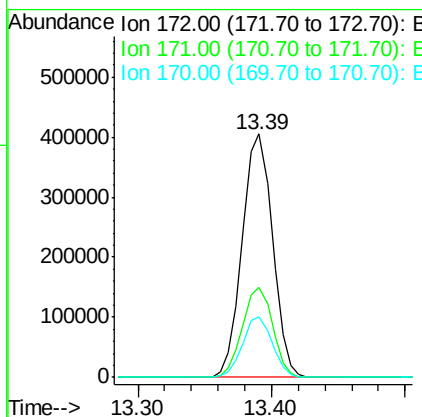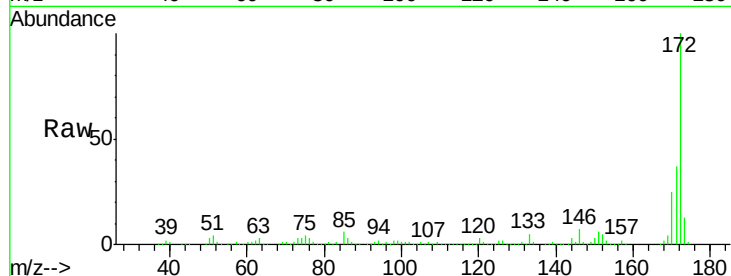

#50
Dimethylphthalate
Concen: 5.072 ng
RT: 14.21 min Scan# 1894
Delta R.T. -0.03 min
Lab File: BG040050.D
Acq: 21 Mar 2019 00:26

Tgt Ion:163 Resp: 51296
Ion Ratio Lower Upper
163 100
194 5.7 3.6 5.4#
164 9.5 8.4 12.6



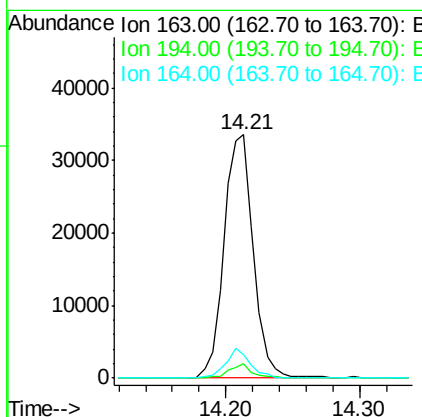





#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.51 min Scan# 2456
 Delta R.T. -0.02 min
 Lab File: BG040050.D
 Acq: 21 Mar 2019 00:26




Instrument :
 BNA_G
 ClientSampleId :
 20190084-FIELD-DUPLICATE


Tgt Ion:188 Resp: 287843
 Ion Ratio Lower Upper
 188 100
 94 7.4 6.9 10.3
 80 8.6 8.1 12.1

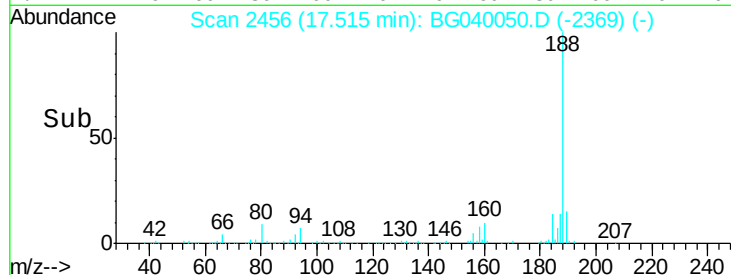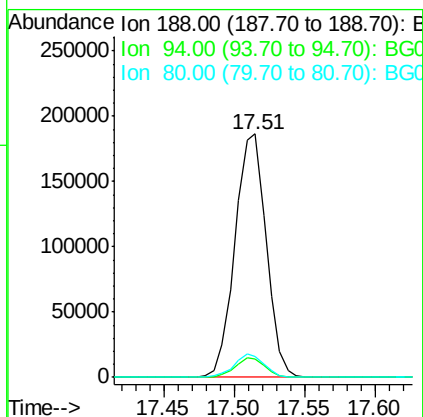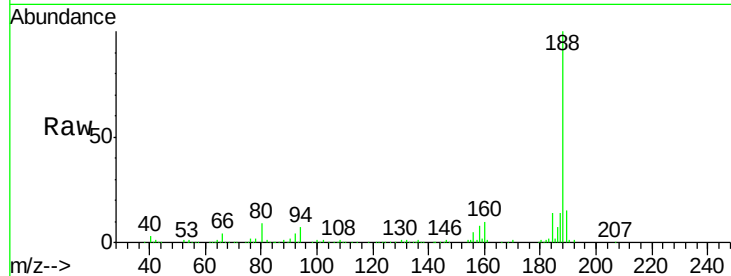

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.80 min Scan# 3185
 Delta R.T. -0.03 min
 Lab File: BG040050.D
 Acq: 21 Mar 2019 00:26

Tgt Ion:240 Resp: 278180
 Ion Ratio Lower Upper
 240 100
 120 8.9 7.0 10.6
 236 25.5 21.0 31.4

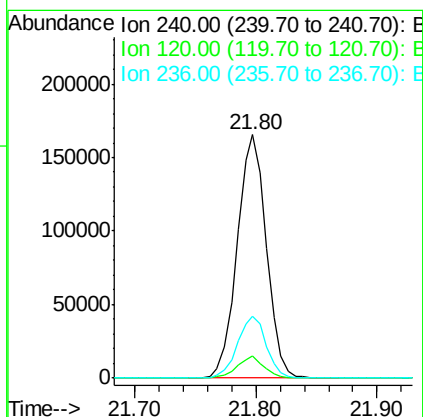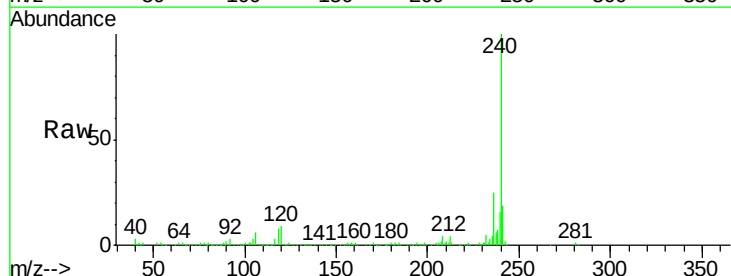

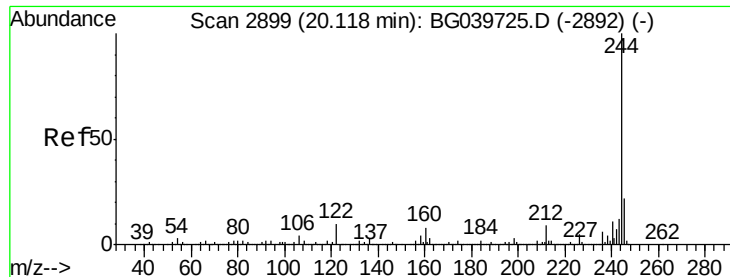

#79

Terphenyl-d14

Concen: 73.371 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26

Instrument :

BNA_G

ClientSampleId :

20190084-FIELD-DUPLICATE


Tgt Ion:244 Resp: 926982

Ion Ratio Lower Upper

244 100

212 8.7 7.3 10.9




122 9.0 8.4 12.6

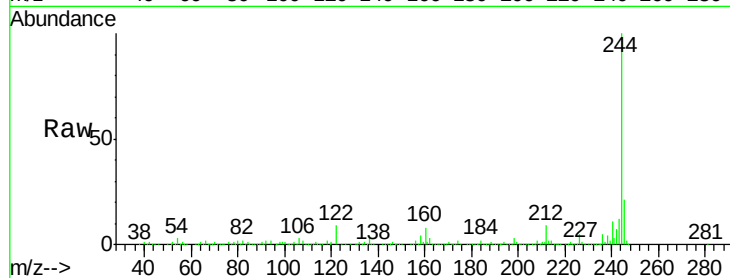

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

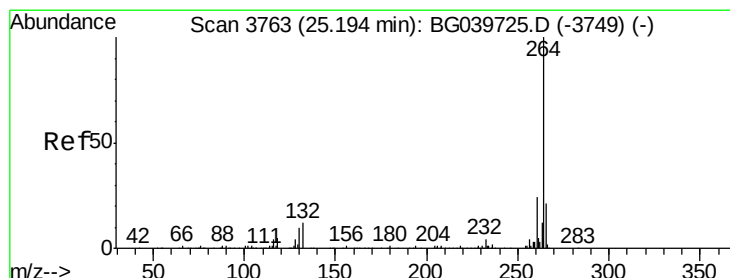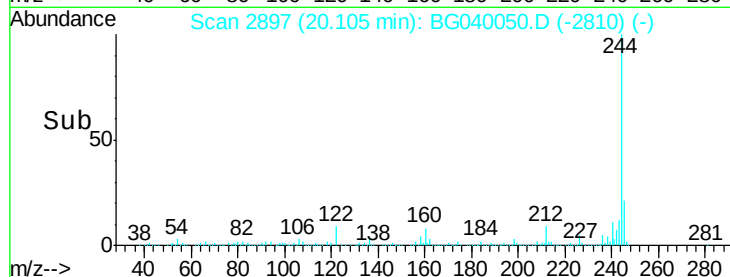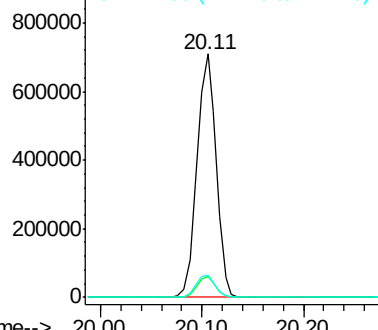

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.16 min Scan# 3757

Delta R.T. -0.04 min

Lab File: BG040050.D

Acq: 21 Mar 2019 00:26


Tgt Ion:264 Resp: 279267

Ion Ratio Lower Upper

264 100

260 22.9 18.2 27.4

265 20.8 18.5 27.7

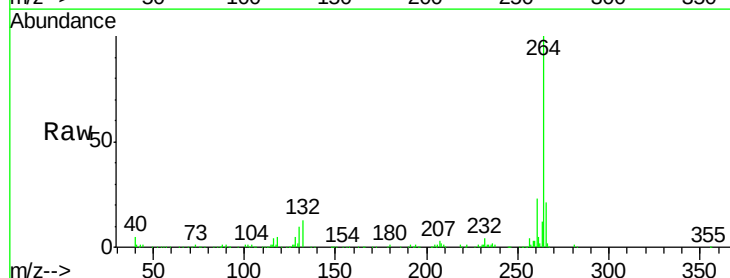

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

