


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG032019\
 Data File : BG040035.D
 Acq On : 20 Mar 2019 14:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

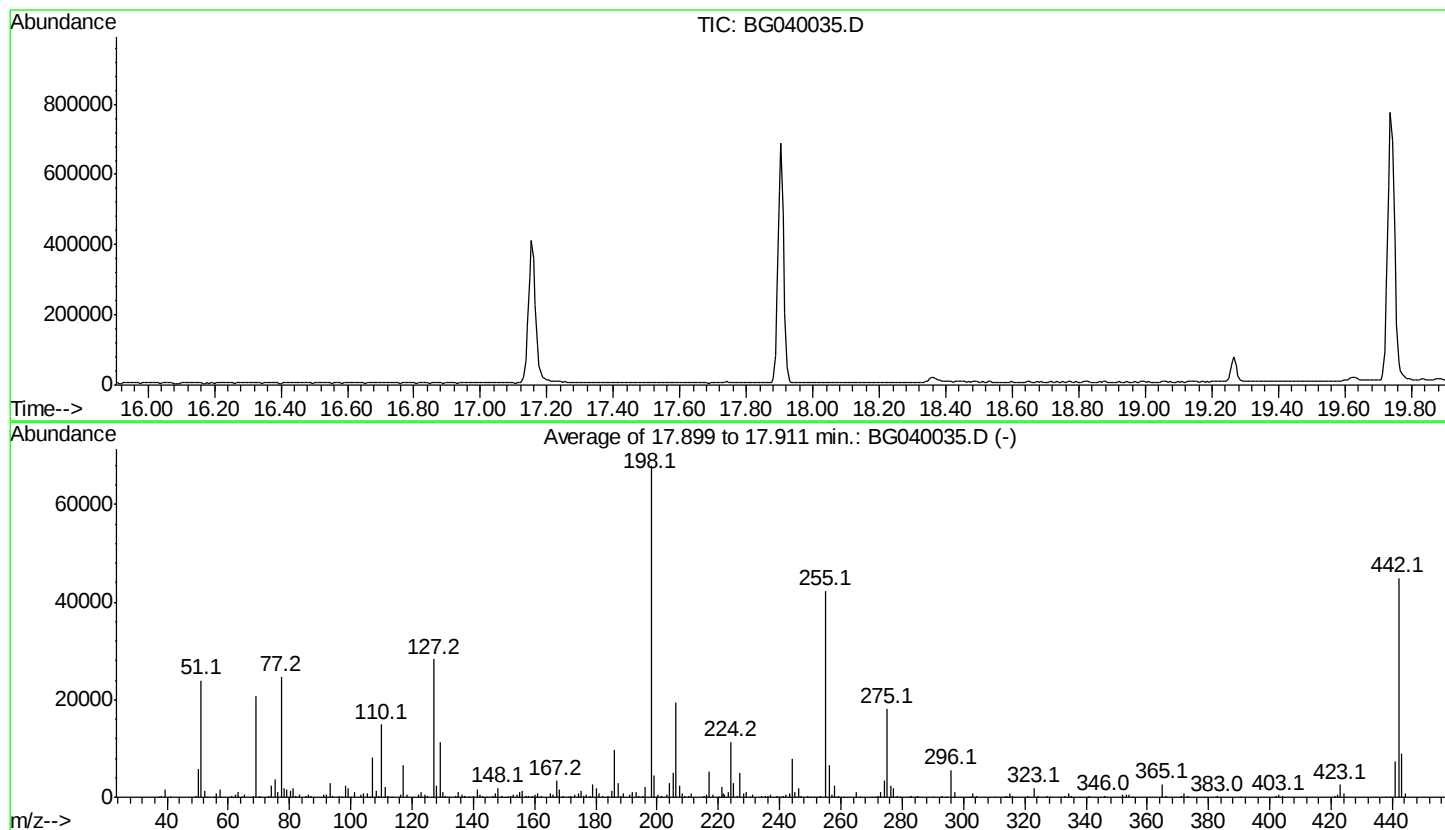

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	23885	PASS
68	69	0.00	2	1.5	308	PASS
69	198	0.00	100	30.5	20731	PASS
70	69	0.00	2	0.7	142	PASS
127	198	10	80	41.6	28264	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67941	PASS
199	198	5	9	6.6	4482	PASS
275	198	10	60	26.8	18205	PASS
365	198	1	100	3.9	2650	PASS
441	198	0.01	100	10.6	7224	PASS
442	198	50	100	66.1	44914	PASS
443	442	15	24	19.9	8935	PASS