


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032019\
 Data File : BG040054.D
 Acq On : 21 Mar 2019 4:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

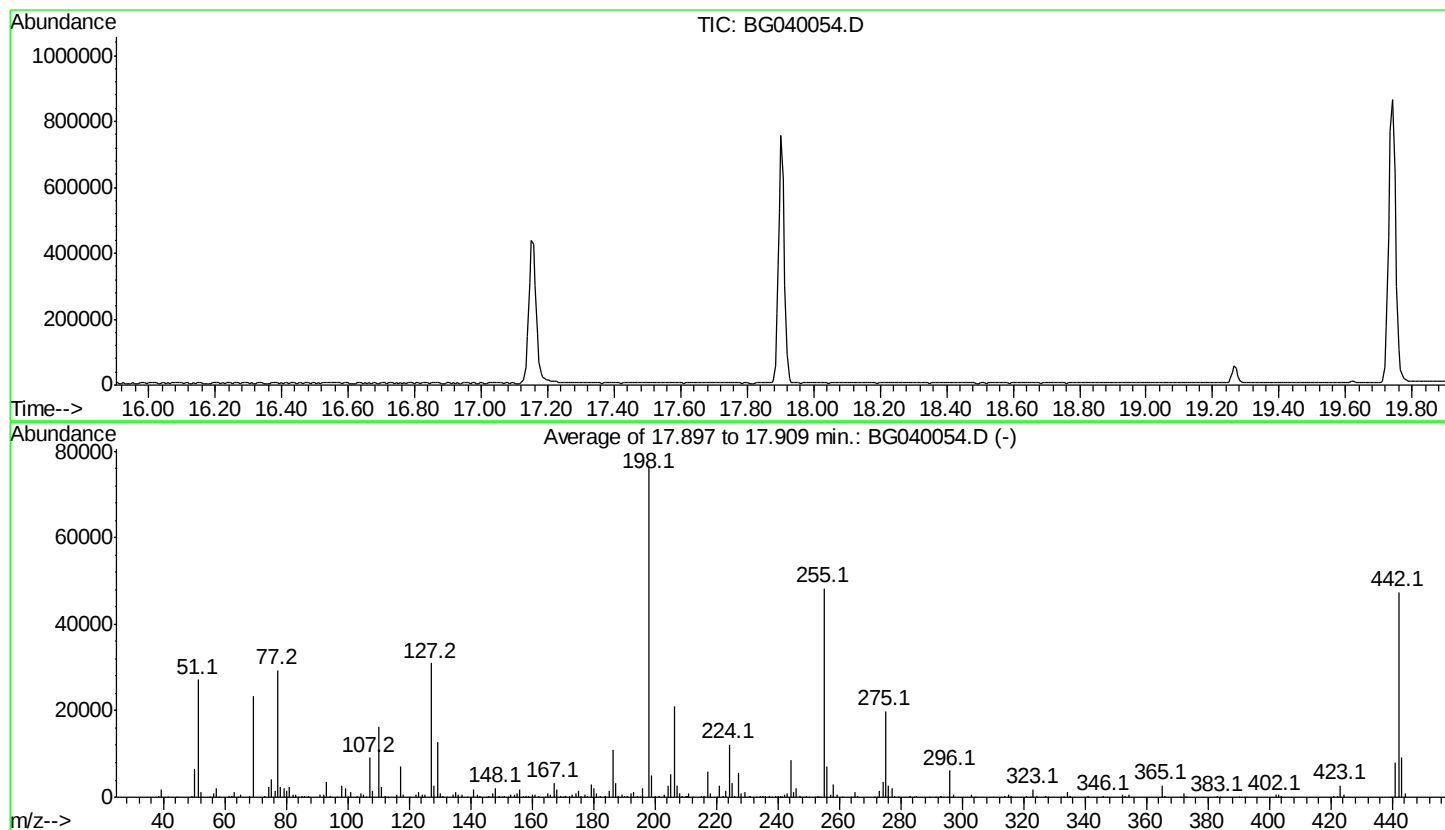

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	27197	PASS
68	69	0.00	2	0.9	200	PASS
69	198	0.00	100	30.7	23522	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.5	31016	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76674	PASS
199	198	5	9	6.5	4970	PASS
275	198	10	60	25.9	19850	PASS
365	198	1	100	3.5	2687	PASS
441	198	0.01	100	10.4	7956	PASS
442	198	50	100	61.8	47416	PASS
443	442	15	24	19.5	9268	PASS