
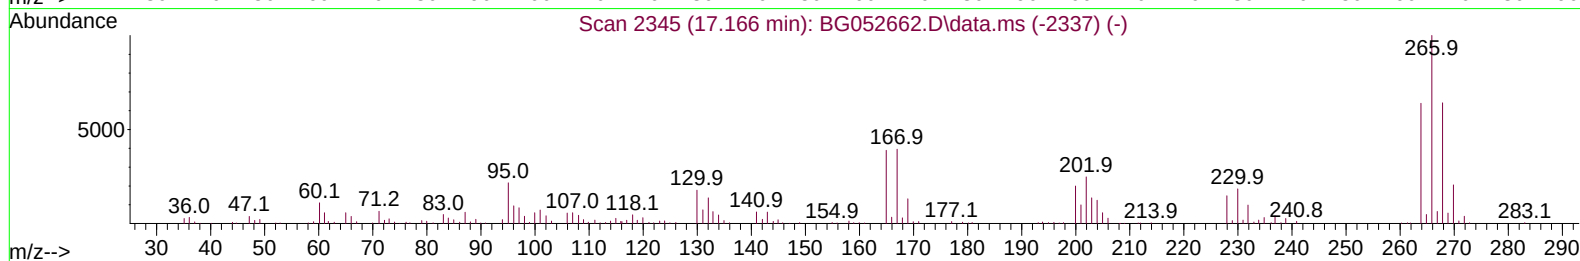
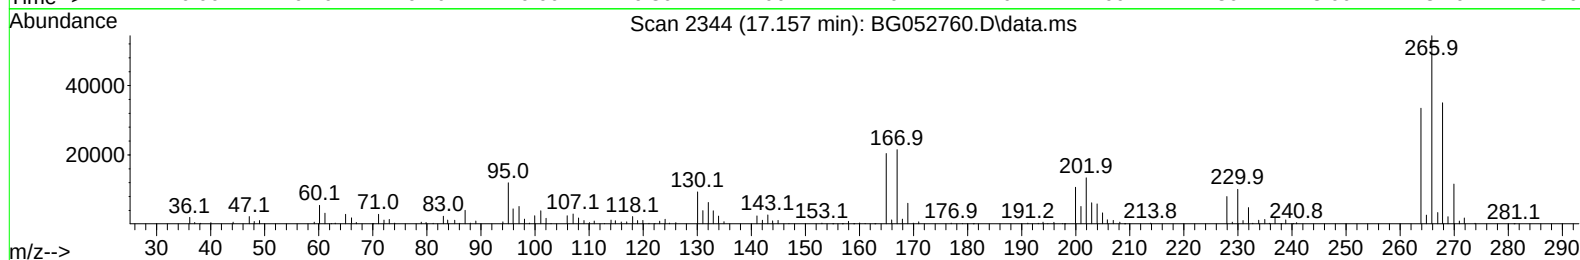


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\
Data File : BG052760.D
Acq On : 21 Mar 2022 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 13:32:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration

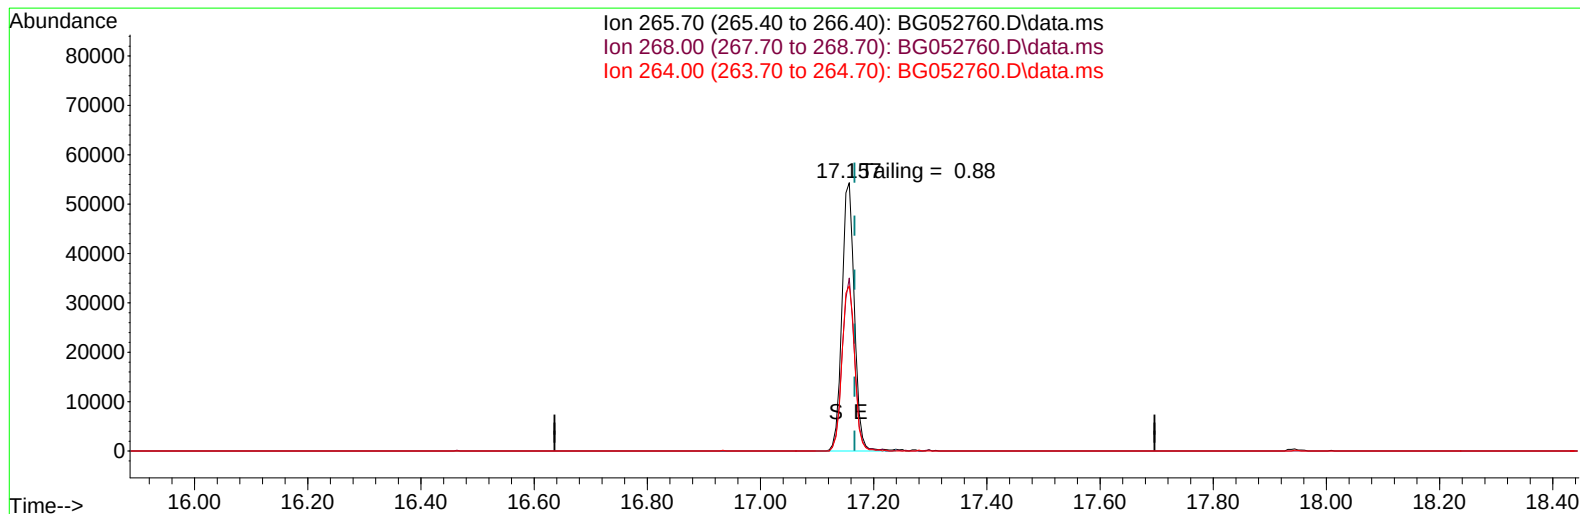

TIC: BG052760.D\data.ms

(70) Pentachlorophenol (C)




17.157min (-0.009) 193625.10 ng

response 82503

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.44
264.00	56.60	61.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\
Data File : BG052760.D
Acq On : 21 Mar 2022 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 13:32:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration

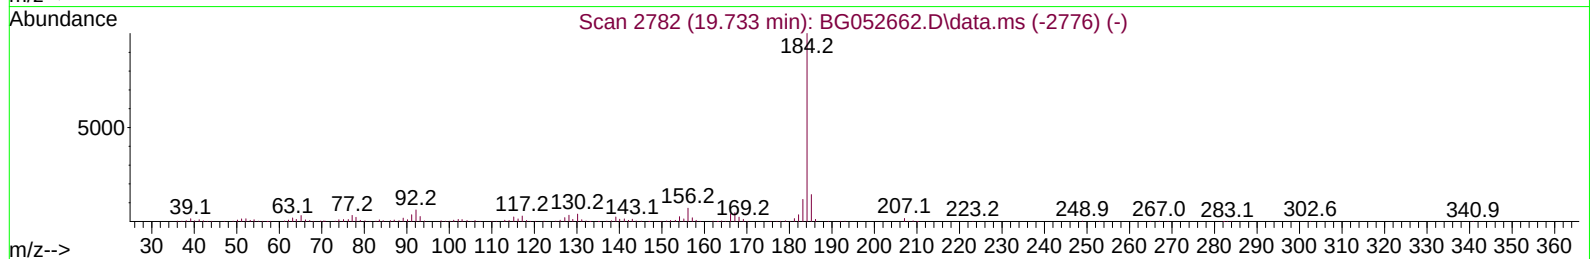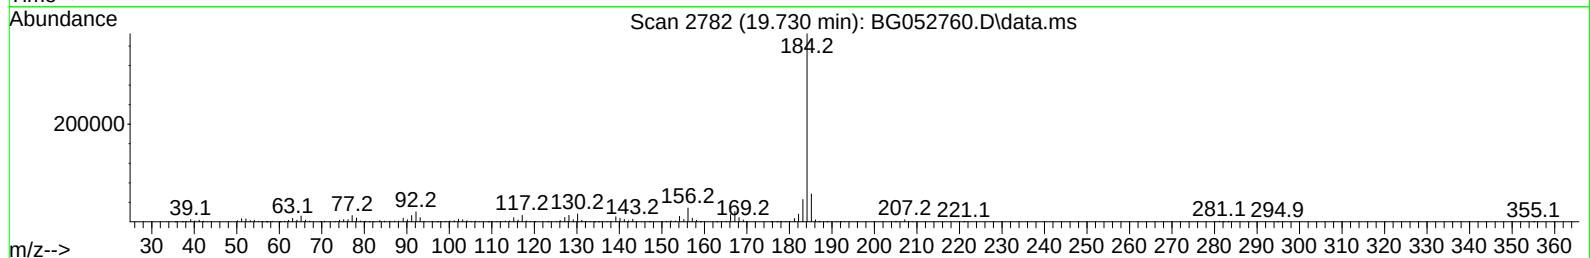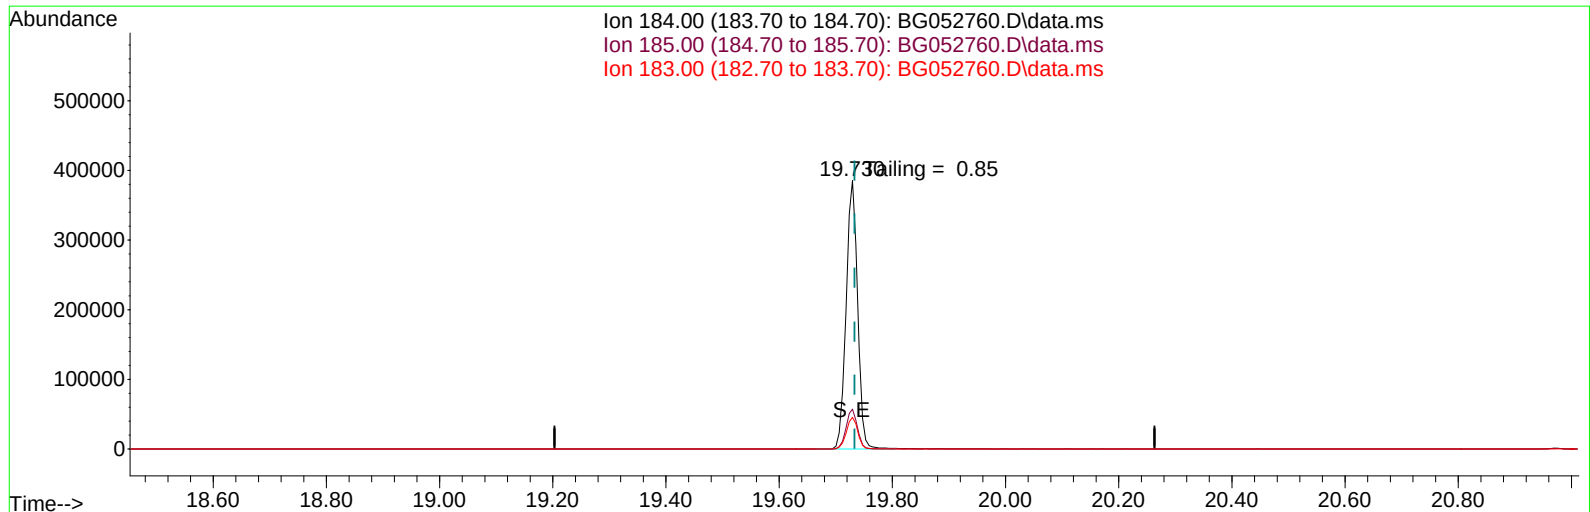

TIC: BG052760.D\data.ms

(77) Benzidine

19.730min (-0.003) 351250.33 ng

response 543567

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.85
183.00	11.80	11.86
0.00	0.00	0.00