

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\
 Data File : BG052773.D
 Acq On : 21 Mar 2022 18:28
 Operator : CG/JU
 Sample : N2007-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP3

Quant Time: Mar 22 02:54:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.146	152	53020	20.000	ng	-0.01
21) Naphthalene-d8	10.959	136	211549	20.000	ng	#-0.01
39) Acenaphthene-d10	14.766	164	144625	20.000	ng	0.00
64) Phenanthrene-d10	17.509	188	304204	20.000	ng	0.00
76) Chrysene-d12	21.798	240	291325	20.000	ng	-0.01
86) Perylene-d12	25.117	264	303149	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.702	112	286714	94.175	ng	0.00
7) Phenol-d6	7.294	99	425203	92.639	ng	0.00
23) Nitrobenzene-d5	9.303	82	295400	70.084	ng	-0.01
42) 2,4,6-Tribromophenol	16.246	330	184049	94.706	ng	-0.01
45) 2-Fluorobiphenyl	13.391	172	636782	64.937	ng	-0.01
79) Terphenyl-d14	20.112	244	954410	58.277	ng	-0.01
Target Compounds						
						Qvalue
75) Fluoranthene	19.554	202	50682	2.453	ng	98
78) Pyrene	19.912	202	50086	2.478	ng	96
84) Bis(2-ethylhexyl)phtha...	21.680	149	23689	2.430	ng	# 91
88) Benzo(b)fluoranthene	24.054	252	42461	2.256	ng	# 89
92) Benzo(g,h,i)perylene	30.075	276	40815	2.413	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\
Data File : BG052773.D
Acq On : 21 Mar 2022 18:28
Operator : CG/JU
Sample : N2007-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP3

Quant Time: Mar 22 02:54:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration




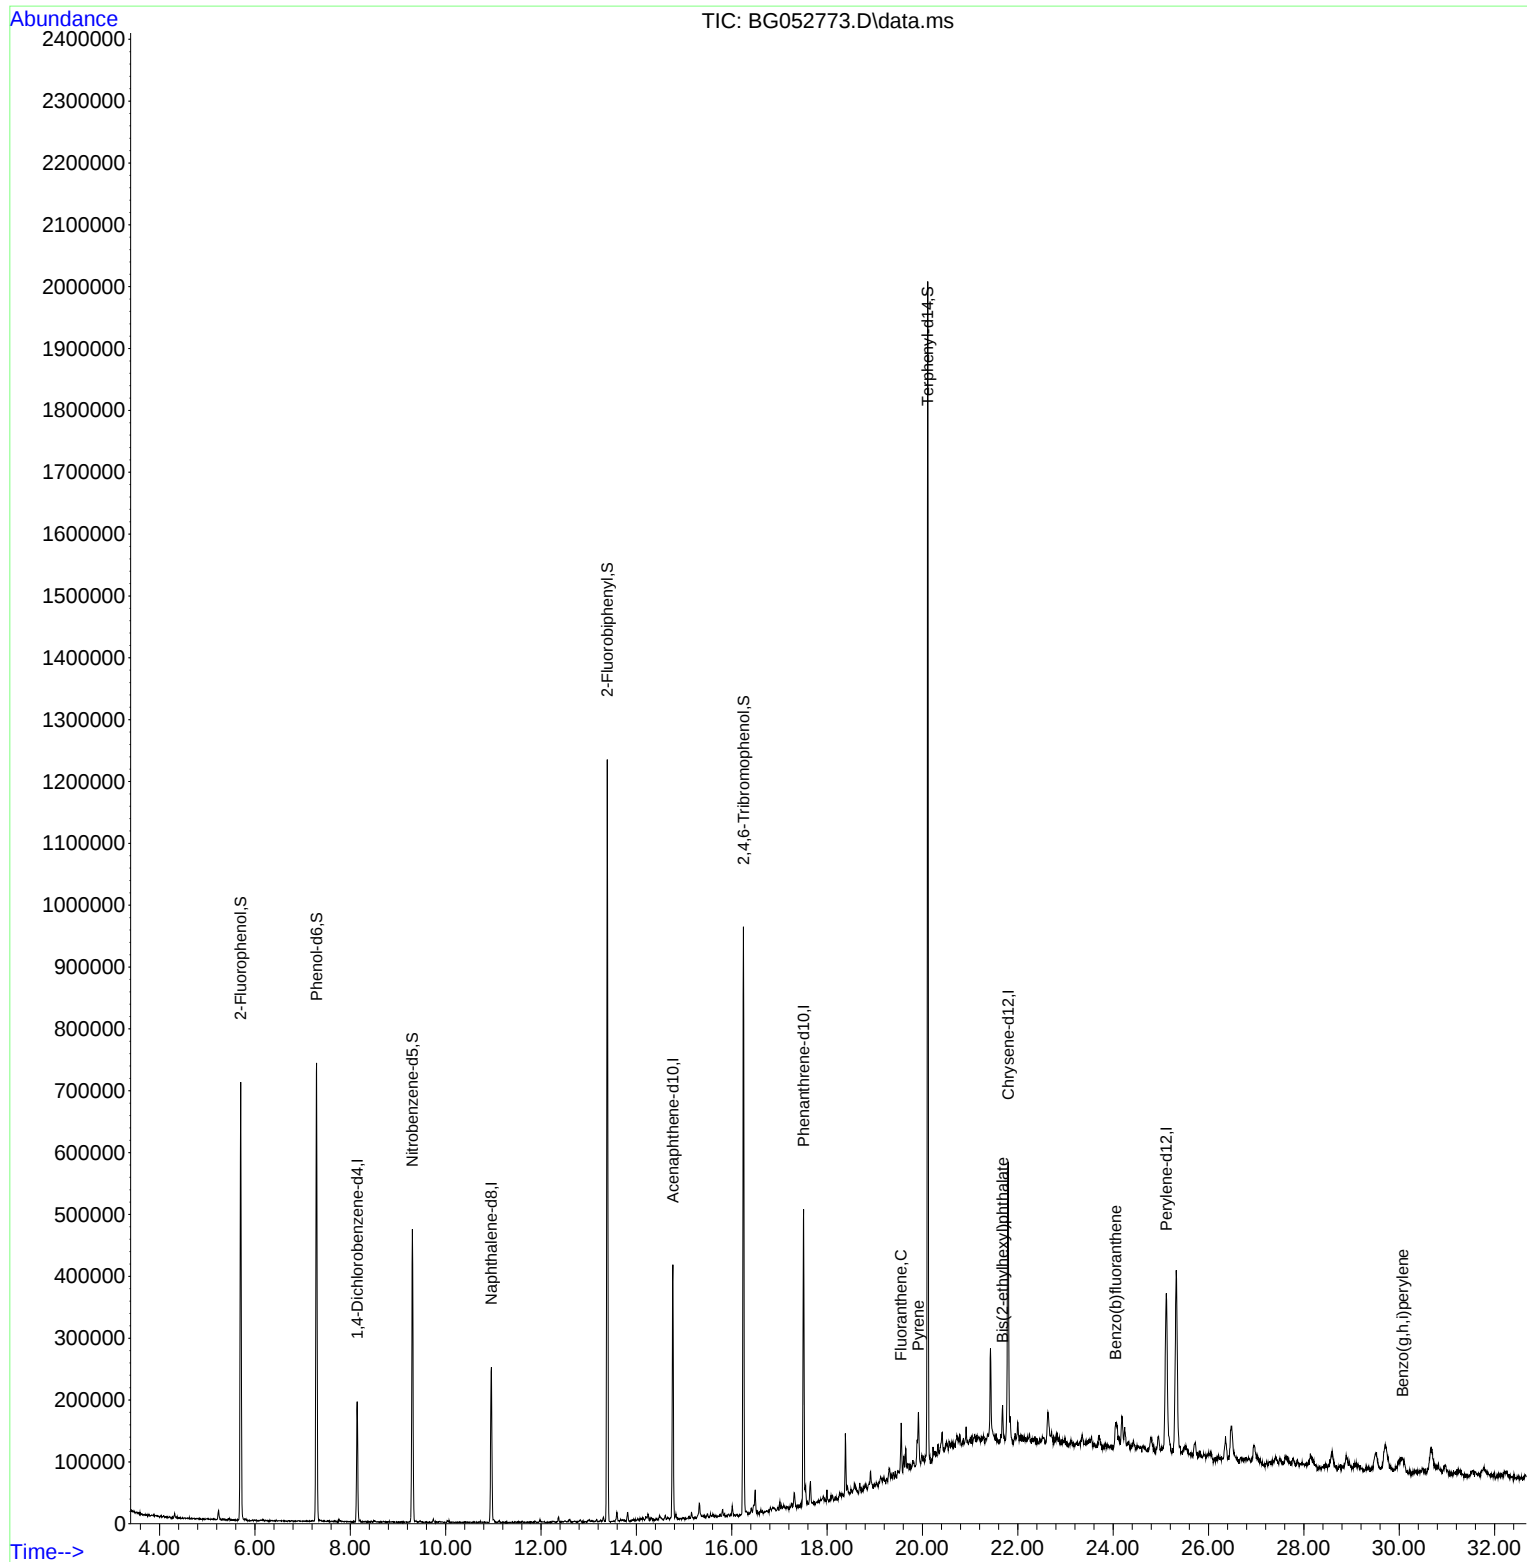




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.146 min Scan# 812
Delta R.T. -0.014 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28




Instrument :
BNA_G
ClientSampleId :
SP3


Tgt Ion:152 Resp: 53020
Ion Ratio Lower Upper
152 100
150 162.5 114.6 172.0
115 59.6 45.9 68.9

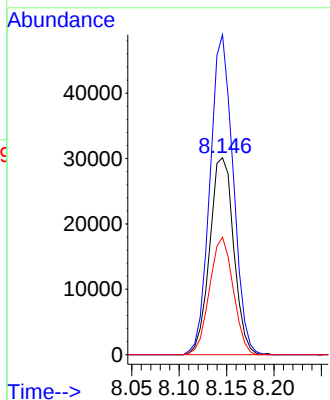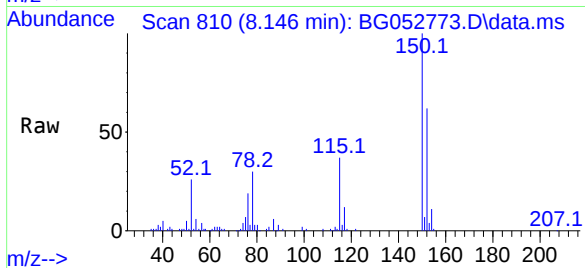

#5
2-Fluorophenol
Concen: 94.175 ng
RT: 5.702 min Scan# 394
Delta R.T. -0.009 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28

Tgt Ion:112 Resp: 286714
Ion Ratio Lower Upper
112 100
64 70.7 48.0 72.0
63 39.1 26.5 39.7


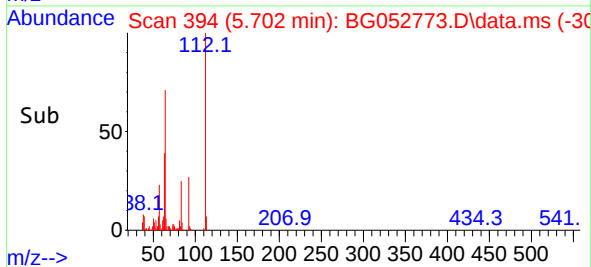
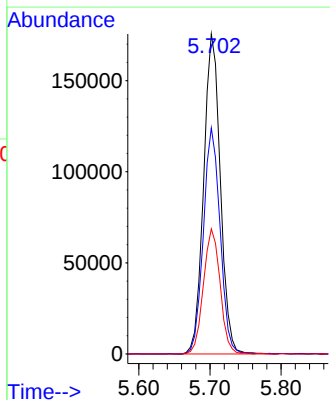
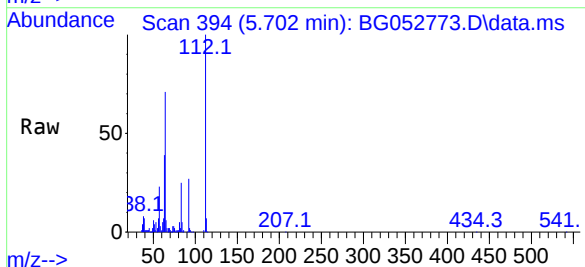




#7
Phenol-d6
Concen: 92.639 ng
RT: 7.294 min Scan# 61
Delta R.T. -0.003 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28




Instrument :
BNA_G
ClientSampleId :
SP3


Tgt Ion: 99 Resp: 425203
Ion Ratio Lower Upper
99 100
42 19.5 14.7 22.1
71 39.1 29.2 43.8

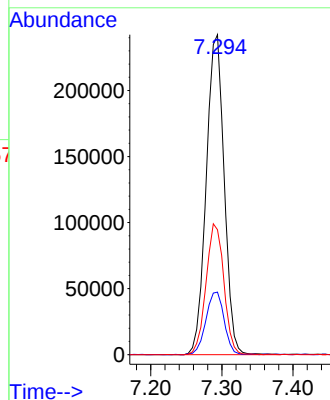

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.959 min Scan# 1289
Delta R.T. -0.015 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28

Tgt Ion:136 Resp: 211549
Ion Ratio Lower Upper
136 100
137 12.2 9.4 14.2
54 9.7 6.4 9.6#
68 7.2 5.0 7.6

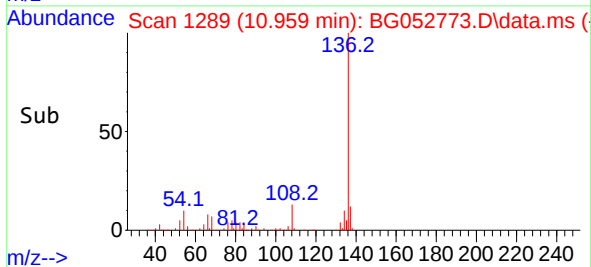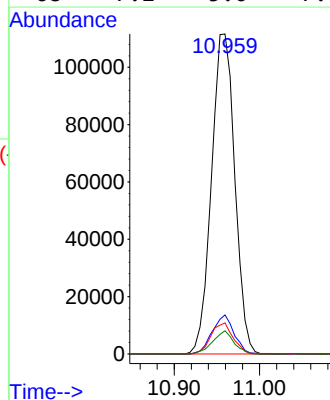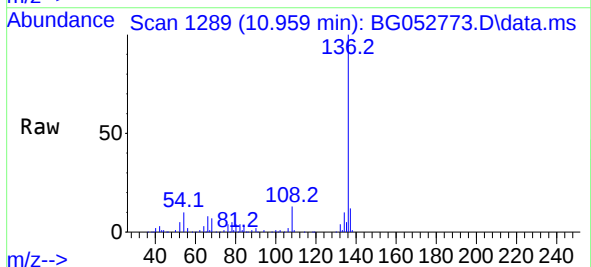

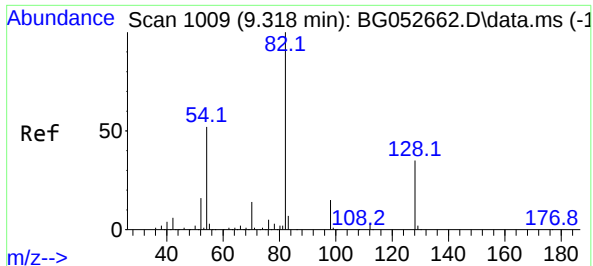

#23

Nitrobenzene-d5

Concen: 70.084 ng

RT: 9.303 min Scan# 1009

Delta R.T. -0.015 min

Lab File: BG052773.D

Acq: 21 Mar 2022 18:28

Instrument :

BNA_G

ClientSampleId :

SP3





Tgt Ion: 82 Resp: 295400

Ion Ratio Lower Upper

82 100

128 35.6 31.3 46.9

54 51.3 37.8 56.8

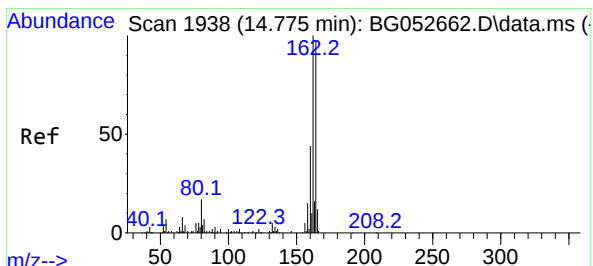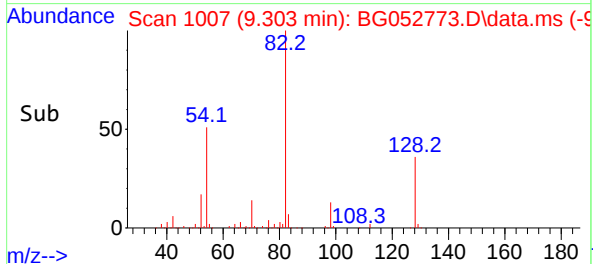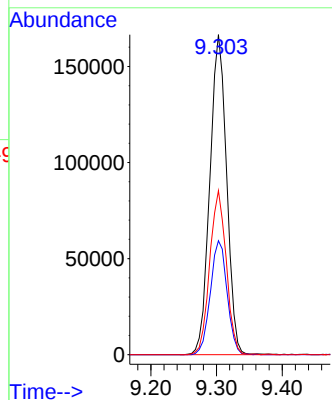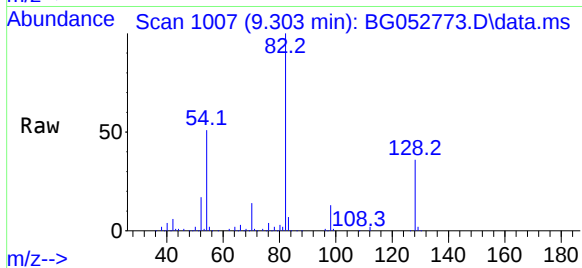

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.766 min Scan# 1937

Delta R.T. -0.009 min

Lab File: BG052773.D

Acq: 21 Mar 2022 18:28




Tgt Ion:164 Resp: 144625


Ion Ratio Lower Upper

164 100

162 103.5 80.0 120.0

160 43.0 38.8 58.2


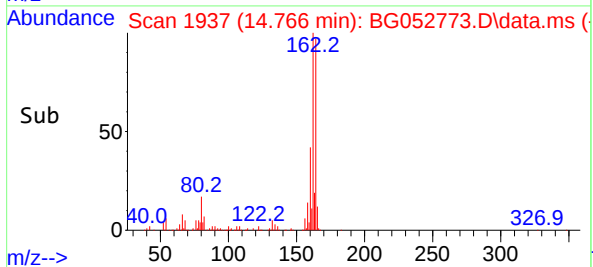
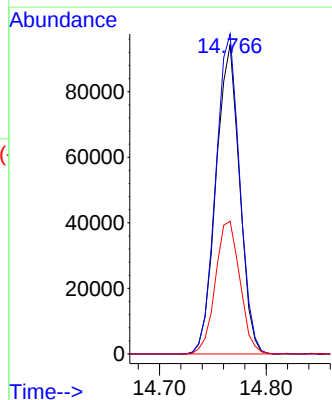
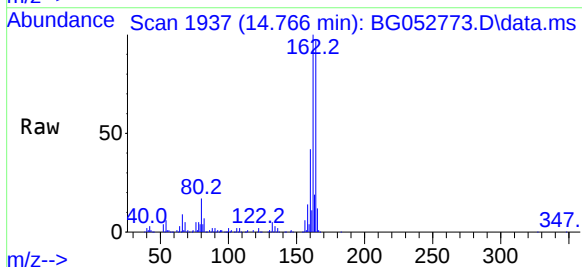




#42
2,4,6-Tribromophenol
Concen: 94.706 ng
RT: 16.246 min Scan# 2191
Delta R.T. -0.015 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28




Instrument :
BNA_G
ClientSampleId :
SP3


Tgt Ion:330 Resp: 184049
Ion Ratio Lower Upper
330 100
332 97.4 75.8 113.6
141 34.4 24.6 36.8

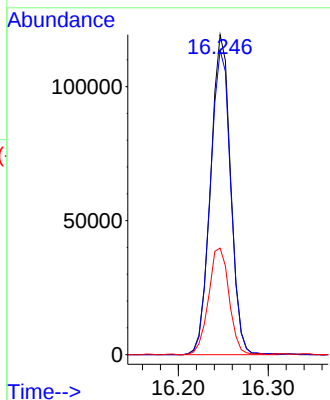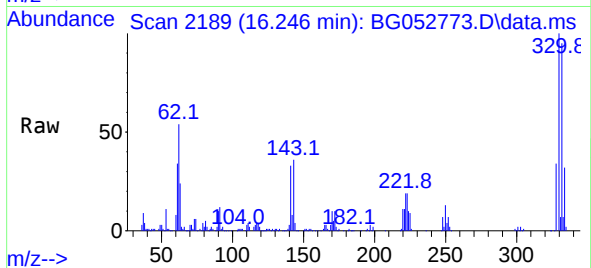

#45
2-Fluorobiphenyl
Concen: 64.937 ng
RT: 13.391 min Scan# 1703
Delta R.T. -0.015 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28

Tgt Ion:172 Resp: 636782
Ion Ratio Lower Upper
172 100
171 35.1 28.3 42.5
170 23.1 18.0 27.0


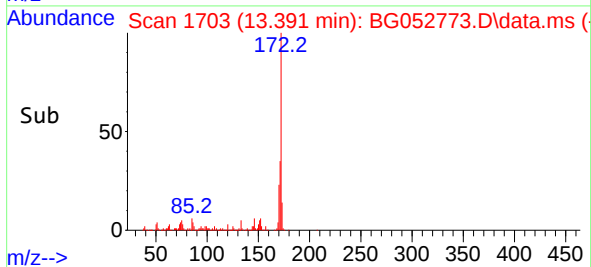
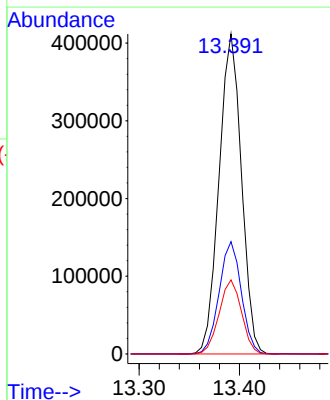
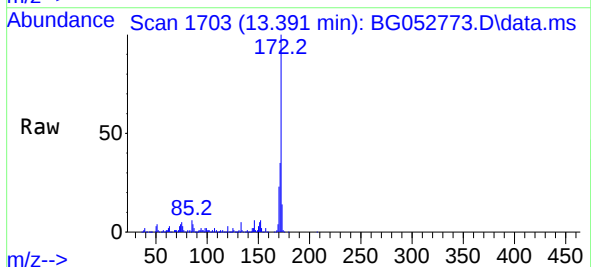




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.509 min Scan# 24
Delta R.T. -0.009 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28




Instrument :
BNA_G
ClientSampleId :
SP3


Tgt Ion:188 Resp: 304204
Ion Ratio Lower Upper
188 100
94 7.2 5.7 8.5
80 9.1 7.2 10.8

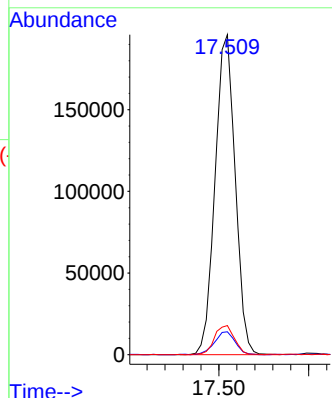

#75
Fluoranthene
Concen: 2.453 ng
RT: 19.554 min Scan# 2752
Delta R.T. -0.015 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28

Tgt Ion:202 Resp: 50682
Ion Ratio Lower Upper
202 100
101 6.9 0.0 27.3
203 18.9 0.0 37.7


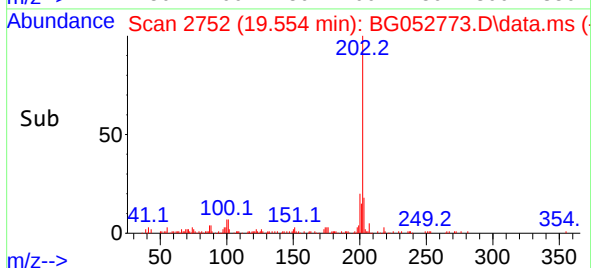
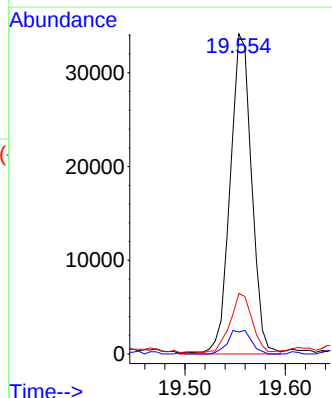





#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.798 min Scan# 31
Delta R.T. -0.015 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28




Instrument :
BNA_G
ClientSampleId :
SP3


Tgt Ion:240 Resp: 291325
Ion Ratio Lower Upper
240 100
120 6.8 5.4 8.0
236 25.2 19.8 29.6

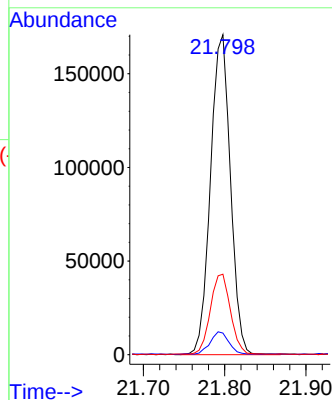

#78
Pyrene
Concen: 2.478 ng
RT: 19.912 min Scan# 2813
Delta R.T. -0.015 min
Lab File: BG052773.D
Acq: 21 Mar 2022 18:28

Tgt Ion:202 Resp: 50086
Ion Ratio Lower Upper
202 100
200 22.6 17.0 25.6
203 16.2 15.0 22.6


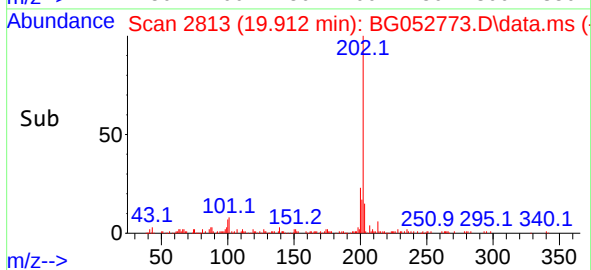
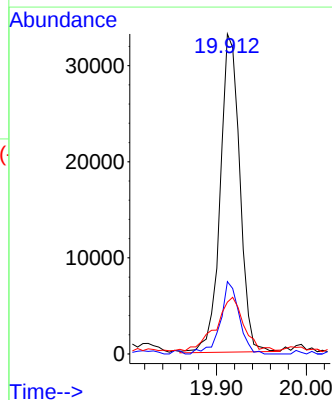





#79
 Terphenyl-d14
 Concen: 58.277 ng
 RT: 20.112 min Scan# 21
 Delta R.T. -0.015 min
 Lab File: BG052773.D
 Acq: 21 Mar 2022 18:28




Instrument :
 BNA_G
 ClientSampleId :
 SP3


Tgt Ion:244 Resp: 954410
 Ion Ratio Lower Upper
 244 100
 212 7.9 5.4 8.2
 122 6.5 5.8 8.6

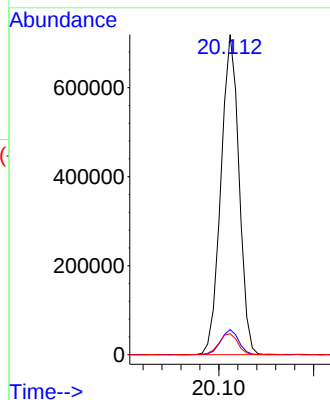

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.430 ng
 RT: 21.680 min Scan# 3114
 Delta R.T. -0.021 min
 Lab File: BG052773.D
 Acq: 21 Mar 2022 18:28

Tgt Ion:149 Resp: 23689
 Ion Ratio Lower Upper
 149 100
 167 31.7 21.4 32.2
 279 6.2 3.8 5.8#


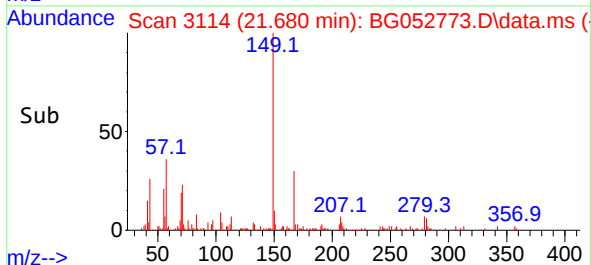
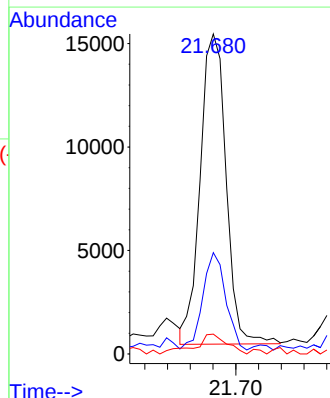
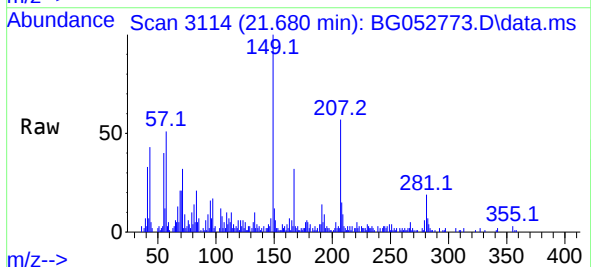




#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.117 min Scan# 30
 Delta R.T. -0.021 min
 Lab File: BG052773.D
 Acq: 21 Mar 2022 18:28




Instrument :
 BNA_G
 ClientSampleId :
 SP3


Tgt Ion:264 Resp: 303149
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.2 27.2
 265 22.6 15.1 22.7

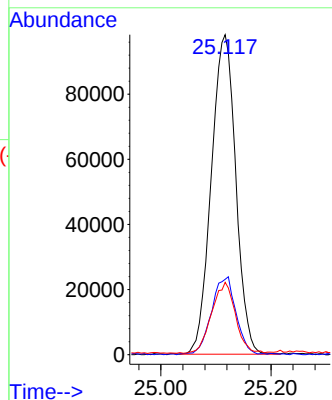

#88
 Benzo(b)fluoranthene
 Concen: 2.256 ng
 RT: 24.054 min Scan# 3518
 Delta R.T. -0.027 min
 Lab File: BG052773.D
 Acq: 21 Mar 2022 18:28


Tgt Ion:252 Resp: 42461
 Ion Ratio Lower Upper
 252 100
 253 27.2 17.2 25.8#
 125 8.3 5.2 7.8#

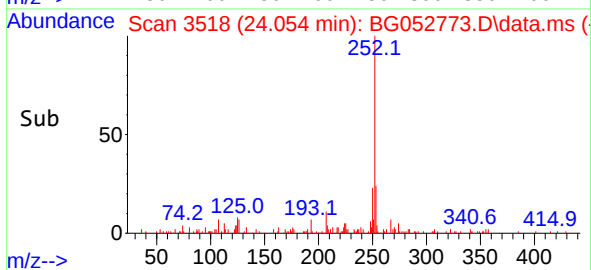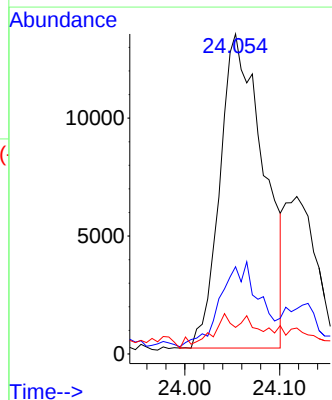



#92
 Benzo(g,h,i)perylene
 Concen: 2.413 ng
 RT: 30.075 min Scan# 4
 Delta R.T. -0.062 min
 Lab File: BG052773.D
 Acq: 21 Mar 2022 18:28

Instrument :
 BNA_G
 ClientSampleId :
 SP3

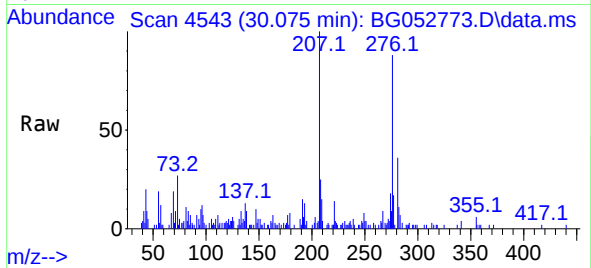

Tgt Ion:	276	Resp:	40815
Ion	Ratio	Lower	Upper
276	100		
277	19.8	18.2	27.2
138	10.8	9.1	13.7

