


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\
 Data File : BG052760.D
 Acq On : 21 Mar 2022 9:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 15 15:56:10 2022

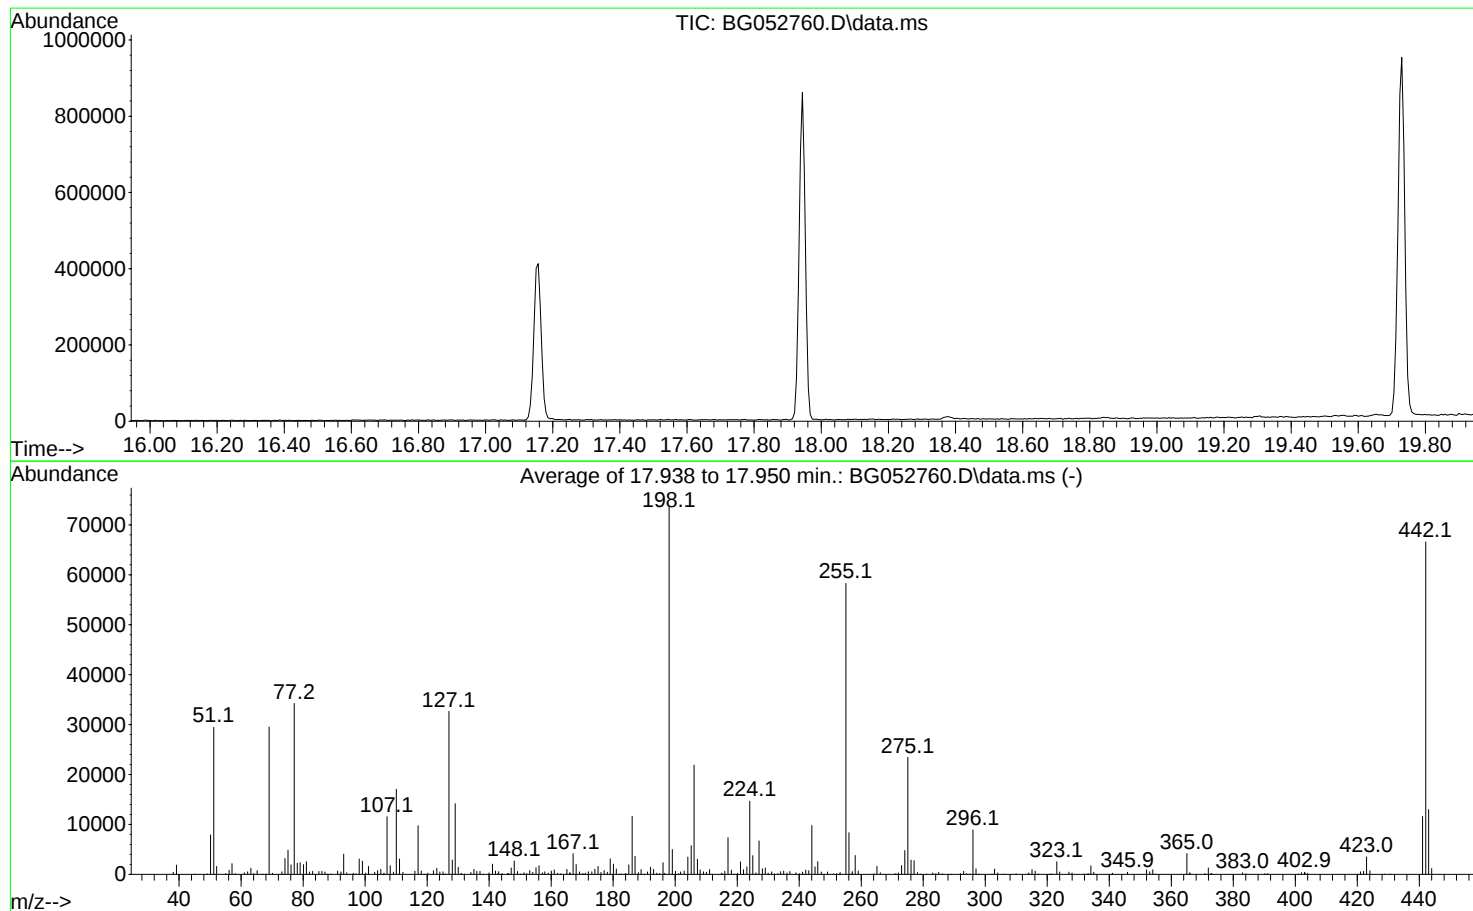

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	29469	PASS
68	69	0.00	2	0.4	110	PASS
69	198	0.00	100	40.1	29525	PASS
70	69	0.00	2	0.8	224	PASS
127	198	10	80	44.3	32659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73680	PASS
199	198	5	9	6.8	4985	PASS
275	198	10	60	31.8	23416	PASS
365	198	1	100	5.7	4182	PASS
441	198	0.01	100	15.8	11612	PASS
442	442	50	100	100.0	66611	PASS
443	442	15	24	19.5	12973	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/21/2022	BNA_G	<u>BG052760.D</u>
Compound Name	Response	Retention Time
DDT	245890	20.97
DDD	3741	20.51
DDE	96	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3837	249727	1.54

Instrument :
BNA_G
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\  
Data File : BG052760.D  
Acq On    : 21 Mar 2022    9:04  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 21 13:32:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration

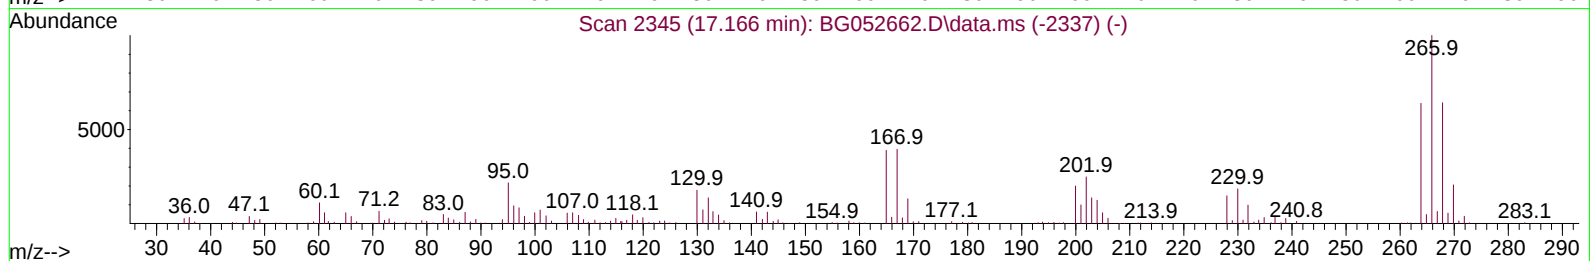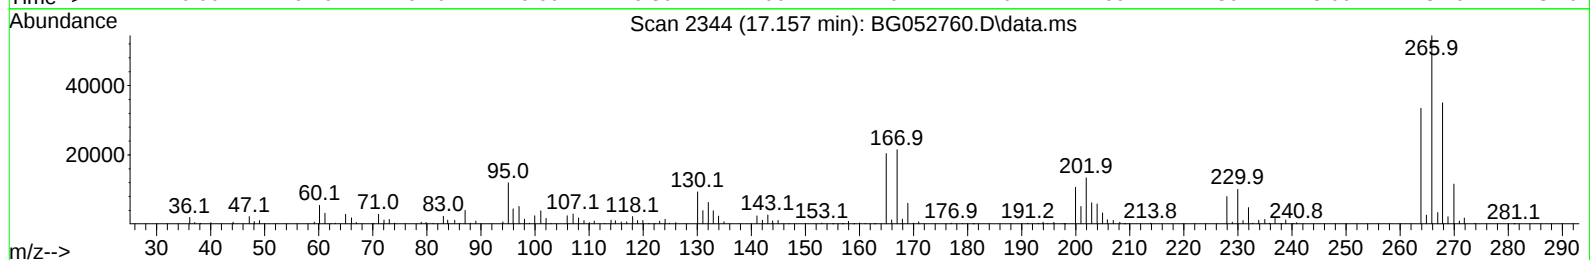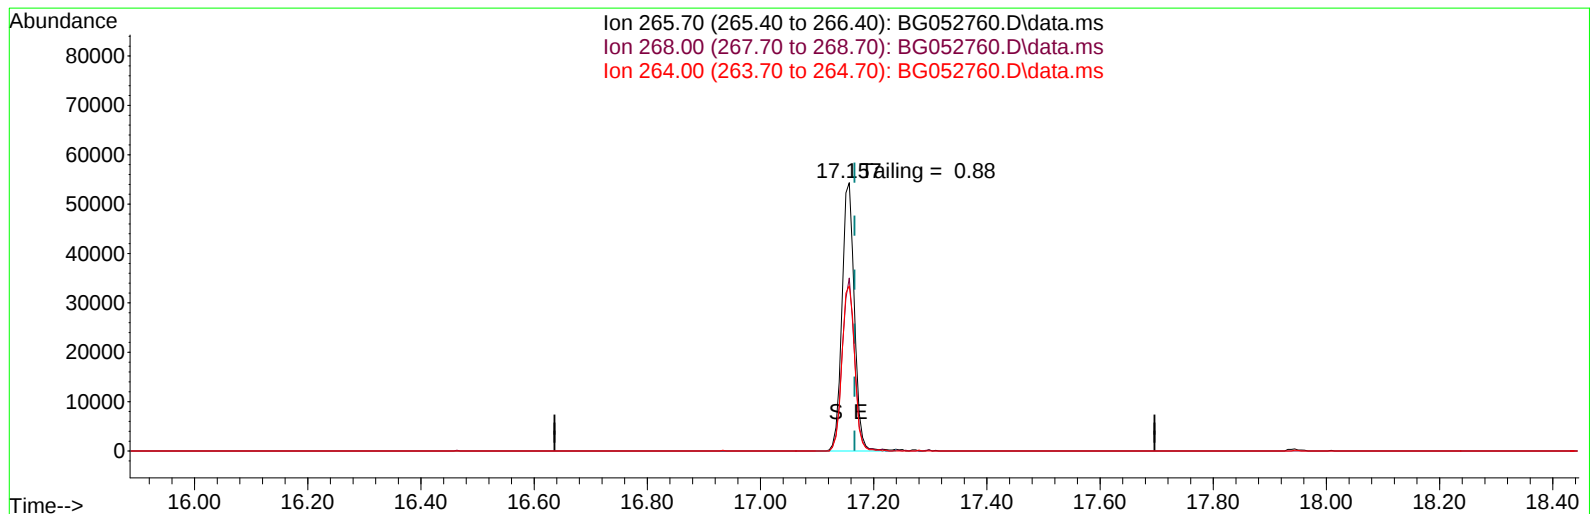

TIC: BG052760.D\data.ms

(70) Pentachlorophenol (C)

17.157min (-0.009) 193625.10 ng




response **82503**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.44
264.00	56.60	61.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032122\
 Data File : BG052760.D
 Acq On : 21 Mar 2022 9:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 21 13:32:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

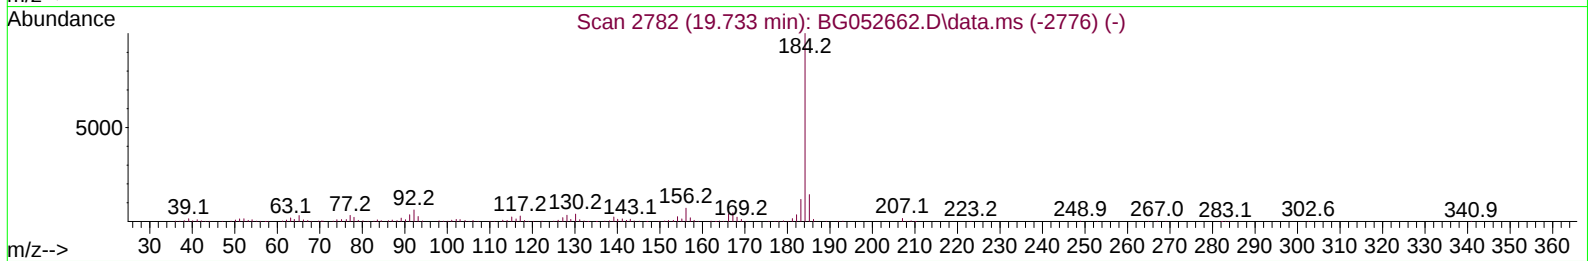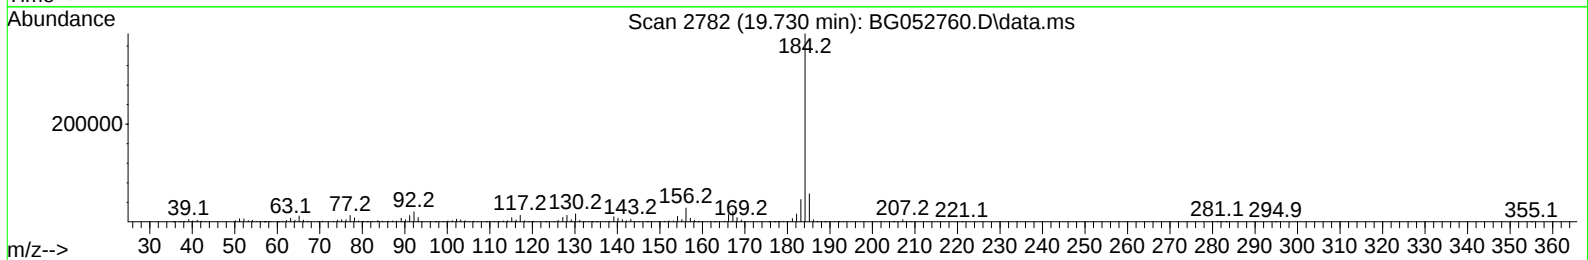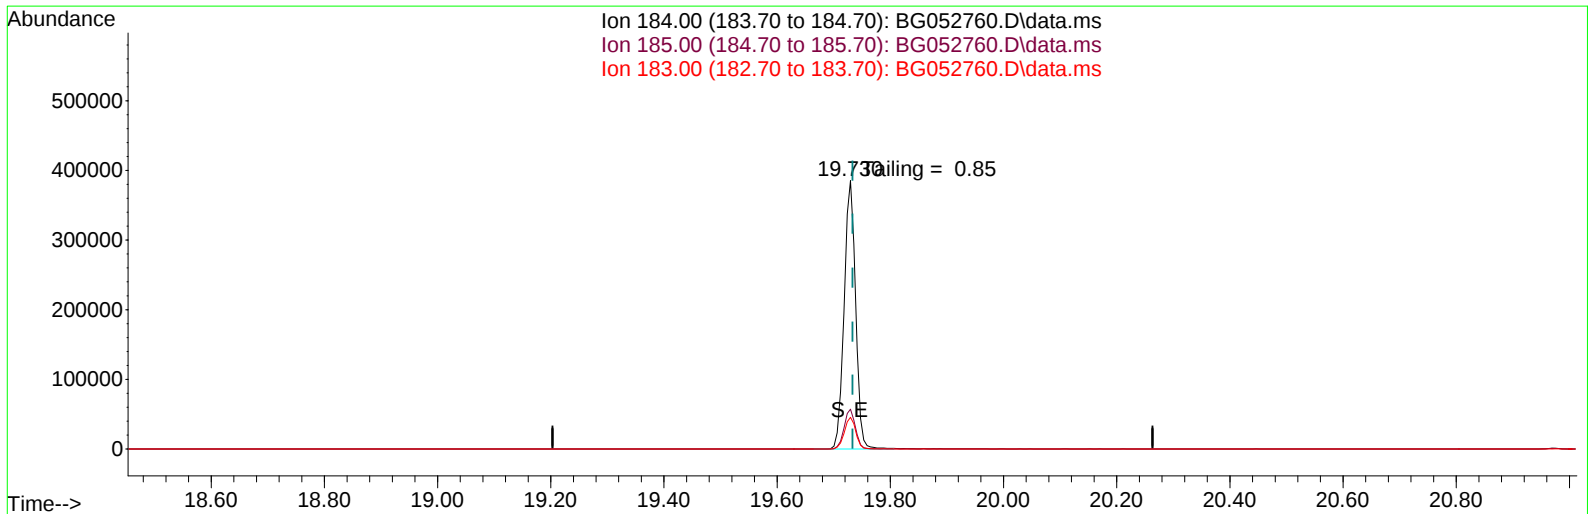

TIC: BG052760.D\data.ms

(77) Benzidine

19.730min (-0.003) 351250.33 ng

response 543567

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.85
183.00	11.80	11.86
0.00	0.00	0.00