

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032219\
 Data File : BG040107.D
 Acq On : 23 Mar 2019 8:13
 Operator : JU/SJ
 Sample : K2035-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 031919-LIFT-F-D-S

Quant Time: Mar 23 22:39:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	39040	20.00	ng	-0.03
21) Naphthalene-d8	10.96	136	169978	20.00	ng	-0.03
39) Acenaphthene-d10	14.77	164	117728	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	288549	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	281304	20.00	ng	-0.03
87) Perylene-d12	25.16	264	277551	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	94621	41.35	ng	-0.02
7) Phenol-d6	7.28	99	88780	26.02	ng	-0.03
23) Nitrobenzene-d5	9.32	82	276651	88.03	ng	-0.03
42) 2,4,6-Tribromophenol	16.25	330	124730	90.90	ng	-0.02
45) 2-Fluorobiphenyl	13.39	172	727345	87.97	ng	-0.03
79) Terphenyl-d14	20.11	244	992211	77.66	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032219\
Data File : BG040107.D
Acq On : 23 Mar 2019 8:13
Operator : JU/SJ
Sample : K2035-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
031919-LIFT-F-D-S

Quant Time: Mar 23 22:39:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

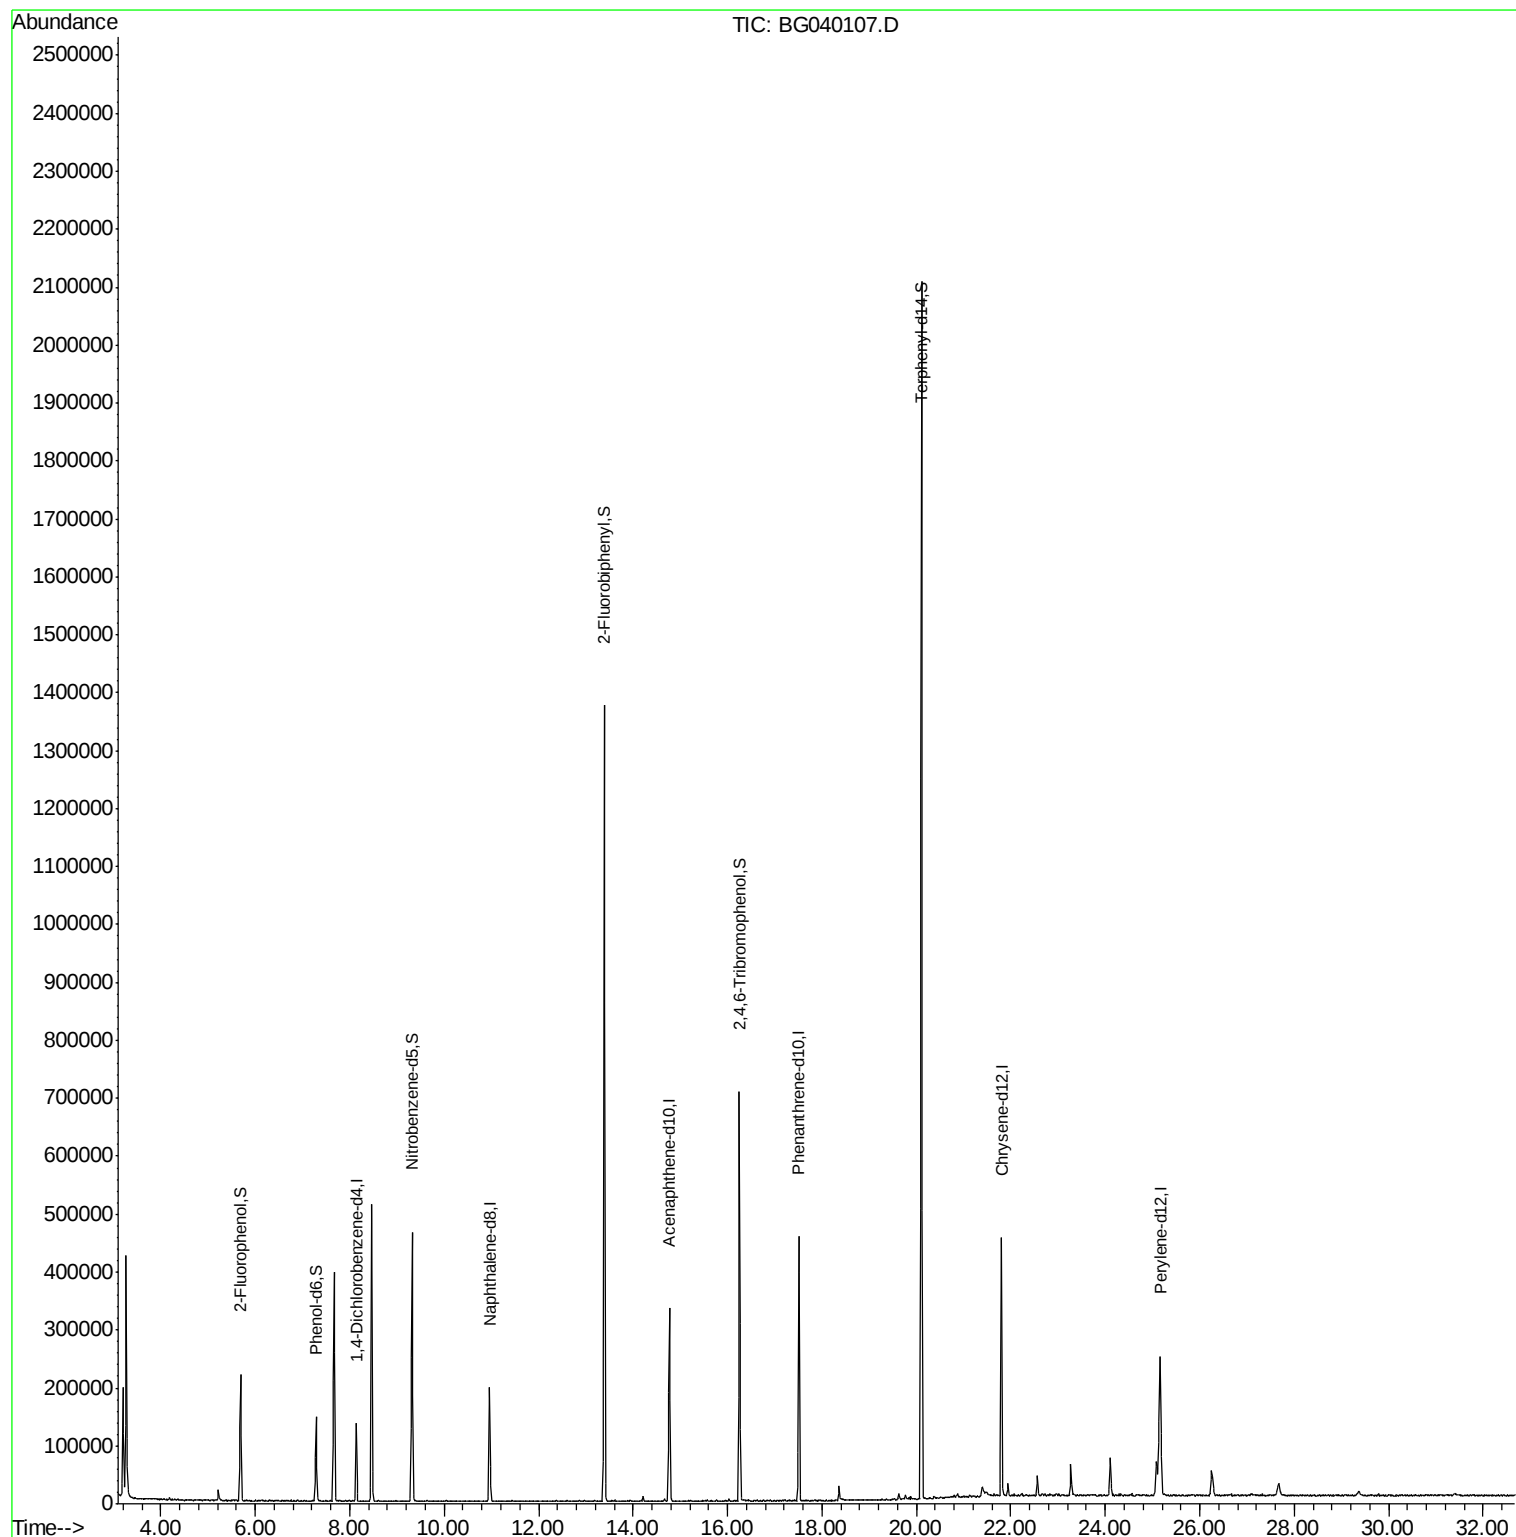




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 860
Delta R.T. -0.03 min
Lab File: BG040107.D
Acq: 23 Mar 2019 8:13

Instrument :
BNA_G
ClientSampleId :
031919-LIFT-F-D-S

Tot Ion:152 Resp: 39040
Ion Ratio Lower Upper
152 100
150 153.4 123.7 185.5
115 61.3 45.9 68.9

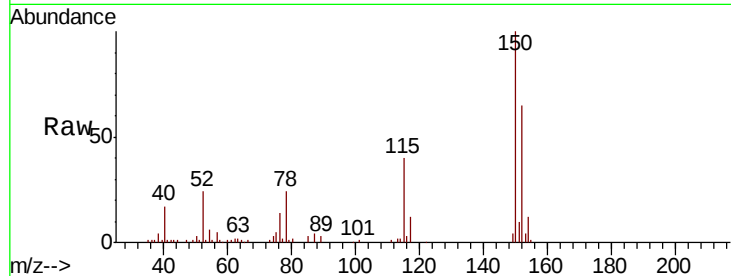


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

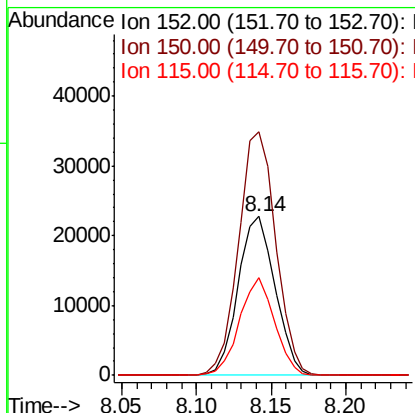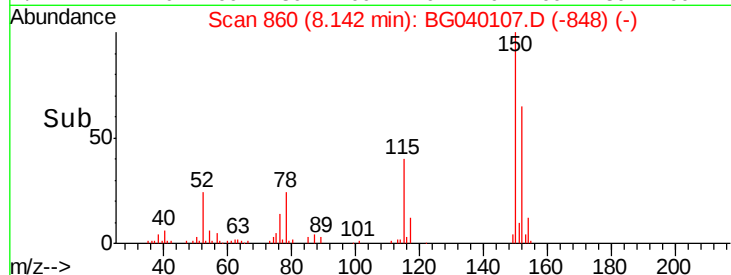



#5

2-Fluorophenol
Concen: 41.348 ng
RT: 5.69 min Scan# 442
Delta R.T. -0.02 min
Lab File: BG040107.D
Acq: 23 Mar 2019 8:13

Tgt Ion:112 Resp: 94621
Ion Ratio Lower Upper
112 100
64 70.1 57.8 86.8
63 36.2 29.8 44.6

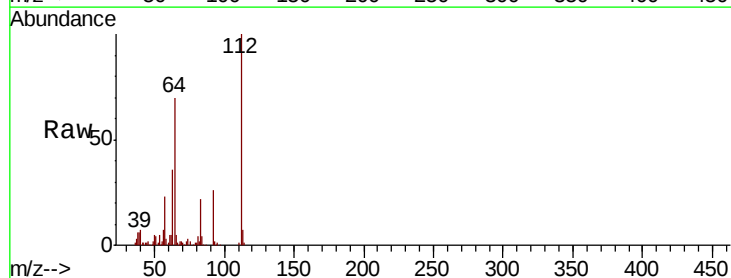

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

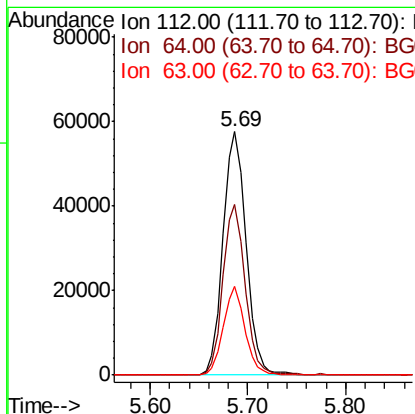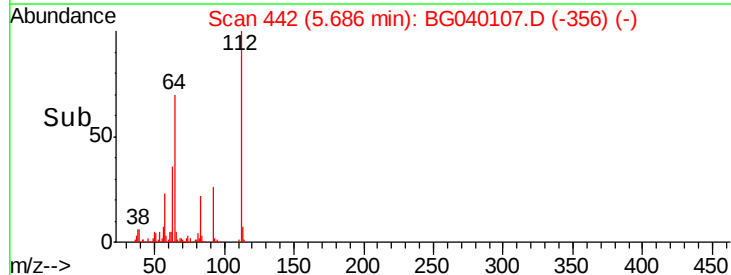



#7

Phenol-d6

Concen: 26.019 ng

RT: 7.28 min Scan# 714

Delta R.T. -0.03 min

Lab File: BG040107.D

Acq: 23 Mar 2019 8:13

Instrument :

BNA_G

ClientSampleId :

031919-LIFT-F-D-S


Tot Ion: 99 Resp: 88780

Ion Ratio Lower Upper



99 100

42 17.5 18.2 27.2#

71 34.7 28.0 42.0

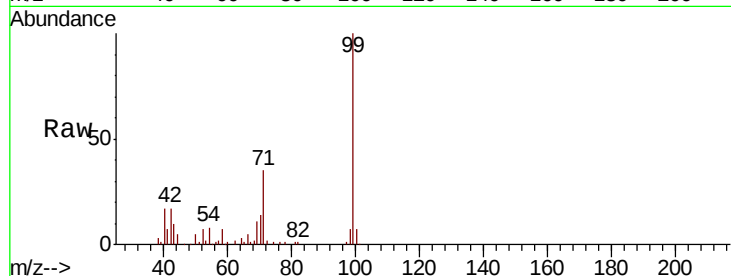

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

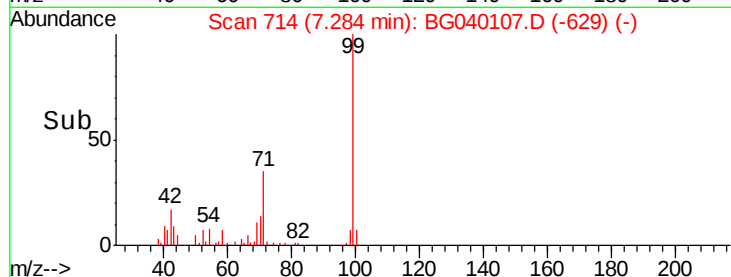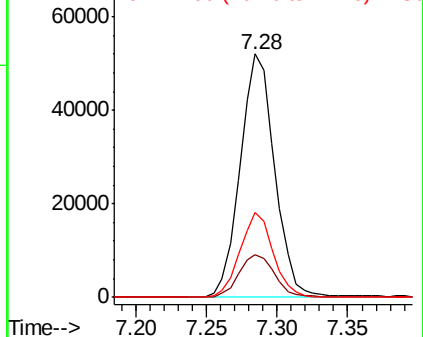

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.96 min Scan# 1340

Delta R.T. -0.03 min

Lab File: BG040107.D

Acq: 23 Mar 2019 8:13

Tgt Ion: 136 Resp: 169978


Ion Ratio Lower Upper

136 100



137 10.4 9.1 13.7


54 9.3 9.4 14.2#

68 6.4 4.2 6.4

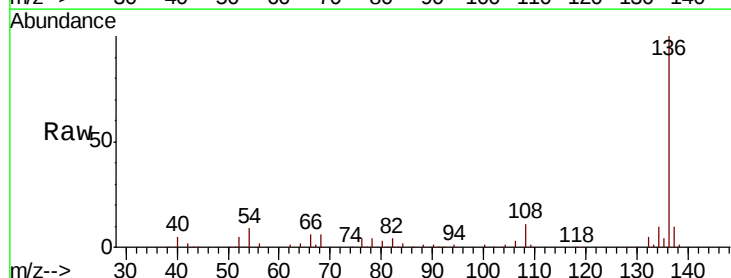

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



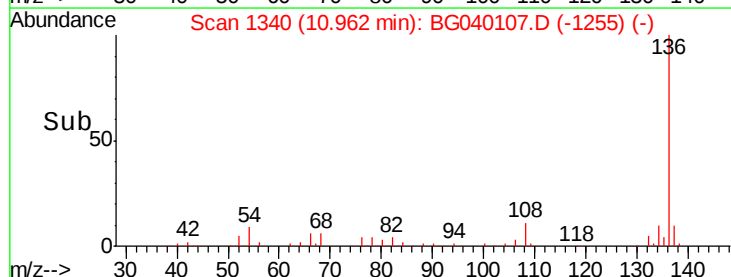
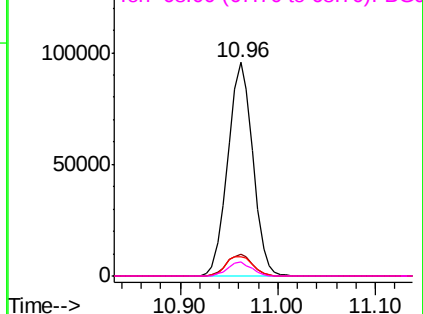


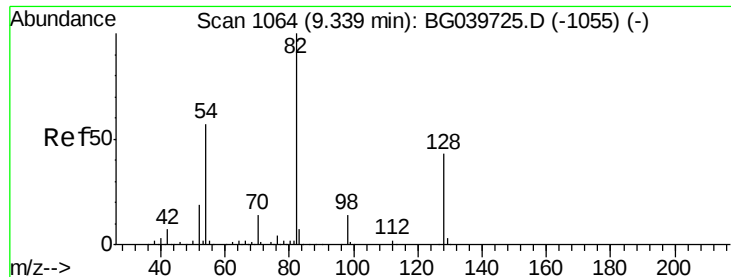

#23
Nitrobenzene-d5
Concen: 88.026 ng
RT: 9.32 min Scan# 1060
Delta R.T. -0.03 min
Lab File: BG040107.D
Acq: 23 Mar 2019 8:13




Instrument :
BNA_G
ClientSampleId :
031919-LIFT-F-D-S


Tot Ion	82	Resp	276651
Ion Ratio	Lower	Upper	
82	100		
128	43.4	31.3	46.9
54	55.9	50.9	76.3

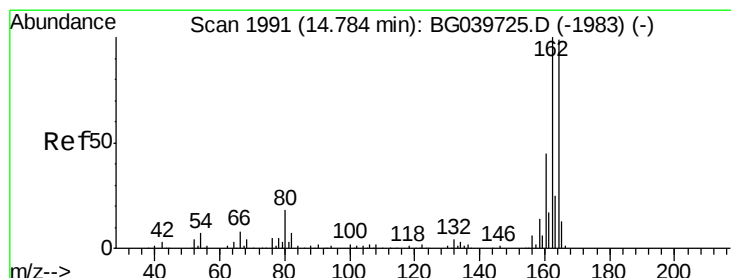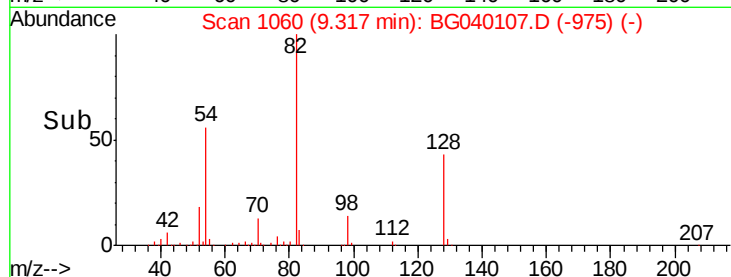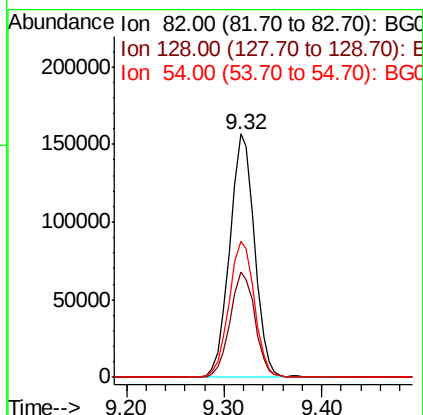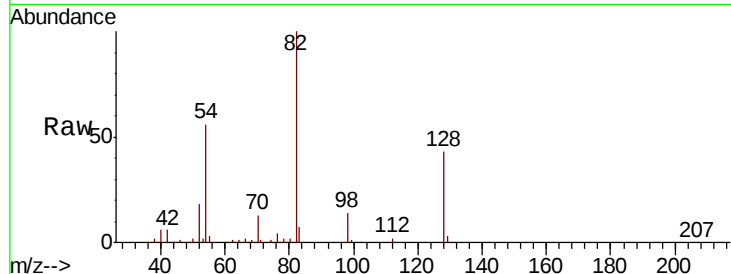

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1988
Delta R.T. -0.02 min
Lab File: BG040107.D
Acq: 23 Mar 2019 8:13

Tgt Ion	164	Resp	117728
Ion Ratio	Lower	Upper	
164	100		
162	101.8	81.6	122.4
160	44.2	34.2	51.2

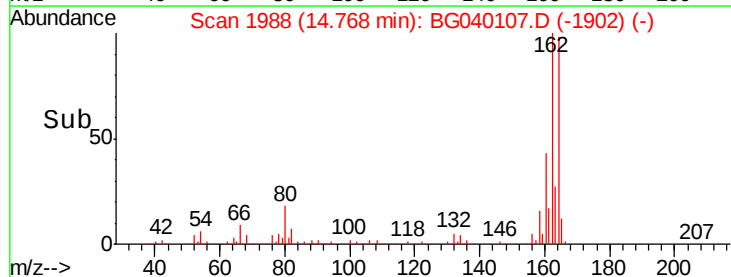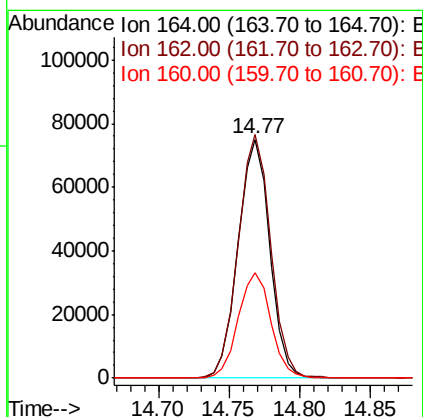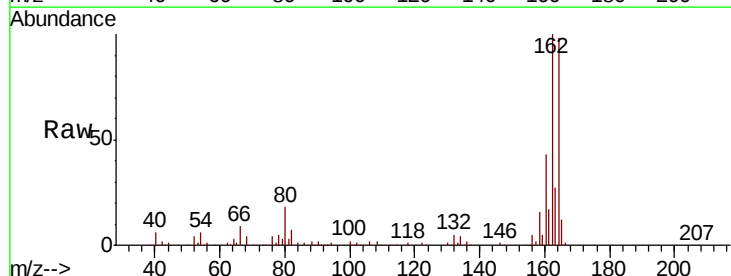


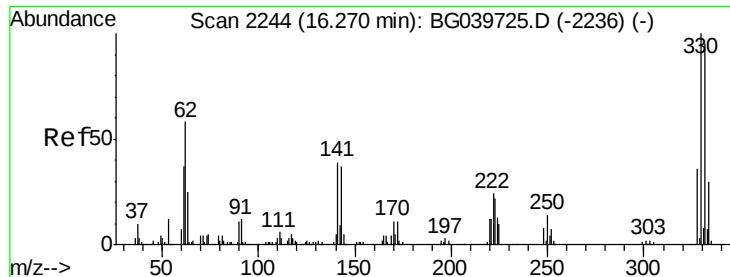

#42
 2,4,6-Tribromophenol
 Concen: 90.897 ng
 RT: 16.25 min Scan# 2241
 Delta R.T. -0.02 min
 Lab File: BG040107.D
 Acq: 23 Mar 2019 8:13

Instrument :
 BNA_G
 ClientSampleId :
 031919-LIFT-F-D-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	75.7	113.5
141	40.3	35.6	53.4



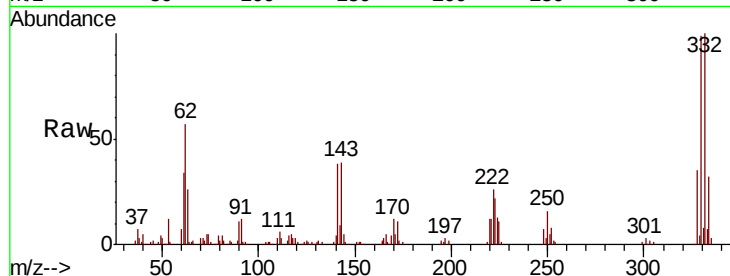


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

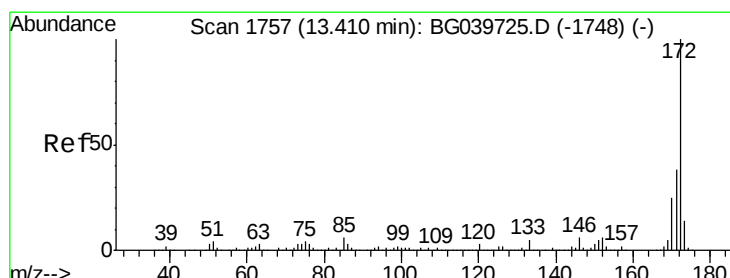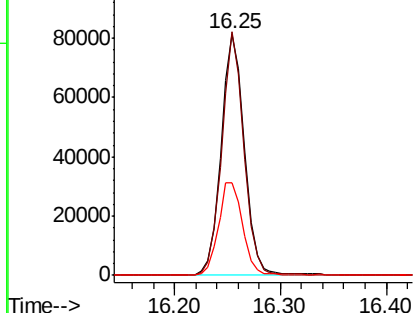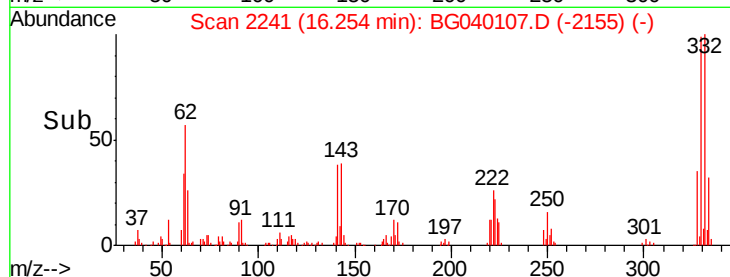

#45
 2-Fluorobiphenyl
 Concen: 87.967 ng
 RT: 13.39 min Scan# 1753
 Delta R.T. -0.03 min
 Lab File: BG040107.D
 Acq: 23 Mar 2019 8:13

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	30.8	46.2
170	24.8	20.2	30.4


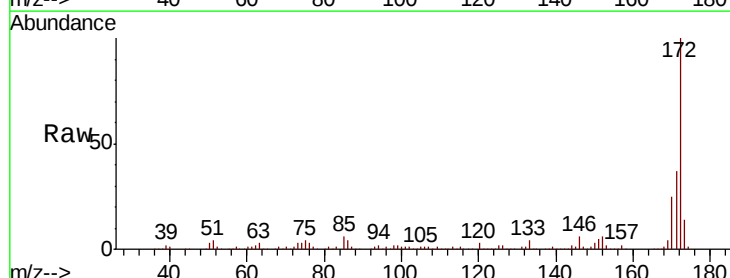


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

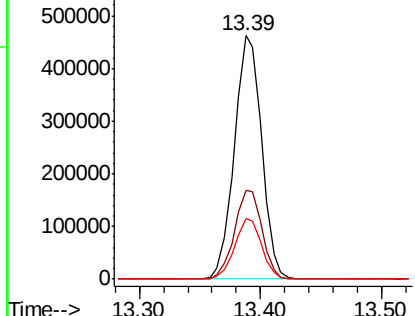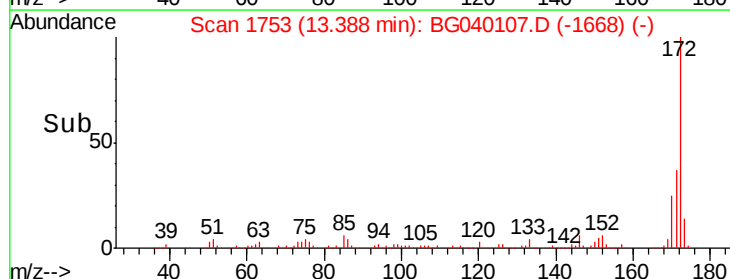



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.51 min Scan# 2455

Delta R.T. -0.02 min

Lab File: BG040107.D

Acq: 23 Mar 2019 8:13

Instrument :

BNA_G

ClientSampleId :

031919-LIFT-F-D-S


Tot Ion:188 Resp: 288549

Ion Ratio Lower Upper

188 100

94 8.4 6.9 10.3




80 9.0 8.1 12.1

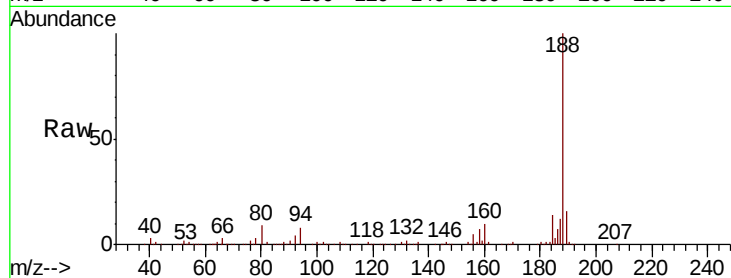

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

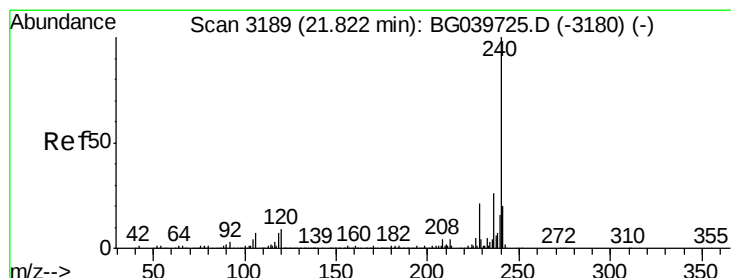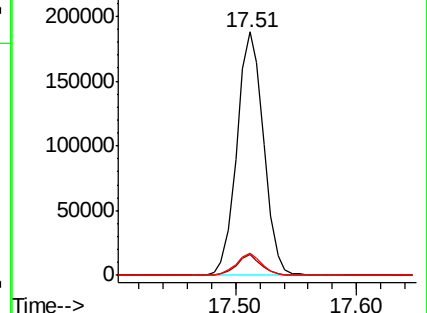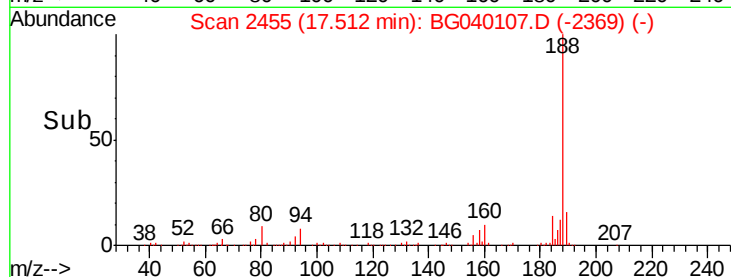

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3185

Delta R.T. -0.03 min

Lab File: BG040107.D

Acq: 23 Mar 2019 8:13


Tgt Ion:240 Resp: 281304

Ion Ratio Lower Upper

240 100

120 8.0 7.0 10.6



236 25.8 21.0 31.4

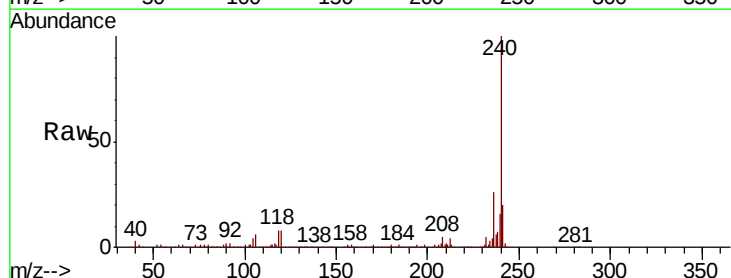

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

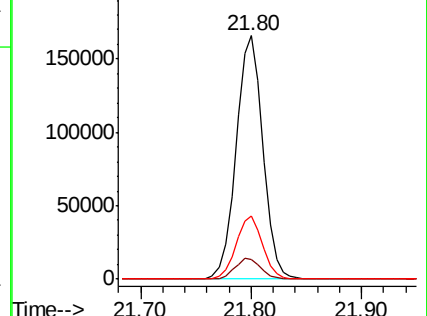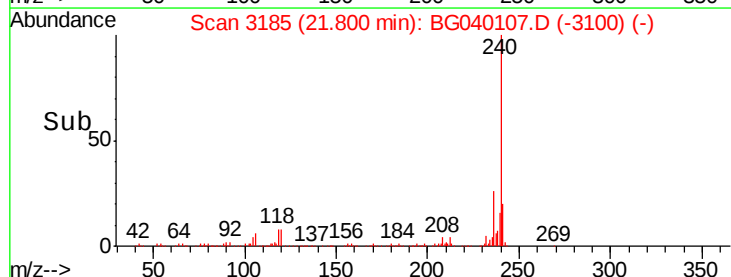



#79

Terphenyl-d14

Concen: 77.662 ng

RT: 20.11 min Scan# 2897

Delta R.T. -0.02 min

Lab File: BG040107.D

Acq: 23 Mar 2019 8:13

Instrument :

BNA_G

ClientSampleId :

031919-LIFT-F-D-S


Tot Ion:244 Resp: 992211

Ion Ratio Lower Upper

244 100

212 9.1 7.3 10.9




122 8.9 8.4 12.6

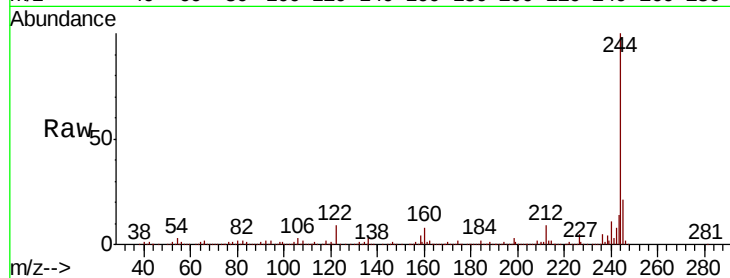

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

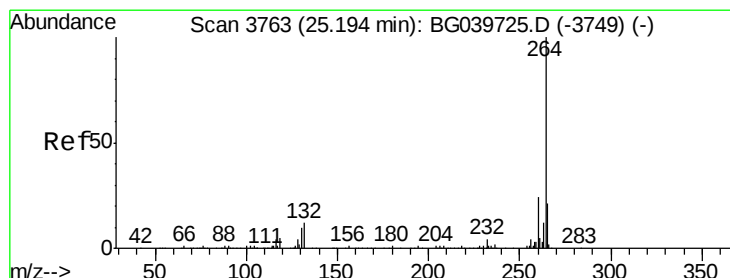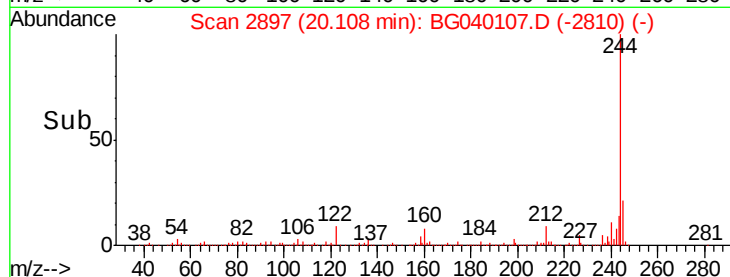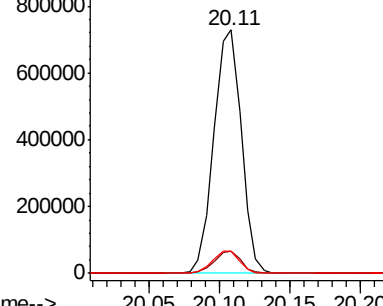

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.16 min Scan# 3757

Delta R.T. -0.04 min

Lab File: BG040107.D

Acq: 23 Mar 2019 8:13


Tgt Ion:264 Resp: 277551

Ion Ratio Lower Upper

264 100

260 23.2 18.2 27.4

265 21.4 18.5 27.7

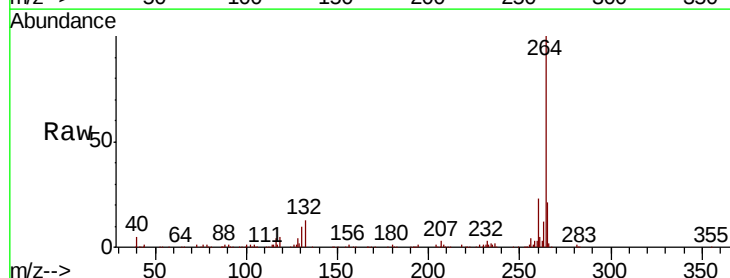

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

