


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032219\
 Data File : BG040079.D
 Acq On : 22 Mar 2019 12:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

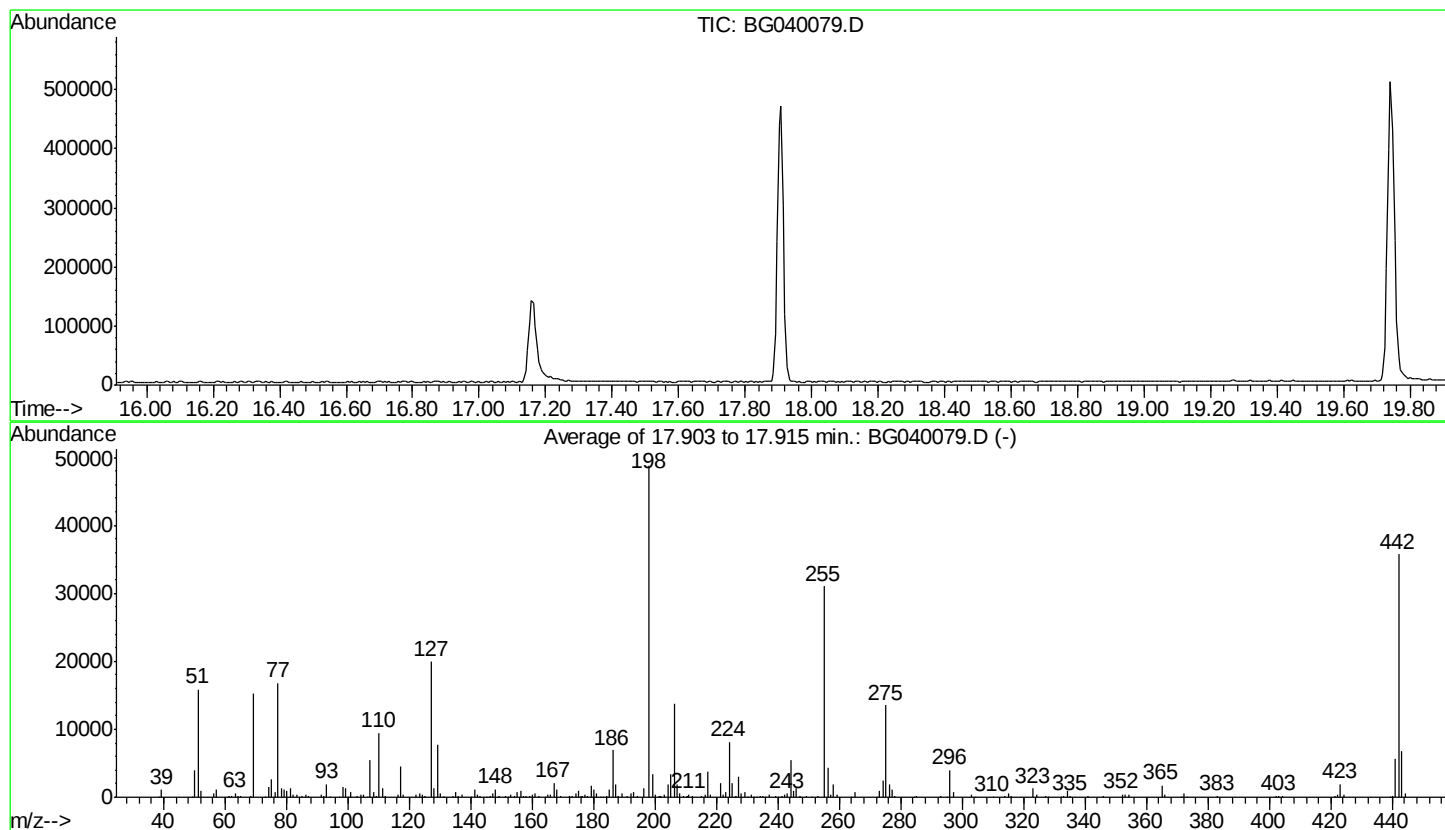

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	15866	PASS
68	69	0.00	2	0.9	136	PASS
69	198	0.00	100	31.2	15199	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	19945	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48789	PASS
199	198	5	9	6.9	3360	PASS
275	198	10	60	27.7	13526	PASS
365	198	1	100	3.7	1781	PASS
441	198	0.01	100	11.5	5589	PASS
442	198	50	100	73.3	35765	PASS
443	442	15	24	19.0	6795	PASS