


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032219\
 Data File : BG040097.D
 Acq On : 23 Mar 2019 1:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

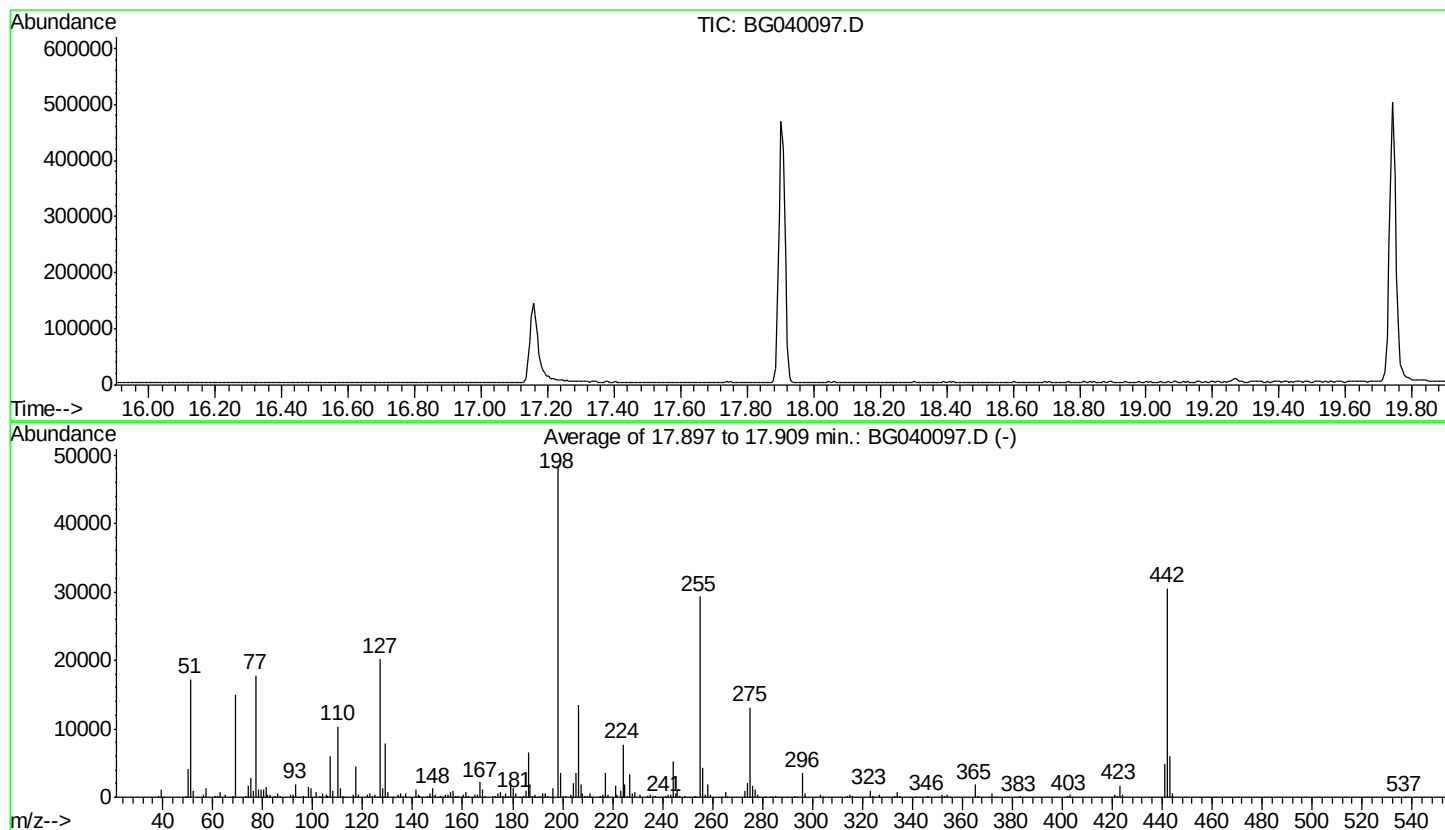

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	17242	PASS
68	69	0.00	2	1.6	240	PASS
69	198	0.00	100	30.8	14920	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	20222	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48434	PASS
199	198	5	9	7.2	3489	PASS
275	198	10	60	27.1	13139	PASS
365	198	1	100	3.7	1809	PASS
441	198	0.01	100	9.9	4800	PASS
442	198	50	100	63.0	30530	PASS
443	442	15	24	19.7	6012	PASS