

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052792.D
 Acq On : 23 Mar 2022 11:16
 Operator : CG/JU
 Sample : PB143280BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.556	24	28	33	rVB3	11673	16129	1.42%	0.152%
2	3.826	72	74	76	rBV2	1486	1201	0.11%	0.011%
3	3.908	87	88	91	rBV2	2122	1872	0.16%	0.018%
4	3.973	95	99	112	rVV	106568	188296	16.54%	1.771%
5	4.061	112	114	115	rVV2	2809	2201	0.19%	0.021%
6	4.073	115	116	123	rVV6	2412	4162	0.37%	0.039%
7	4.120	123	124	127	rVB3	2572	1545	0.14%	0.015%
8	4.208	137	139	141	rBV2	1966	1265	0.11%	0.012%
9	4.308	154	156	157	rBV2	3027	2380	0.21%	0.022%
10	4.390	169	170	174	rBV4	1291	1173	0.10%	0.011%
11	4.725	225	227	229	rVB2	2471	2036	0.18%	0.019%
12	4.742	229	230	232	rBV2	2259	1618	0.14%	0.015%
13	5.112	290	293	295	rBV3	1837	1863	0.16%	0.018%
14	5.189	305	306	310	rBV2	1878	1425	0.13%	0.013%
15	5.230	310	313	315	rBV2	1661	1963	0.17%	0.018%
16	5.365	335	336	339	rBV3	1326	1144	0.10%	0.011%
17	5.482	353	356	357	rBV2	1470	1599	0.14%	0.015%
18	5.612	377	378	384	rVB6	1599	2339	0.21%	0.022%
19	6.264	486	489	490	rVB3	1603	1288	0.11%	0.012%
20	6.293	490	494	495	rBV2	1219	1264	0.11%	0.012%
21	6.458	519	522	525	rVB3	1744	2019	0.18%	0.019%
22	6.493	525	528	529	rBV2	1039	1238	0.11%	0.012%
23	6.534	532	535	538	rBV3	926	1614	0.14%	0.015%
24	6.622	548	550	554	rVB3	1160	1453	0.13%	0.014%
25	6.963	606	608	611	rVB2	1086	1209	0.11%	0.011%
26	7.133	636	637	641	rVB2	1597	1299	0.11%	0.012%
27	7.180	641	645	647	rBV3	1063	1348	0.12%	0.013%
28	7.286	656	663	673	rVB	152695	260693	22.90%	2.452%
29	7.456	684	692	703	rBV	105028	183514	16.12%	1.726%
30	7.674	721	729	736	rBV	140048	242373	21.29%	2.280%
31	7.867	761	762	765	rBV	1052	1139	0.10%	0.011%
32	7.897	765	767	770	rVV2	1056	1445	0.13%	0.014%
33	8.003	784	785	791	rVB4	905	1203	0.11%	0.011%
34	8.067	793	796	799	rVB2	1032	1352	0.12%	0.013%
35	8.144	802	809	816	rVB	95321	164312	14.43%	1.546%
36	8.467	862	864	868	rBV2	823	1185	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052792.D
 Acq On : 23 Mar 2022 11:16
 Operator : CG/JU
 Sample : PB143280BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	8.743	909	911	914	rBV	1037	1184	0.10%	0.011%
38	8.831	920	926	936	rBV	170088	305560	26.84%	2.875%
39	9.230	990	994	996	rBV	1013	1152	0.10%	0.011%
40	9.301	998	1006	1013	rVV	148843	257753	22.64%	2.425%
41	9.389	1019	1021	1025	rVB3	1053	1514	0.13%	0.014%
42	9.454	1029	1032	1036	rVB3	832	1238	0.11%	0.012%
43	10.023	1123	1129	1143	rVB2	118430	219012	19.24%	2.060%
44	10.570	1214	1222	1231	rVB	170627	319434	28.06%	3.005%
45	10.957	1280	1288	1296	rVB	135250	240979	21.17%	2.267%
46	11.081	1301	1309	1321	rVV	176056	330141	29.00%	3.106%
47	11.598	1394	1397	1399	rBV	1205	1393	0.12%	0.013%
48	12.532	1551	1556	1560	rVB2	3208	4818	0.42%	0.045%
49	14.159	1825	1833	1841	rBV	383741	572143	50.26%	5.382%
50	14.459	1877	1884	1892	rBV	390629	626000	54.99%	5.889%
51	14.764	1929	1936	1943	rVB2	240839	372316	32.70%	3.503%
52	14.928	1958	1964	1977	rBV	184889	314968	27.67%	2.963%
53	15.751	2096	2104	2112	rBV	529937	812736	71.39%	7.646%
54	15.857	2116	2122	2133	rVV	164551	253419	22.26%	2.384%
55	15.992	2142	2145	2148	rVB2	1759	1977	0.17%	0.019%
56	16.321	2197	2201	2203	rBV2	1447	1687	0.15%	0.016%
57	16.456	2221	2224	2227	rVV3	1212	1619	0.14%	0.015%
58	16.509	2230	2233	2237	rVB3	1076	1779	0.16%	0.017%
59	16.755	2273	2275	2278	rVB3	1173	1179	0.10%	0.011%
60	16.961	2304	2310	2311	rBV2	2148	2075	0.18%	0.020%
61	17.131	2336	2339	2341	rBV2	1256	1707	0.15%	0.016%
62	17.172	2343	2346	2348	rBV2	1319	1605	0.14%	0.015%
63	17.290	2364	2366	2368	rVV	1526	1532	0.13%	0.014%
64	17.425	2386	2389	2391	rBV2	1313	1547	0.14%	0.015%
65	17.507	2395	2403	2411	rVB	345948	513413	45.10%	4.830%
66	17.601	2413	2419	2428	rVV	591515	951440	83.57%	8.951%
67	17.789	2450	2451	2453	rBV	1505	1284	0.11%	0.012%
68	17.866	2462	2464	2467	rVB3	1545	1597	0.14%	0.015%
69	18.171	2514	2516	2518	rVB2	2167	1261	0.11%	0.012%
70	18.201	2518	2521	2523	rBV2	1347	1670	0.15%	0.016%
71	18.242	2525	2528	2531	rVB4	2193	2332	0.20%	0.022%
72	18.435	2558	2561	2562	rBV3	1223	1355	0.12%	0.013%
73	18.477	2567	2568	2571	rVB3	2026	1480	0.13%	0.014%
74	18.506	2571	2573	2576	rBV3	1583	1959	0.17%	0.018%
75	18.600	2588	2589	2592	rVB3	1559	1155	0.10%	0.011%
76	18.641	2592	2596	2597	rBV3	1949	1761	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052792.D
 Acq On : 23 Mar 2022 11:16
 Operator : CG/JU
 Sample : PB143280BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	18.659	2597	2599	2600	rVB2	2117	1273	0.11%	0.012%
78	18.688	2600	2604	2605	rBV2	1952	2262	0.20%	0.021%
79	18.723	2608	2610	2611	rVB2	2346	1234	0.11%	0.012%
80	18.770	2617	2618	2620	rBV2	1628	1442	0.13%	0.014%
81	18.800	2622	2623	2626	rBV3	1268	1200	0.11%	0.011%
82	18.864	2632	2634	2635	rBV2	1897	1875	0.16%	0.018%
83	18.894	2638	2639	2641	rVB2	2474	1659	0.15%	0.016%
84	18.923	2641	2644	2646	rBV2	2111	2456	0.22%	0.023%
85	18.964	2646	2651	2653	rBV5	1676	2367	0.21%	0.022%
86	19.023	2658	2661	2663	rVB4	1631	1394	0.12%	0.013%
87	19.058	2663	2667	2668	rVB4	1716	1828	0.16%	0.017%
88	19.076	2668	2670	2671	rBV	1787	1269	0.11%	0.012%
89	19.281	2703	2705	2706	rVB2	2312	1571	0.14%	0.015%
90	19.311	2708	2710	2712	rVV3	1917	1400	0.12%	0.013%
91	19.452	2730	2734	2740	rBV6	9123	15345	1.35%	0.144%
92	19.522	2743	2746	2749	rVV3	8234	11760	1.03%	0.111%
93	19.563	2749	2753	2759	rVB6	10504	16671	1.46%	0.157%
94	19.804	2790	2794	2799	rBV8	11636	15548	1.37%	0.146%
95	19.886	2802	2808	2818	rVV	814728	1138465	100.00%	10.710%
96	20.633	2933	2935	2940	rBV6	7293	7404	0.65%	0.070%
97	21.790	3126	3132	3140	rVB	332282	555558	48.80%	5.226%
98	24.104	3524	3526	3529	rBV4	8621	10296	0.90%	0.097%
99	24.886	3648	3659	3668	rVB3	352231	1019947	89.59%	9.595%
100	25.109	3687	3697	3715	rVB4	177715	578275	50.79%	5.440%




Sum of corrected areas: 10629832

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052792.D
Acq On : 23 Mar 2022 11:16
Operator : CG/JU
Sample : PB143280BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

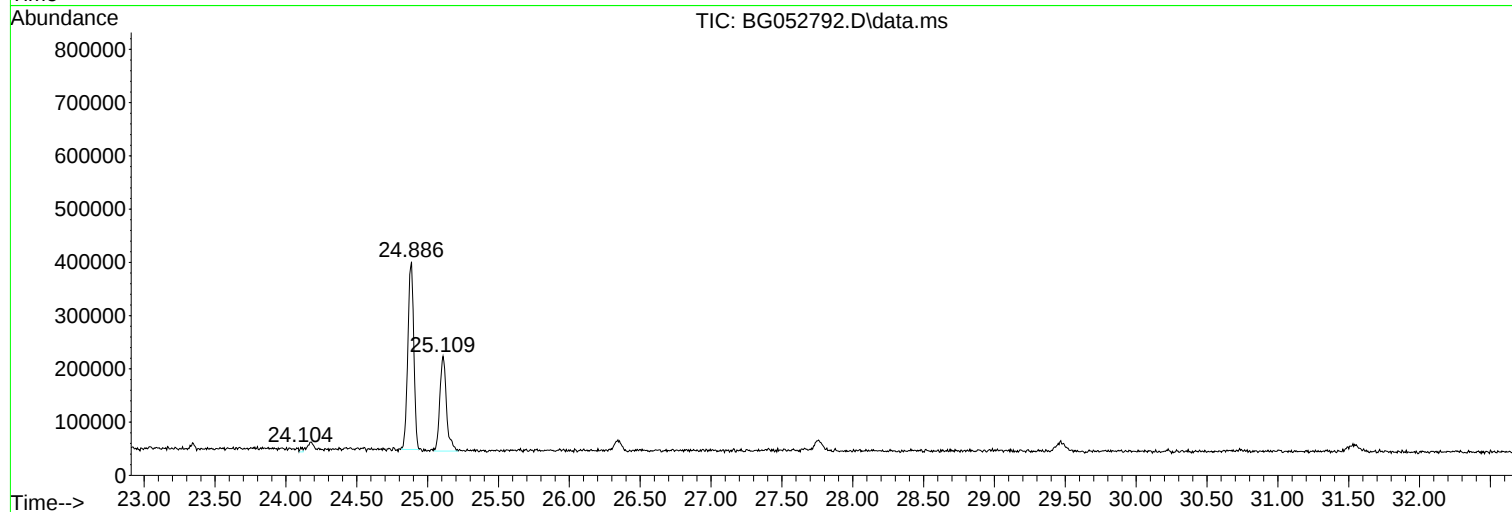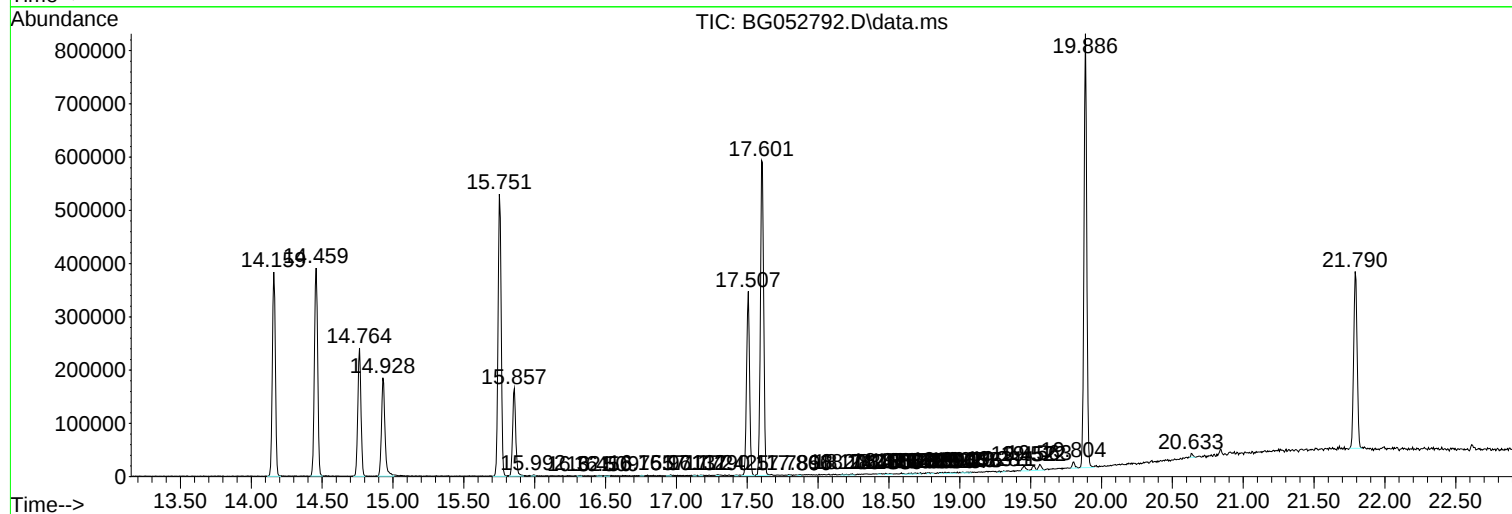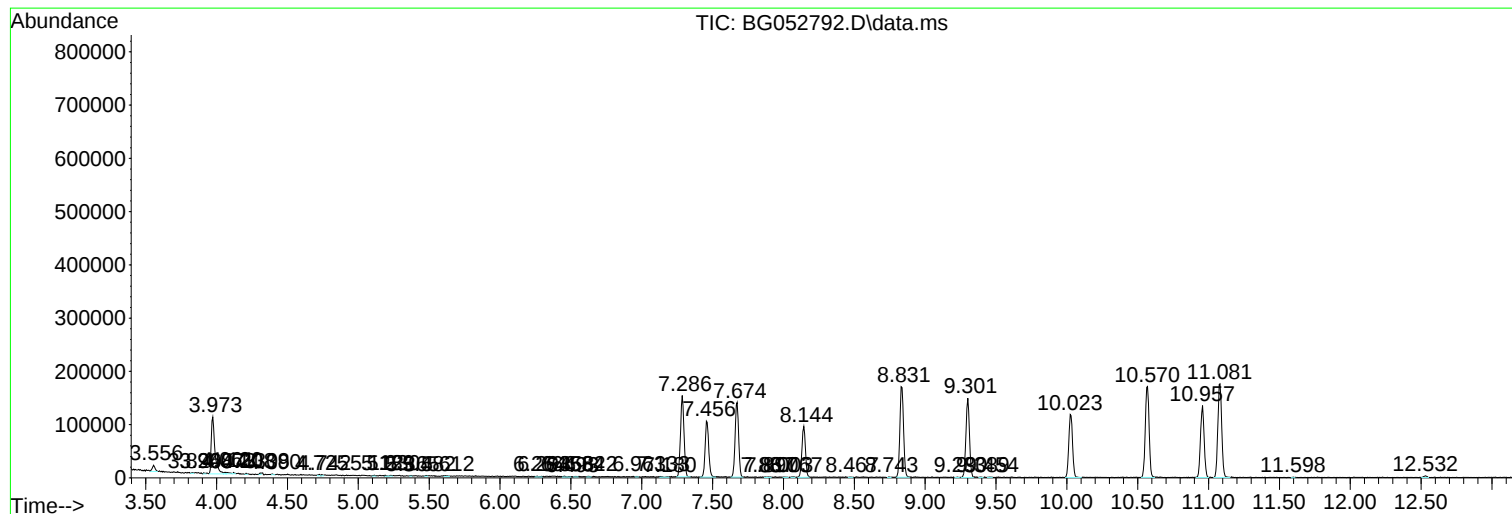

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052792.D
Acq On : 23 Mar 2022 11:16
Operator : CG/JU
Sample : PB143280BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052792.D
Acq On : 23 Mar 2022 11:16
Operator : CG/JU
Sample : PB143280BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------