

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052795.D
 Acq On : 23 Mar 2022 13:24
 Operator : CG/JU
 Sample : N1883-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.553	26	28	34	rVB4	7697	10461	1.15%	0.114%
2	3.976	96	100	109	rBV	63281	105955	11.61%	1.159%
3	4.898	255	257	260	rBV4	1517	1538	0.17%	0.017%
4	5.039	279	281	285	rBV2	1531	2129	0.23%	0.023%
5	5.104	291	292	294	rBV	1680	1282	0.14%	0.014%
6	6.314	495	498	501	rBV2	1319	1752	0.19%	0.019%
7	6.461	521	523	525	rBV2	1586	1392	0.15%	0.015%
8	6.513	530	532	537	rBV4	1564	2376	0.26%	0.026%
9	6.643	553	554	556	rBV2	1394	1274	0.14%	0.014%
10	6.772	574	576	581	rBV3	1349	1698	0.19%	0.019%
11	6.913	597	600	601	rBV2	1116	1252	0.14%	0.014%
12	6.977	609	611	615	rVB3	1279	1542	0.17%	0.017%
13	7.283	656	663	674	rBV2	113642	209660	22.97%	2.294%
14	7.459	686	693	701	rBV	78650	138128	15.13%	1.511%
15	7.547	705	708	710	rBV3	1386	1600	0.18%	0.018%
16	7.671	722	729	736	rVB	102675	176524	19.34%	1.931%
17	7.923	770	772	776	rBV3	1282	1397	0.15%	0.015%
18	7.970	776	780	783	rBV3	1488	1622	0.18%	0.018%
19	8.141	803	809	818	rBV	110573	188854	20.69%	2.066%
20	8.605	885	888	891	rBV3	1186	1405	0.15%	0.015%
21	8.834	919	927	936	rBV2	131976	226528	24.82%	2.478%
22	8.963	945	949	953	rBV3	1063	1313	0.14%	0.014%
23	9.257	995	999	1000	rBV2	1070	1247	0.14%	0.014%
24	9.298	1000	1006	1014	rVV	104129	189247	20.73%	2.070%
25	9.468	1030	1035	1039	rVB4	2351	3018	0.33%	0.033%
26	9.744	1077	1082	1087	rVB4	3460	4647	0.51%	0.051%
27	10.026	1121	1130	1138	rBV	86764	156518	17.15%	1.712%
28	10.567	1215	1222	1231	rVB	132426	237567	26.02%	2.599%
29	10.631	1231	1233	1237	rVV	1169	1445	0.16%	0.016%
30	10.690	1239	1243	1244	rBV	963	1367	0.15%	0.015%
31	10.719	1244	1248	1252	rVV2	5099	8336	0.91%	0.091%
32	10.784	1256	1259	1262	rVB2	1207	1652	0.18%	0.018%
33	10.954	1281	1288	1297	rVB	155848	282253	30.92%	3.088%
34	11.078	1301	1309	1319	rBV	134520	241022	26.40%	2.637%
35	11.836	1433	1438	1440	rBV2	795	1291	0.14%	0.014%
36	11.959	1455	1459	1464	rVB	921	1541	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052795.D
 Acq On : 23 Mar 2022 13:24
 Operator : CG/JU
 Sample : N1883-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	12.012	1464	1468	1471	rVB2	1138	1280	0.14%	0.014%
38	12.529	1550	1556	1560	rBV3	2834	3996	0.44%	0.044%
39	13.586	1732	1736	1739	rBV3	2818	3348	0.37%	0.037%
40	14.156	1827	1833	1840	rBV	275625	408125	44.71%	4.465%

41	14.209	1840	1842	1844	rVB2	1694	1626	0.18%	0.018%
42	14.356	1865	1867	1870	rBV	1306	1862	0.20%	0.020%
43	14.397	1870	1874	1878	rVV4	4910	8195	0.90%	0.090%
44	14.456	1878	1884	1894	rVB	306550	476269	52.17%	5.210%
45	14.649	1914	1917	1921	rBV2	2166	2846	0.31%	0.031%

46	14.761	1930	1936	1945	rBV	270376	430438	47.15%	4.709%
47	14.931	1958	1965	1975	rBV	113315	200755	21.99%	2.196%
48	15.096	1991	1993	1996	rVB2	1565	1677	0.18%	0.018%
49	15.395	2040	2044	2047	rVB	3408	4215	0.46%	0.046%
50	15.501	2060	2062	2066	rBV2	898	1519	0.17%	0.017%

51	15.560	2066	2072	2076	rVV4	4551	8219	0.90%	0.090%
52	15.595	2076	2078	2083	rVB3	3192	4533	0.50%	0.050%
53	15.701	2094	2096	2098	rBV2	1183	1226	0.13%	0.013%
54	15.754	2098	2105	2112	rVV	388272	621933	68.13%	6.804%
55	15.854	2116	2122	2130	rBV	97366	147322	16.14%	1.612%

56	15.989	2142	2145	2146	rBV2	2526	2380	0.26%	0.026%
57	16.083	2159	2161	2164	rBV3	1304	1427	0.16%	0.016%
58	16.153	2169	2173	2177	rBV4	2020	3341	0.37%	0.037%
59	16.294	2194	2197	2202	rVB3	1807	1508	0.17%	0.016%
60	16.347	2205	2206	2209	rVB2	1691	1310	0.14%	0.014%

61	16.382	2209	2212	2213	rBV3	1767	1646	0.18%	0.018%
62	16.465	2223	2226	2228	rBV2	2660	3288	0.36%	0.036%
63	16.529	2234	2237	2238	rBV3	1199	1212	0.13%	0.013%
64	16.641	2251	2256	2260	rVB5	4024	6347	0.70%	0.069%
65	16.811	2282	2285	2286	rBV2	2017	1804	0.20%	0.020%

66	16.835	2286	2289	2292	rVB3	2073	2051	0.22%	0.022%
67	16.876	2292	2296	2299	rVB4	1916	2563	0.28%	0.028%
68	16.917	2299	2303	2304	rBV3	1859	1782	0.20%	0.019%
69	16.958	2307	2310	2311	rBV	2141	2263	0.25%	0.025%
70	17.175	2344	2347	2349	rBV2	1527	2173	0.24%	0.024%

71	17.252	2357	2360	2364	rBV3	4591	6255	0.69%	0.068%
72	17.287	2364	2366	2367	rBV2	2065	1608	0.18%	0.018%
73	17.387	2381	2383	2384	rBV2	1973	1299	0.14%	0.014%
74	17.410	2384	2387	2393	rVB3	6260	9098	1.00%	0.100%
75	17.504	2396	2403	2410	rVV	396895	593627	65.03%	6.494%

76	17.604	2413	2420	2431	rVV	467640	743633	81.46%	8.135%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052795.D
 Acq On : 23 Mar 2022 13:24
 Operator : CG/JU
 Sample : N1883-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	17.681	2431	2433	2436	rVB3	3511	3816	0.42%	0.042%
78	17.763	2444	2447	2448	rBV2	1900	1972	0.22%	0.022%
79	17.980	2481	2484	2485	rBV3	1732	1894	0.21%	0.021%
80	18.145	2509	2512	2513	rBV3	2064	1760	0.19%	0.019%
81	18.168	2513	2516	2519	rVV3	4488	5556	0.61%	0.061%
82	18.215	2522	2524	2526	rBV2	2398	1916	0.21%	0.021%
83	18.350	2544	2547	2548	rBV2	2165	1902	0.21%	0.021%
84	18.391	2550	2554	2560	rBV6	9814	20212	2.21%	0.221%
85	19.455	2732	2735	2738	rBV4	6072	6380	0.70%	0.070%
86	19.525	2743	2747	2751	rBV4	6687	11312	1.24%	0.124%
87	19.884	2802	2808	2816	rVB	615922	912857	100.00%	9.986%
88	21.423	3067	3070	3078	rBV4	30874	53561	5.87%	0.586%
89	21.793	3127	3133	3139	rVB	406911	663289	72.66%	7.256%
90	24.877	3650	3658	3672	rVB2	295958	851138	93.24%	9.311%
91	25.106	3689	3697	3711	rVB2	224792	672609	73.68%	7.358%




Sum of corrected areas: 9141006

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052795.D
Acq On : 23 Mar 2022 13:24
Operator : CG/JU
Sample : N1883-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

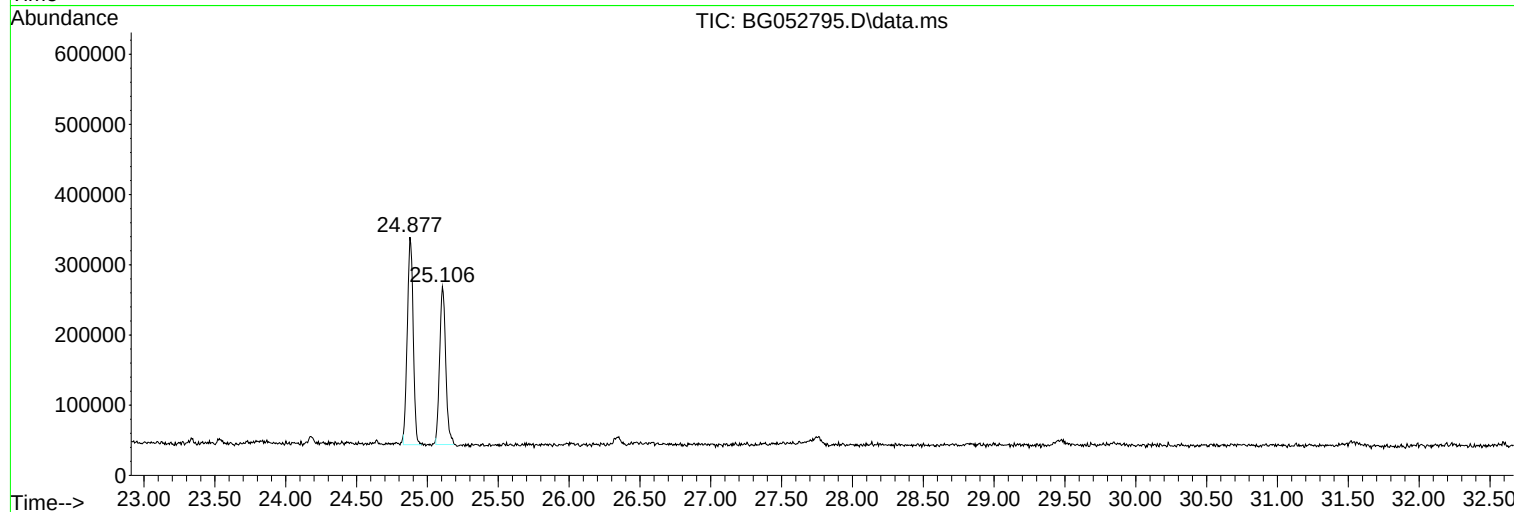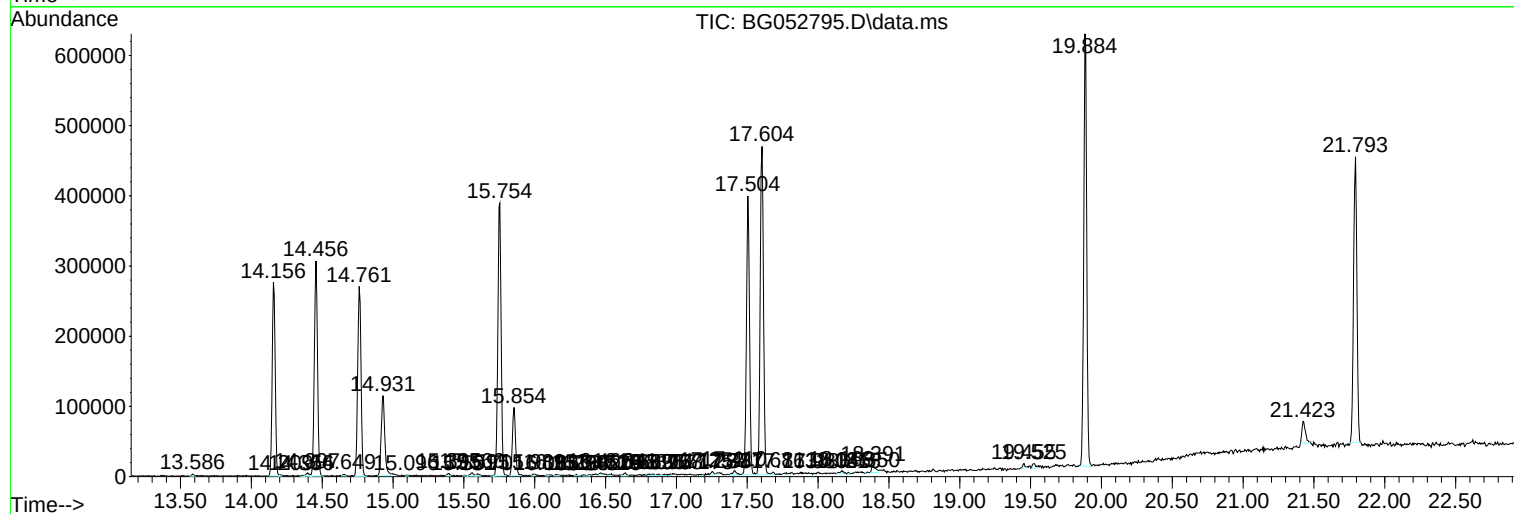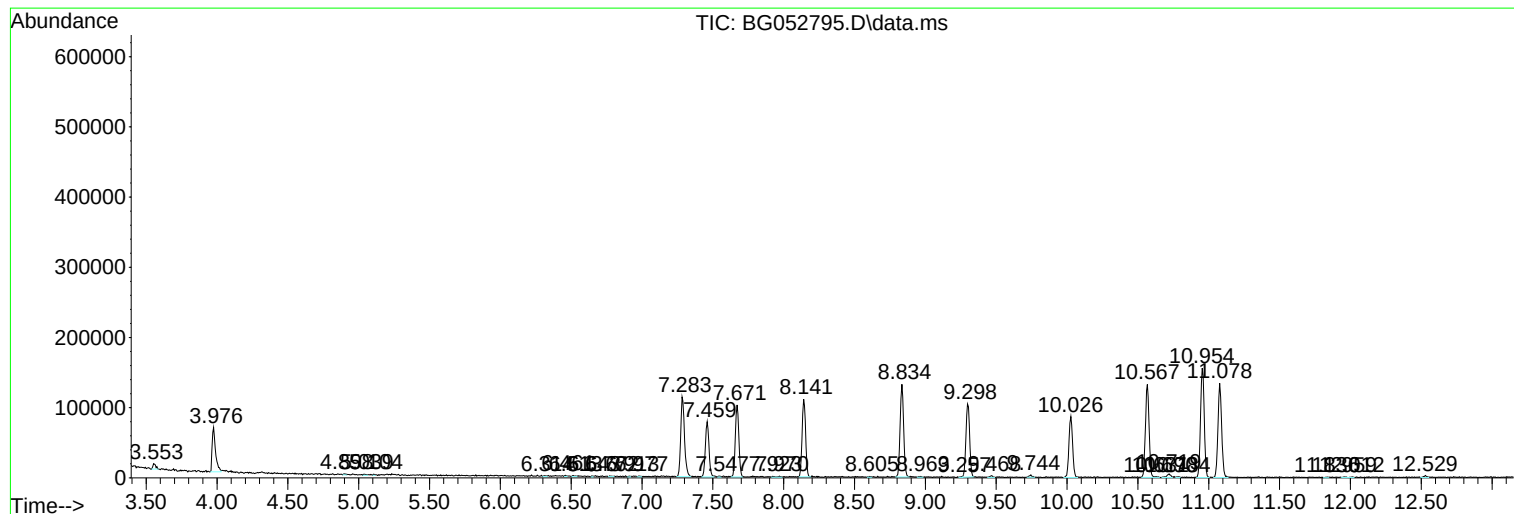

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052795.D
Acq On : 23 Mar 2022 13:24
Operator : CG/JU
Sample : N1883-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052795.D
Acq On : 23 Mar 2022 13:24
Operator : CG/JU
Sample : N1883-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc