

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052797.D
 Acq On : 23 Mar 2022 14:41
 Operator : CG/JU
 Sample : N2026-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.053	282	283	285	rBV2	1773	825	0.14%	0.032%
2	5.082	286	288	289	rVB2	1731	852	0.14%	0.033%
3	5.165	301	302	304	rBV2	2209	1242	0.21%	0.048%
4	5.241	313	315	316	rBV2	1352	823	0.14%	0.032%
5	5.488	355	357	358	rBV2	1423	1006	0.17%	0.039%
6	5.723	395	397	400	rBV3	1191	1150	0.20%	0.045%
7	5.952	433	436	439	rVB3	1175	1304	0.22%	0.051%
8	6.128	463	466	467	rBV2	1229	1247	0.21%	0.049%
9	6.187	473	476	477	rBV2	1595	1485	0.25%	0.058%
10	6.381	506	509	511	rBV3	1400	1733	0.29%	0.068%
11	6.469	522	524	526	rVB	1146	890	0.15%	0.035%
12	6.727	567	568	572	rVB2	813	804	0.14%	0.031%
13	6.921	597	601	603	rBV3	1021	1204	0.20%	0.047%
14	6.956	606	607	611	rVB2	1172	1025	0.17%	0.040%
15	7.174	642	644	647	rVB3	1137	927	0.16%	0.036%
16	7.197	647	648	651	rVB3	1178	784	0.13%	0.031%
17	7.232	651	654	657	rBV3	1163	1493	0.25%	0.058%
18	7.338	670	672	674	rVB2	2064	1314	0.22%	0.051%
19	7.362	674	676	678	rBV2	1007	930	0.16%	0.036%
20	7.685	729	731	735	rBV2	913	1060	0.18%	0.041%
21	7.978	778	781	784	rVB3	806	993	0.17%	0.039%
22	8.020	786	788	789	rBV	1013	755	0.13%	0.029%
23	8.143	803	809	816	rVB	100231	168241	28.58%	6.560%
24	8.296	832	835	836	rVB3	807	775	0.13%	0.030%
25	8.425	856	857	861	rBV2	1005	981	0.17%	0.038%
26	8.472	864	865	868	rBV2	858	1023	0.17%	0.040%
27	8.537	873	876	877	rBV2	938	781	0.13%	0.030%
28	8.548	877	878	880	rBV2	994	781	0.13%	0.030%
29	8.613	887	889	892	rVB3	809	943	0.16%	0.037%
30	8.754	911	913	918	rVB2	1421	2198	0.37%	0.086%
31	8.830	923	926	929	rVB2	1359	1466	0.25%	0.057%
32	8.983	950	952	954	rBV2	889	1053	0.18%	0.041%
33	9.200	987	989	996	rVB	1104	1509	0.26%	0.059%
34	9.253	996	998	1000	rBV	1239	1104	0.19%	0.043%
35	9.365	1014	1017	1018	rBV	798	747	0.13%	0.029%
36	9.494	1036	1039	1042	rBV2	1196	1156	0.20%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052797.D
 Acq On : 23 Mar 2022 14:41
 Operator : CG/JU
 Sample : N2026-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	9.635	1061	1063	1065	rVB3	1206	924	0.16%	0.036%
38	9.682	1069	1071	1074	rVB2	863	782	0.13%	0.030%
39	9.723	1074	1078	1080	rBV	697	952	0.16%	0.037%
40	9.811	1091	1093	1095	rVB	1139	955	0.16%	0.037%
41	9.941	1112	1115	1117	rVB2	872	1059	0.18%	0.041%
42	10.005	1125	1126	1130	rVB	1184	830	0.14%	0.032%
43	10.070	1134	1137	1140	rVB3	777	883	0.15%	0.034%
44	10.463	1201	1204	1209	rBV2	1119	1396	0.24%	0.054%
45	10.734	1249	1250	1255	rBV2	790	1026	0.17%	0.040%
46	10.804	1260	1262	1264	rVB	1032	882	0.15%	0.034%
47	10.833	1264	1267	1268	rBV2	967	928	0.16%	0.036%
48	10.957	1280	1288	1295	rVB2	128150	240108	40.79%	9.363%
49	11.468	1371	1375	1376	rBV3	964	1106	0.19%	0.043%
50	11.515	1382	1383	1387	rBV2	887	829	0.14%	0.032%
51	11.591	1393	1396	1397	rBV2	843	746	0.13%	0.029%
52	11.673	1408	1410	1412	rVB	1217	882	0.15%	0.034%
53	11.691	1412	1413	1416	rBV	881	1107	0.19%	0.043%
54	11.920	1450	1452	1453	rVB	1523	778	0.13%	0.030%
55	11.938	1453	1455	1459	rBV2	1062	1212	0.21%	0.047%
56	12.138	1485	1489	1492	rVB2	1202	1459	0.25%	0.057%
57	12.355	1525	1526	1529	rBV	941	950	0.16%	0.037%
58	12.472	1545	1546	1549	rBV	547	749	0.13%	0.029%
59	12.531	1552	1556	1557	rBV	835	932	0.16%	0.036%
60	12.578	1560	1564	1566	rBV2	1054	983	0.17%	0.038%
61	12.619	1568	1571	1572	rBV	950	969	0.16%	0.038%
62	12.719	1586	1588	1590	rVB2	857	827	0.14%	0.032%
63	12.848	1606	1610	1612	rBV3	754	787	0.13%	0.031%
64	13.171	1661	1665	1667	rBV2	813	789	0.13%	0.031%
65	14.123	1825	1827	1830	rBV2	1112	981	0.17%	0.038%
66	14.158	1830	1833	1836	rBV2	1063	1247	0.21%	0.049%
67	14.340	1860	1864	1865	rVB	964	1060	0.18%	0.041%
68	14.382	1865	1871	1875	rBV3	1100	2252	0.38%	0.088%
69	14.564	1900	1902	1904	rVB	1283	861	0.15%	0.034%
70	14.587	1904	1906	1908	rBV	832	819	0.14%	0.032%
71	14.687	1919	1923	1924	rBV	914	860	0.15%	0.034%
72	14.763	1929	1936	1944	rBV	231457	365300	62.05%	14.244%
73	15.515	2061	2064	2065	rBV2	998	1117	0.19%	0.044%
74	16.056	2154	2156	2159	rBV2	577	747	0.13%	0.029%
75	16.220	2182	2184	2186	rBV2	890	795	0.14%	0.031%
76	16.355	2204	2207	2208	rVB2	1385	931	0.16%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052797.D
 Acq On : 23 Mar 2022 14:41
 Operator : CG/JU
 Sample : N2026-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	16.379	2208	2211	2212	rBV2	1190	1013	0.17%	0.040%
78	16.555	2237	2241	2242	rBV	2035	1383	0.23%	0.054%
79	16.796	2279	2282	2286	rBV2	1351	1845	0.31%	0.072%
80	16.884	2294	2297	2301	rBV3	1166	1317	0.22%	0.051%
81	17.201	2350	2351	2353	rVB2	1515	775	0.13%	0.030%
82	17.289	2362	2366	2368	rBV2	1382	1743	0.30%	0.068%
83	17.325	2370	2372	2375	rVB3	878	974	0.17%	0.038%
84	17.366	2377	2379	2382	rBV2	972	882	0.15%	0.034%
85	17.507	2396	2403	2411	rBV	322495	511917	86.96%	19.962%
86	17.589	2415	2417	2419	rBV2	884	765	0.13%	0.030%
87	17.847	2460	2461	2463	rBV2	1265	993	0.17%	0.039%
88	17.924	2472	2474	2475	rBV2	2067	1226	0.21%	0.048%
89	17.936	2475	2476	2479	rVV2	902	783	0.13%	0.031%
90	17.988	2484	2485	2488	rVV3	1555	1567	0.27%	0.061%
91	18.035	2492	2493	2495	rBV	1071	796	0.14%	0.031%
92	18.088	2501	2502	2504	rBV2	1464	1235	0.21%	0.048%
93	18.159	2510	2514	2515	rBV4	1754	1799	0.31%	0.070%
94	18.229	2525	2526	2527	rBV	1533	768	0.13%	0.030%
95	18.570	2582	2584	2587	rBV2	1114	1024	0.17%	0.040%
96	19.022	2659	2661	2662	rBV2	1820	1084	0.18%	0.042%
97	19.040	2662	2664	2665	rBV	2151	1257	0.21%	0.049%
98	19.351	2715	2717	2720	rBV4	2241	2978	0.51%	0.116%
99	21.789	3126	3132	3141	rVB	351098	588686	100.00%	22.955%
100	25.108	3689	3697	3712	rVB	195171	588301	99.93%	22.940%




Sum of corrected areas: 2564515

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052797.D
Acq On : 23 Mar 2022 14:41
Operator : CG/JU
Sample : N2026-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

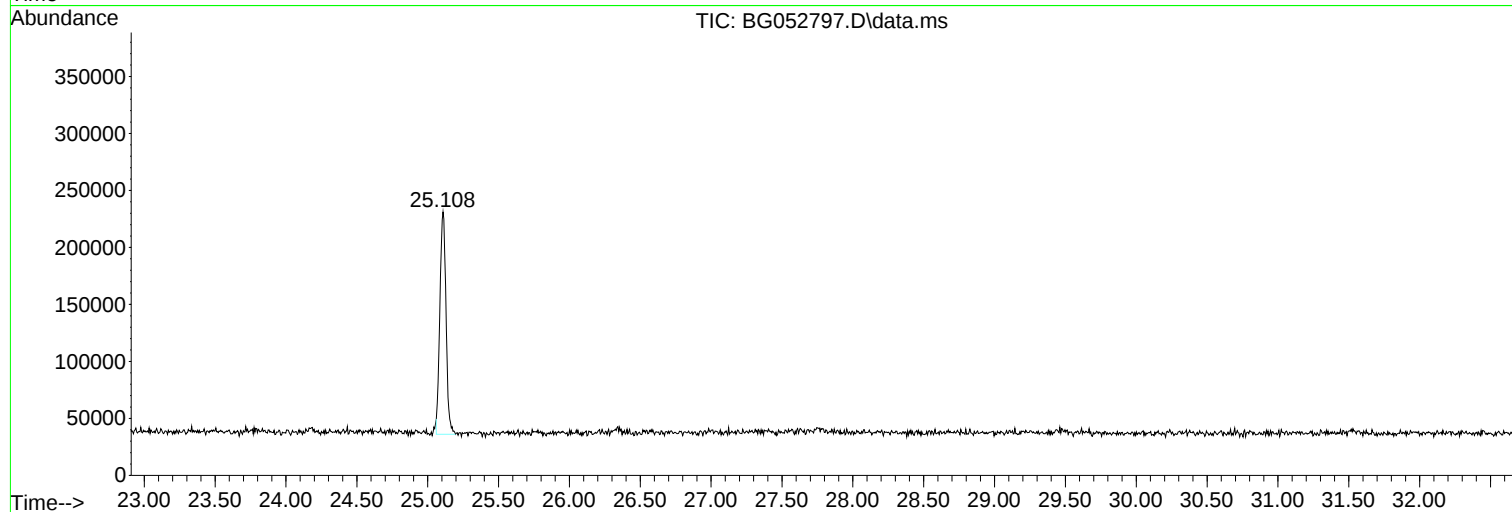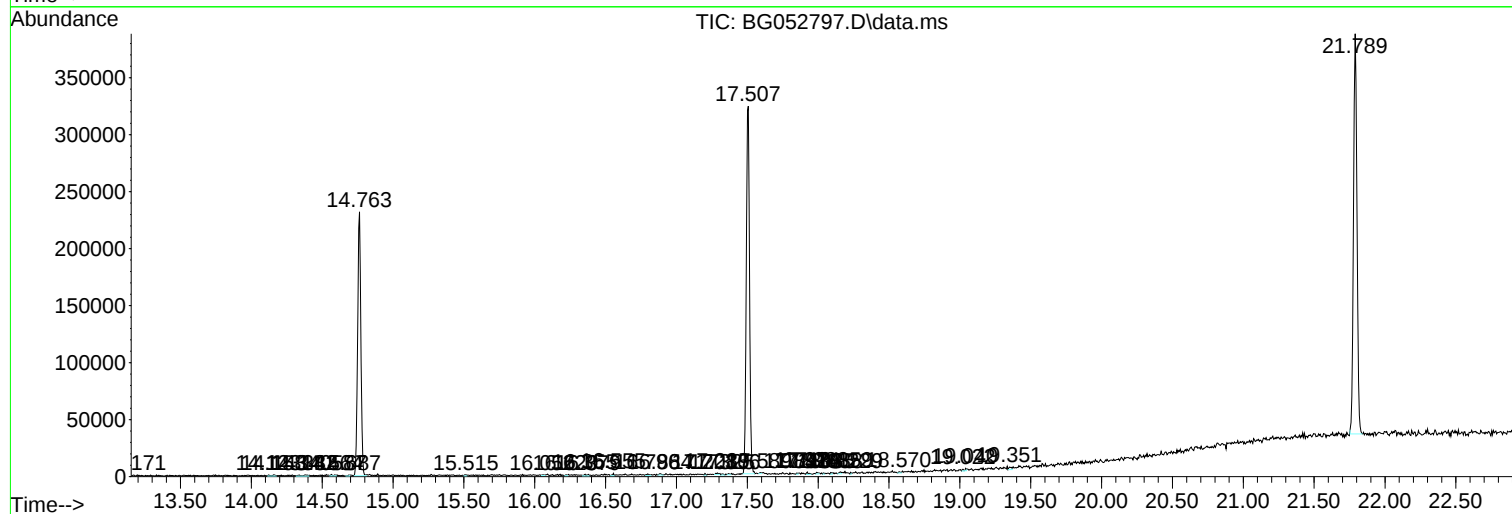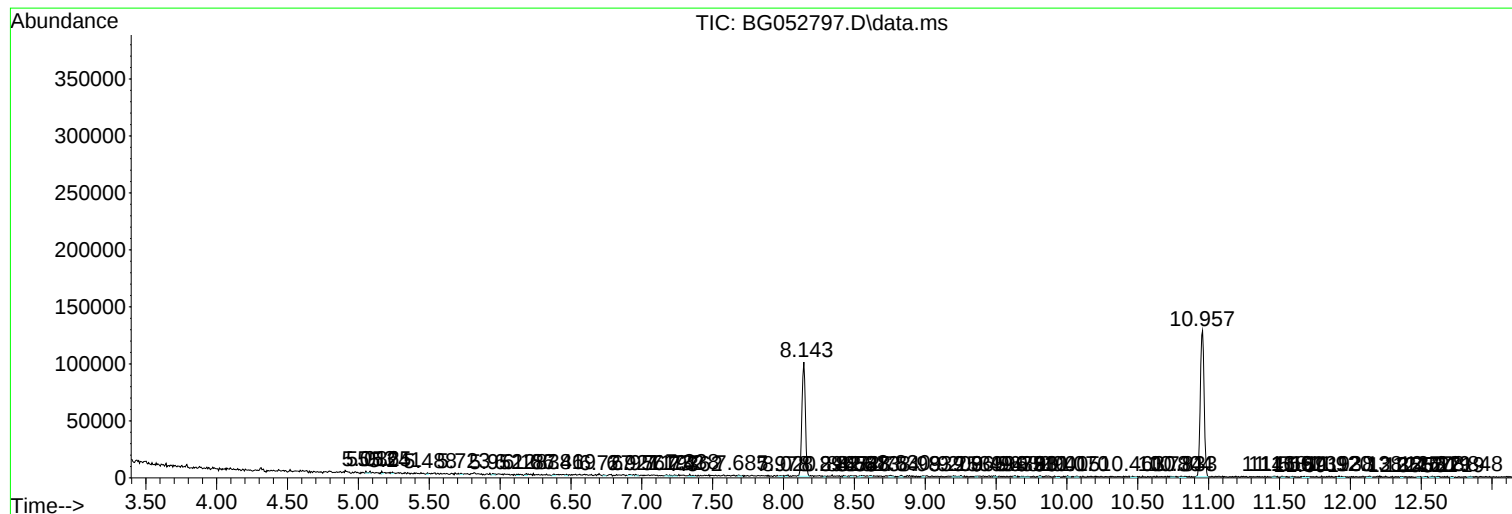

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052797.D
Acq On : 23 Mar 2022 14:41
Operator : CG/JU
Sample : N2026-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052797.D
Acq On : 23 Mar 2022 14:41
Operator : CG/JU
Sample : N2026-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc