

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052798.D
 Acq On : 23 Mar 2022 15:31
 Operator : CG/JU
 Sample : PB143536BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.552	24	28	34	rVB4	9162	14046	1.39%	0.138%
2	3.969	96	99	113	rBV	100491	174566	17.22%	1.717%
3	4.175	132	134	137	rVB3	1430	1182	0.12%	0.012%
4	4.263	147	149	151	rVB2	2387	1413	0.14%	0.014%
5	4.286	151	153	155	rBV	1358	1715	0.17%	0.017%
6	4.445	178	180	181	rVB2	2018	1135	0.11%	0.011%
7	4.468	181	184	186	rBV3	1463	1676	0.17%	0.016%
8	4.492	186	188	190	rBV2	1665	1674	0.17%	0.016%
9	4.598	204	206	209	rBV3	1778	1874	0.18%	0.018%
10	4.686	218	221	222	rVB2	1683	1280	0.13%	0.013%
11	5.097	287	291	293	rVB3	1218	1660	0.16%	0.016%
12	5.132	296	297	300	rVB2	1848	1393	0.14%	0.014%
13	5.167	300	303	305	rBV2	1934	2038	0.20%	0.020%
14	5.250	315	317	321	rVV3	798	1155	0.11%	0.011%
15	5.314	325	328	331	rVB2	1202	1273	0.13%	0.013%
16	5.344	331	333	336	rBV3	1316	1501	0.15%	0.015%
17	5.455	350	352	355	rVB4	1679	1560	0.15%	0.015%
18	5.520	361	363	366	rBV3	877	1172	0.12%	0.012%
19	5.585	373	374	379	rVB3	1175	1106	0.11%	0.011%
20	5.784	405	408	409	rVB3	1825	1407	0.14%	0.014%
21	5.843	416	418	419	rBV2	1774	1188	0.12%	0.012%
22	6.366	505	507	509	rVB2	1372	1108	0.11%	0.011%
23	6.389	509	511	513	rBV2	1335	1402	0.14%	0.014%
24	6.513	530	532	535	rVB3	1245	1153	0.11%	0.011%
25	7.077	624	628	630	rBV3	1271	1486	0.15%	0.015%
26	7.241	653	656	657	rBV	1616	1462	0.14%	0.014%
27	7.288	657	664	673	rVV	138461	239278	23.61%	2.353%
28	7.458	686	693	703	rBV	94876	166646	16.44%	1.639%
29	7.670	723	729	737	rVV	130113	220754	21.78%	2.171%
30	7.729	737	739	743	rVB2	1338	1711	0.17%	0.017%
31	7.970	776	780	784	rBV4	1543	2321	0.23%	0.023%
32	8.146	802	810	819	rVB	108335	190958	18.84%	1.878%
33	8.833	920	927	934	rBV	161997	277788	27.41%	2.732%
34	9.080	966	969	971	rBV	1087	1160	0.11%	0.011%
35	9.297	999	1006	1016	rVB	127648	233999	23.09%	2.301%
36	9.679	1070	1071	1074	rVB2	1506	1105	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052798.D
 Acq On : 23 Mar 2022 15:31
 Operator : CG/JU
 Sample : PB143536BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	10.026	1124	1130	1139	rBV2	109597	197727	19.51%	1.945%
38	10.331	1178	1182	1183	rBV	1187	1209	0.12%	0.012%
39	10.566	1215	1222	1230	rVV	163329	291441	28.76%	2.866%
40	10.654	1233	1237	1239	rVB	933	1131	0.11%	0.011%
41	10.954	1281	1288	1296	rVB	151844	276474	27.28%	2.719%
42	11.077	1302	1309	1319	rBV	163006	296319	29.24%	2.914%
43	11.999	1461	1466	1468	rBV2	930	1403	0.14%	0.014%
44	12.064	1472	1477	1480	rVV2	645	1337	0.13%	0.013%
45	12.117	1482	1486	1489	rVB2	1056	1136	0.11%	0.011%
46	12.528	1552	1556	1562	rVB2	2881	4417	0.44%	0.043%
47	12.745	1589	1593	1596	rBV2	1011	1205	0.12%	0.012%
48	14.161	1827	1834	1841	rBV	343919	504411	49.77%	4.961%
49	14.402	1874	1875	1878	rBV	1146	1397	0.14%	0.014%
50	14.461	1878	1885	1893	rVV	343988	564373	55.69%	5.551%
51	14.760	1929	1936	1945	rVB	259588	422169	41.66%	4.152%
52	14.931	1958	1965	1982	rBV	160536	276960	27.33%	2.724%
53	15.177	2004	2007	2008	rVB2	1212	1128	0.11%	0.011%
54	15.483	2058	2059	2064	rVB2	1001	1259	0.12%	0.012%
55	15.571	2071	2074	2079	rVB3	1071	1695	0.17%	0.017%
56	15.753	2098	2105	2112	rBV	469216	712974	70.35%	7.012%
57	15.853	2116	2122	2136	rBV	141480	221956	21.90%	2.183%
58	15.988	2141	2145	2151	rBV5	1692	2457	0.24%	0.024%
59	16.922	2300	2304	2308	rVB3	1361	1893	0.19%	0.019%
60	16.963	2308	2311	2313	rBV3	1261	1517	0.15%	0.015%
61	17.186	2345	2349	2352	rVB3	2018	2224	0.22%	0.022%
62	17.304	2365	2369	2370	rBV	1295	1239	0.12%	0.012%
63	17.404	2383	2386	2389	rBV3	936	1279	0.13%	0.013%
64	17.427	2389	2390	2396	rVV2	1054	1656	0.16%	0.016%
65	17.510	2396	2404	2411	rVB	361193	577045	56.94%	5.675%
66	17.604	2413	2420	2429	rBV	535718	843584	83.24%	8.297%
67	17.674	2429	2432	2433	rVV3	1357	1583	0.16%	0.016%
68	17.709	2436	2438	2441	rVB4	1201	1182	0.12%	0.012%
69	17.803	2453	2454	2457	rBV2	1341	1113	0.11%	0.011%
70	17.886	2466	2468	2472	rVV4	851	1134	0.11%	0.011%
71	17.938	2476	2477	2480	rVB2	1407	1308	0.13%	0.013%
72	18.291	2535	2537	2541	rBV4	1408	1862	0.18%	0.018%
73	18.455	2563	2565	2570	rBV4	1570	2045	0.20%	0.020%
74	18.696	2605	2606	2611	rVB4	1538	1676	0.17%	0.016%
75	18.743	2611	2614	2616	rBV4	2052	2590	0.26%	0.025%
76	18.831	2627	2629	2633	rVV3	1210	1520	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
 Data File : BG052798.D
 Acq On : 23 Mar 2022 15:31
 Operator : CG/JU
 Sample : PB143536BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	18.972	2652	2653	2655	rBV	2073	1607	0.16%	0.016%
78	19.078	2669	2671	2672	rBV2	1486	1526	0.15%	0.015%
79	19.383	2720	2723	2725	rBV3	2052	2512	0.25%	0.025%
80	19.454	2731	2735	2740	rBV5	8132	11351	1.12%	0.112%
81	19.519	2740	2746	2753	rBV4	7892	14111	1.39%	0.139%
82	19.566	2753	2754	2756	rBV2	2192	1509	0.15%	0.015%
83	19.642	2765	2767	2770	rBV4	2275	2246	0.22%	0.022%
84	19.724	2779	2781	2783	rBV3	1974	1246	0.12%	0.012%
85	19.795	2791	2793	2795	rVB3	2030	1687	0.17%	0.017%
86	19.889	2803	2809	2815	rVB	695742	1013481	100.00%	9.968%
87	19.983	2823	2825	2827	rBV	3817	2441	0.24%	0.024%
88	20.041	2834	2835	2836	rBV	2748	1141	0.11%	0.011%
89	20.094	2843	2844	2846	rBV2	2969	2616	0.26%	0.026%
90	20.218	2863	2865	2866	rBV2	2757	1887	0.19%	0.019%
91	20.259	2871	2872	2874	rBV2	3674	3030	0.30%	0.030%
92	20.412	2897	2898	2900	rBV	3766	3108	0.31%	0.031%
93	20.552	2920	2922	2924	rBV3	3080	2832	0.28%	0.028%
94	20.729	2950	2952	2954	rBV3	4991	4143	0.41%	0.041%
95	21.792	3127	3133	3142	rVB	391278	649236	64.06%	6.385%
96	22.538	3258	3260	3262	rBV3	7225	4648	0.46%	0.046%
97	24.177	3536	3539	3542	rBV5	8748	12027	1.19%	0.118%
98	24.882	3649	3659	3672	rVB3	339897	973373	96.04%	9.573%
99	25.111	3688	3698	3714	rVB	220465	660735	65.19%	6.498%
100	31.344	4757	4759	4760	rBV2	6315	5699	0.56%	0.056%




Sum of corrected areas: 10167565

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052798.D
Acq On : 23 Mar 2022 15:31
Operator : CG/JU
Sample : PB143536BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

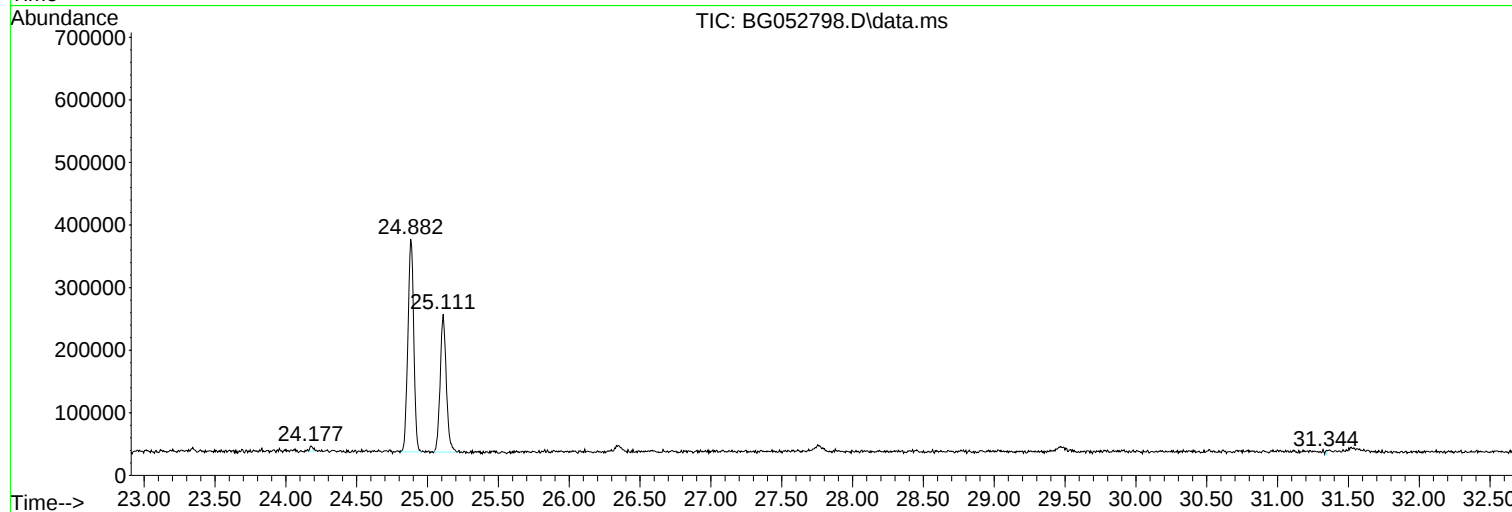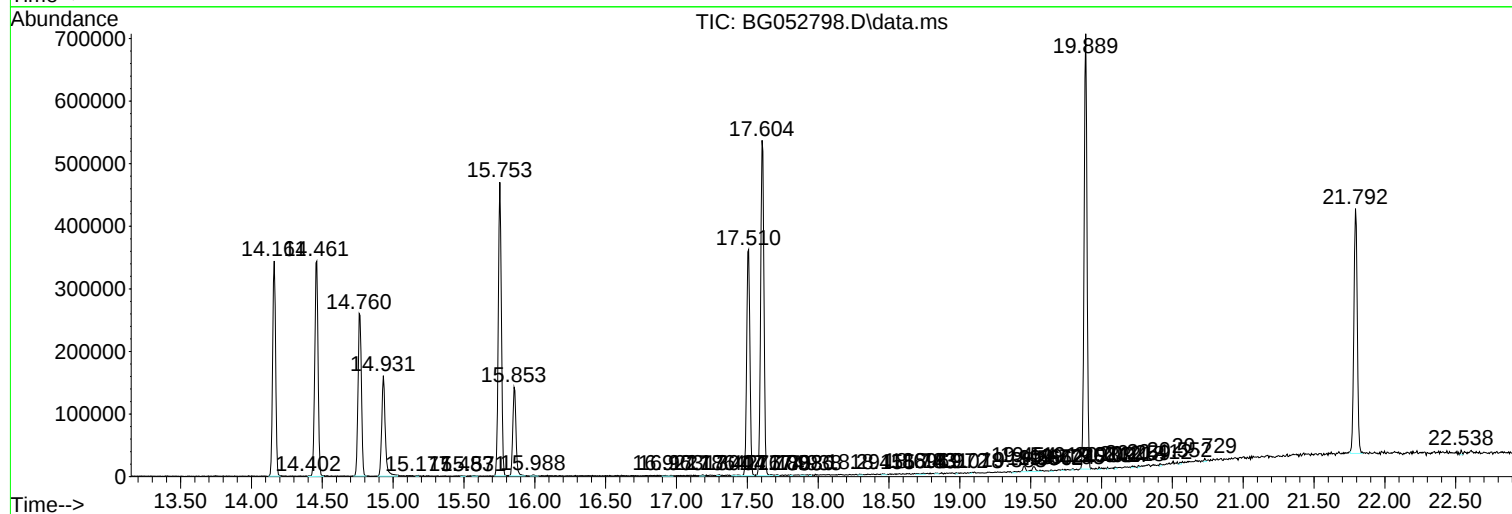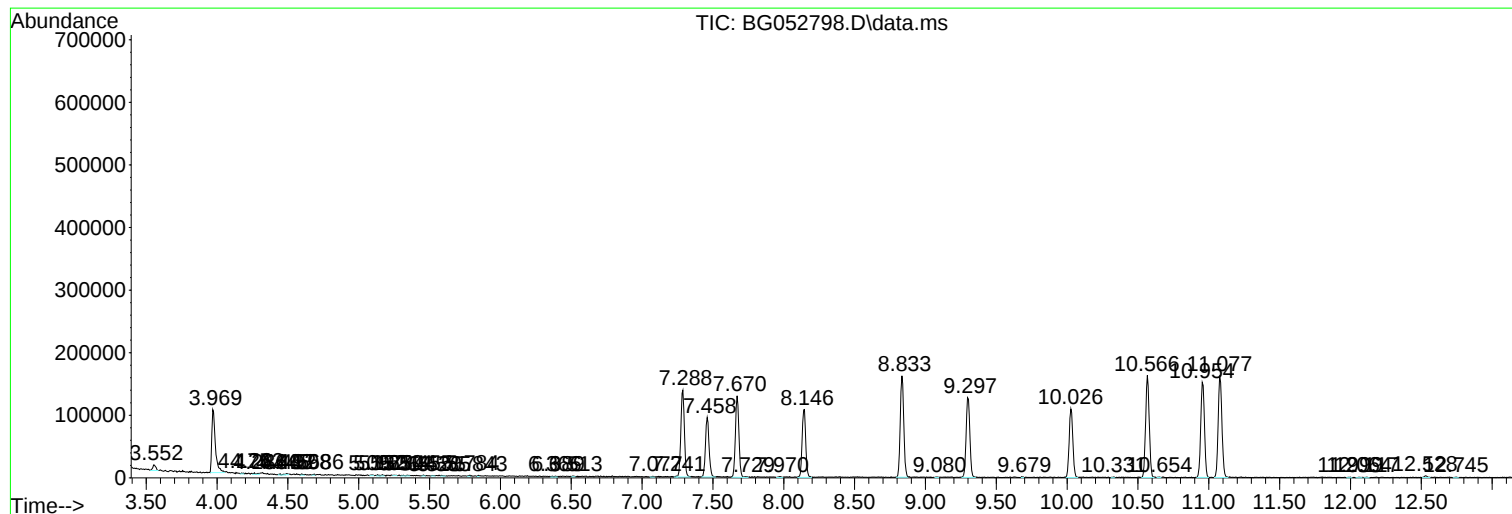

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052798.D
Acq On : 23 Mar 2022 15:31
Operator : CG/JU
Sample : PB143536BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032322\
Data File : BG052798.D
Acq On : 23 Mar 2022 15:31
Operator : CG/JU
Sample : PB143536BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
