

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032420\
 Data File : BG044936.D
 Acq On : 24 Mar 2020 18:47
 Operator : CG/JU
 Sample : PB127773BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB127773BL

Quant Time: Mar 25 05:15:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 23 07:18:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	79243	20.00	ng	-0.01
21) Naphthalene-d8	10.85	136	301474	20.00	ng	-0.01
39) Acenaphthene-d10	14.67	164	196992	20.00	ng	-0.01
64) Phenanthrene-d10	17.42	188	462204	20.00	ng	-0.01
76) Chrysene-d12	21.68	240	468978	20.00	ng	-0.02
87) Perylene-d12	24.88	264	489030	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	434395	85.33	ng	0.00
7) Phenol-d6	7.20	99	597661	80.81	ng	0.00
23) Nitrobenzene-d5	9.20	82	559912	81.50	ng	0.00
42) 2,4,6-Tribromophenol	16.16	330	247981	96.14	ng	-0.01
45) 2-Fluorobiphenyl	13.30	172	1204657	87.57	ng	0.00
79) Terphenyl-d14	20.03	244	2068709	82.51	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032420\
Data File : BG044936.D
Acq On : 24 Mar 2020 18:47
Operator : CG/JU
Sample : PB127773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB127773BL

Quant Time: Mar 25 05:15:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 23 07:18:46 2020
Response via : Initial Calibration

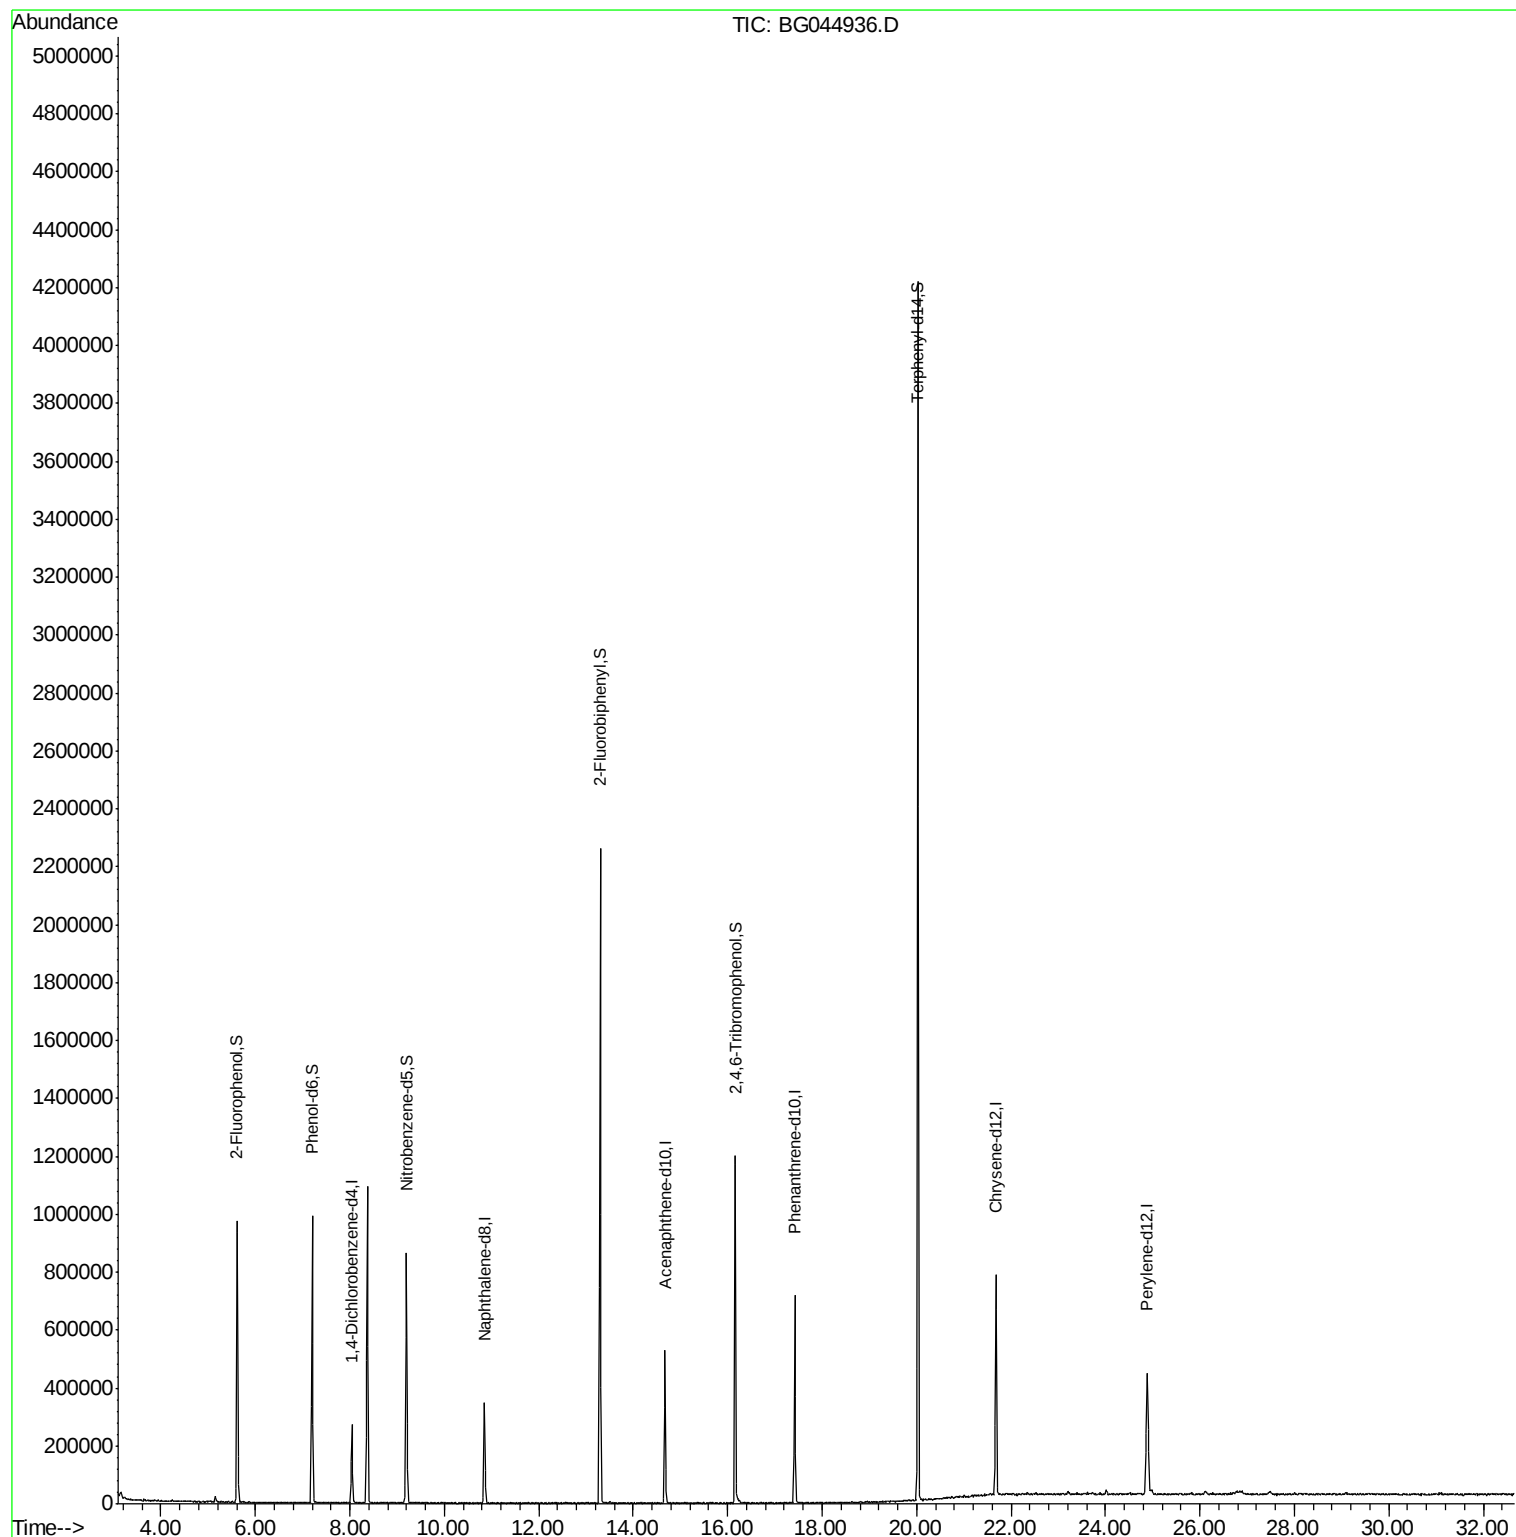

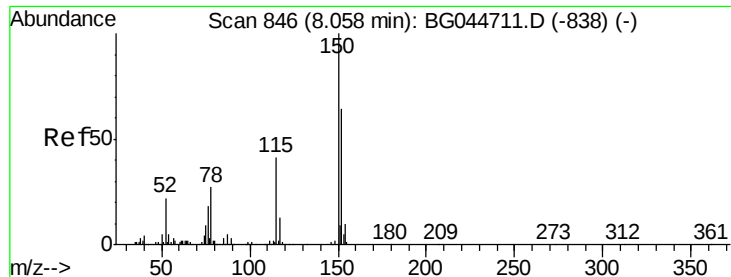


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.01 min
Lab File: BG044936.D
Acq: 24 Mar 2020 18:47

Instrument :
BNA_G
ClientSampleId :
PB127773BL

Tot Ion:152 Resp: 79243
Ion Ratio Lower Upper
152 100
150 157.9 128.8 193.2
115 58.8 52.6 79.0

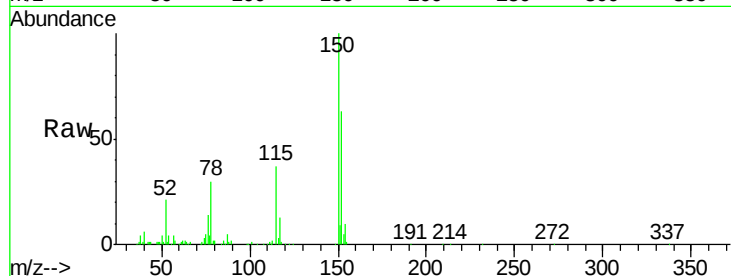


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

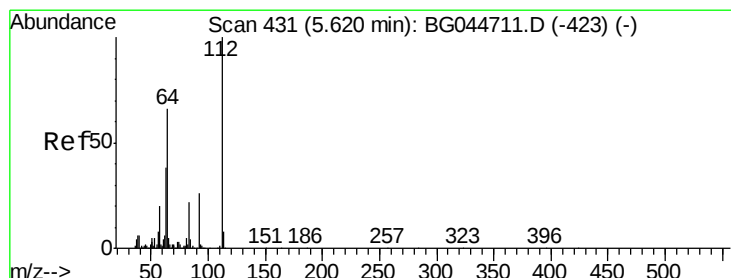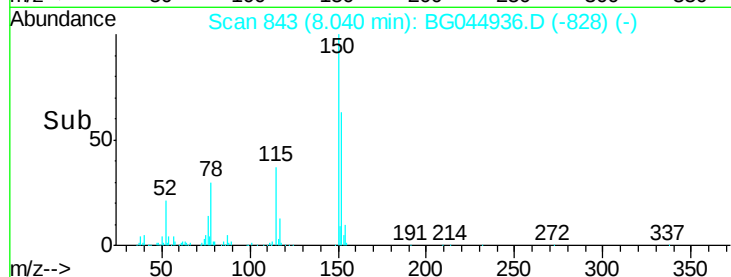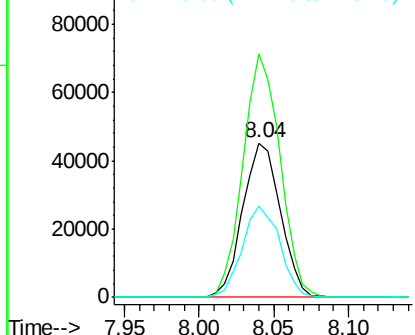



#5


2-Fluorophenol
Concen: 85.335 ng
RT: 5.61 min Scan# 430
Delta R.T. 0.00 min
Lab File: BG044936.D
Acq: 24 Mar 2020 18:47

Tgt Ion:112 Resp: 434395
Ion Ratio Lower Upper
112 100
64 65.1 53.4 80.2
63 36.2 29.4 44.2

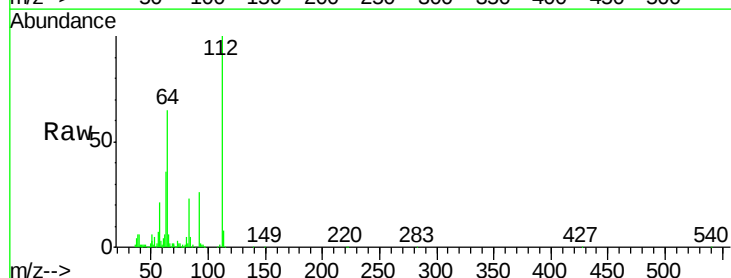

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

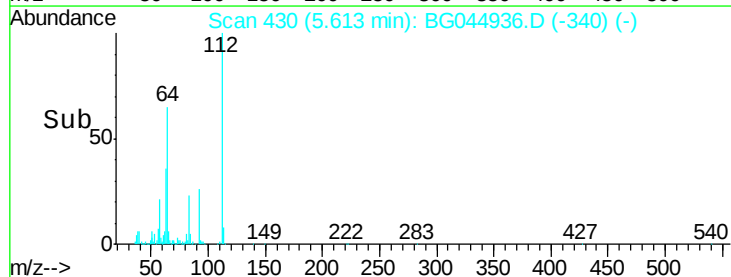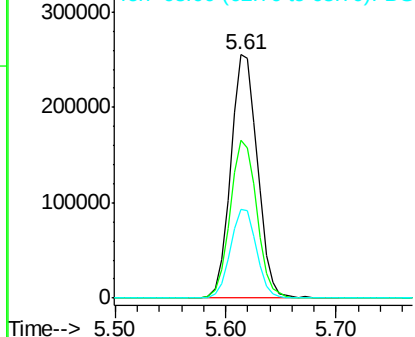

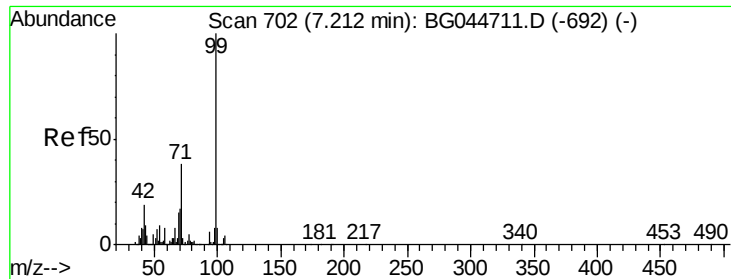

#7

Phenol-d6

Concen: 80.808 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.01 min

Lab File: BG044936.D

Acq: 24 Mar 2020 18:47

Instrument :

BNA_G

ClientSampleId :

PB127773BL


Tot Ion: 99 Resp: 597661

Ion Ratio Lower Upper




99 100

42 16.1 12.6 19.0

71 37.0 29.0 43.4

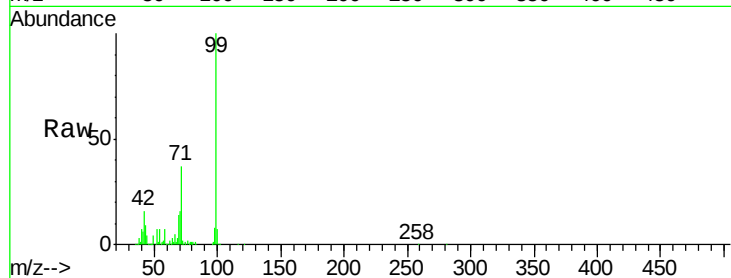

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

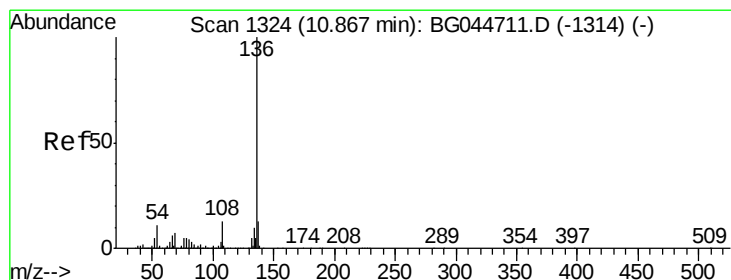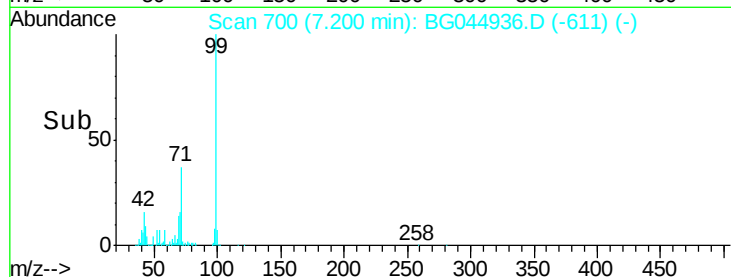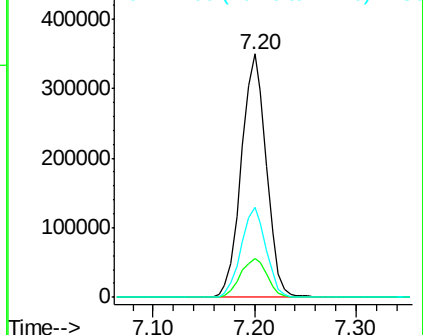

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1321

Delta R.T. -0.01 min

Lab File: BG044936.D

Acq: 24 Mar 2020 18:47

Tgt Ion: 136 Resp: 301474


Ion Ratio Lower Upper

136 100



137 9.7 9.8 14.6#


54 9.5 7.9 11.9

68 6.6 5.4 8.0

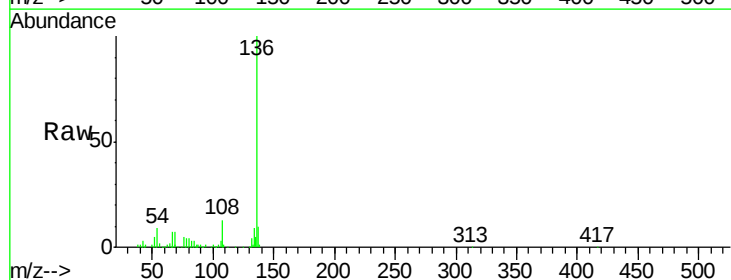

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



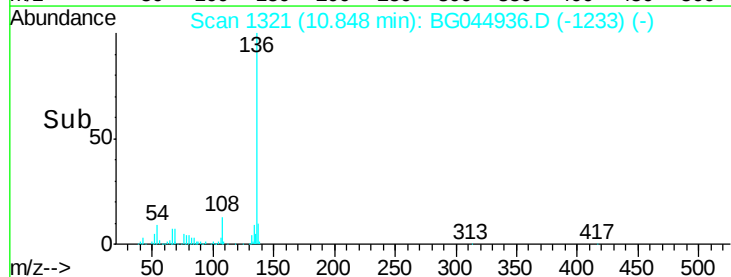
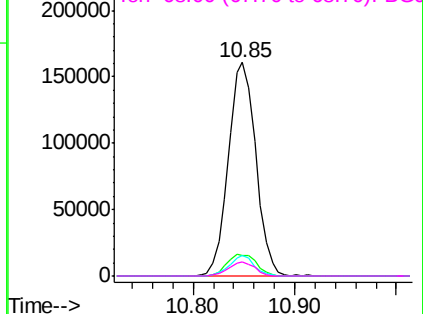


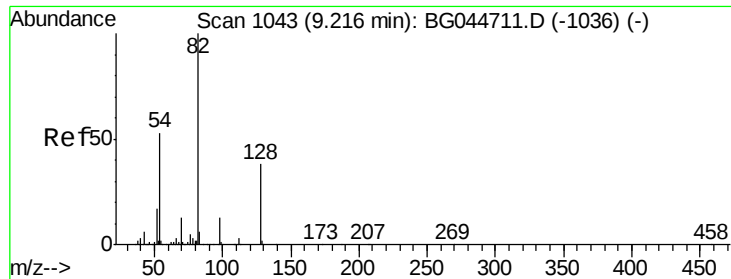

#23
 Nitrobenzene-d5
 Concen: 81.499 ng
 RT: 9.20 min Scan# 1040
 Delta R.T. -0.01 min
 Lab File: BG044936.D
 Acq: 24 Mar 2020 18:47




Instrument :
 BNA_G
 ClientSampleId :
 PB127773BL


Tot Ion	Ratio	Lower	Upper
82	100		
128	38.7	30.6	46.0
54	50.7	37.1	55.7

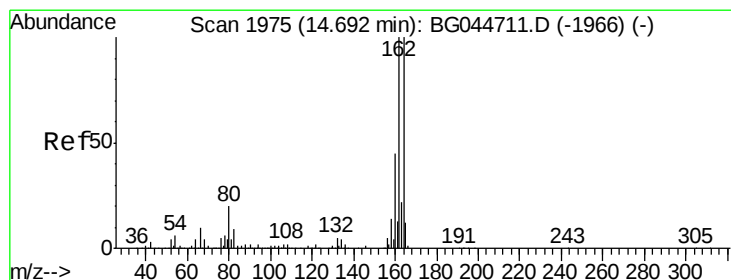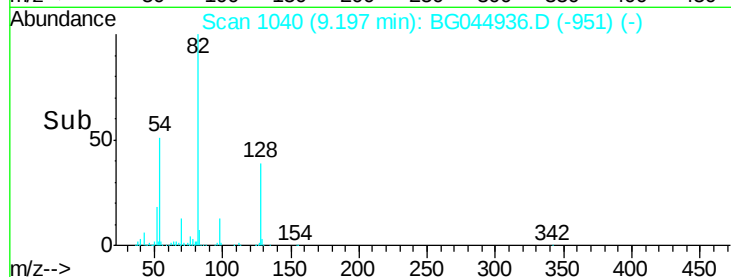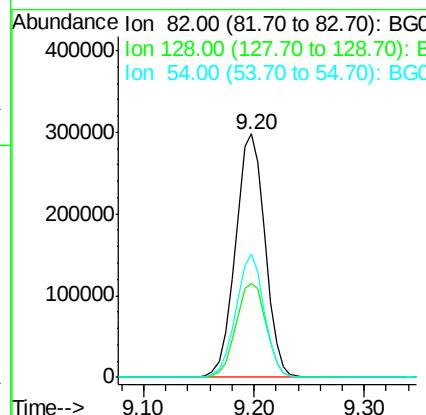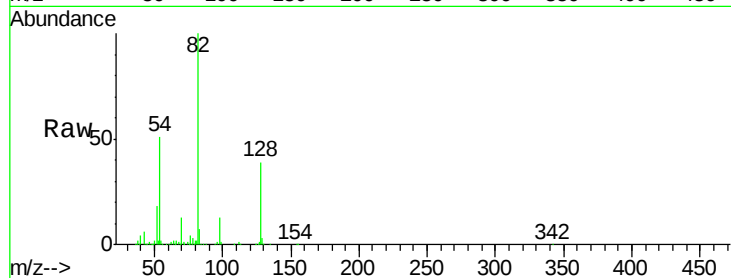

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.67 min Scan# 1972
 Delta R.T. -0.01 min
 Lab File: BG044936.D
 Acq: 24 Mar 2020 18:47

Tgt Ion	Ratio	Lower	Upper
164	100		
162	98.4	76.7	115.1
160	46.2	35.0	52.4


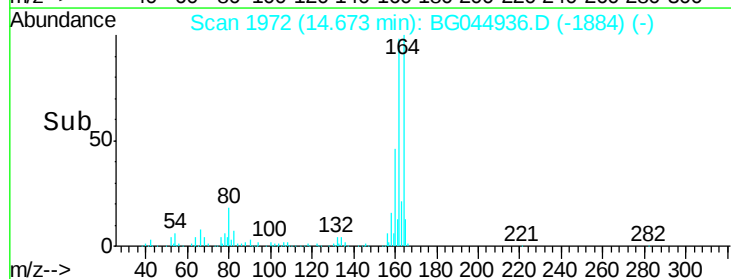
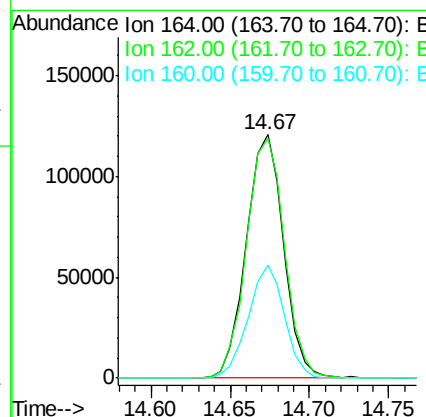
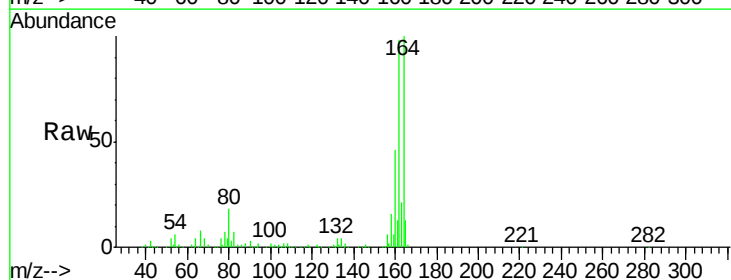


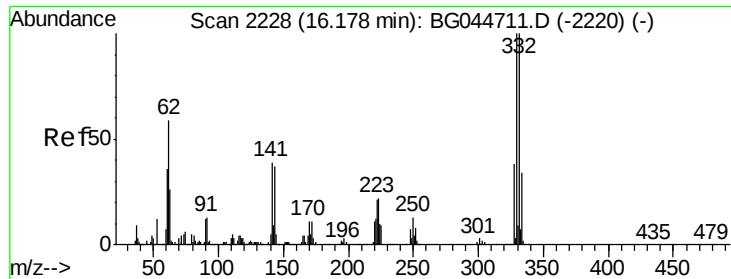

#42
2,4,6-Tribromophenol
Concen: 96.142 ng
RT: 16.16 min Scan# 2225
Delta R.T. -0.01 min
Lab File: BG044936.D
Acq: 24 Mar 2020 18:47




Instrument :
BNA_G
ClientSampleId :
PB127773BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	77.8	116.6
141	36.1	29.5	44.3

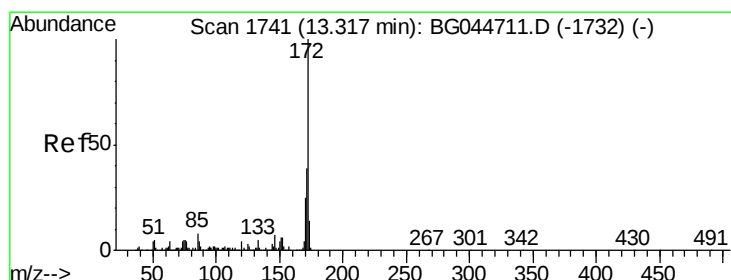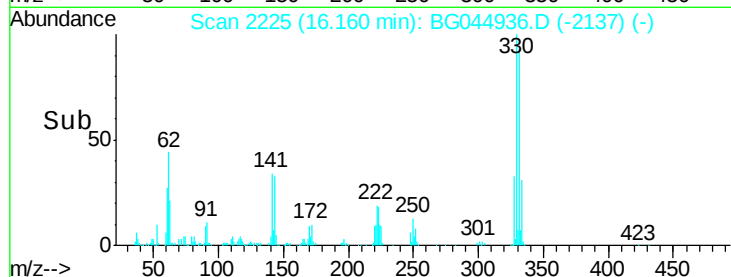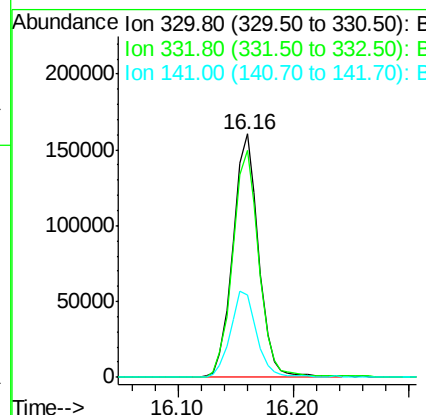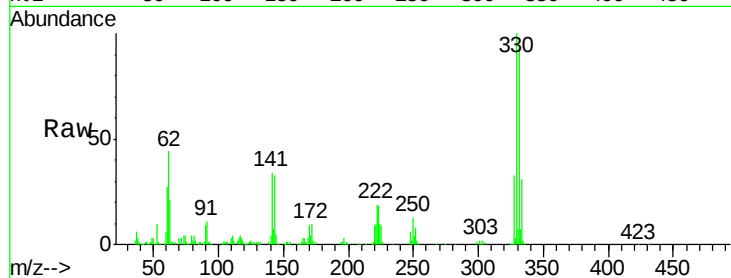

#45
2-Fluorobiphenyl
Concen: 87.573 ng
RT: 13.30 min Scan# 1738
Delta R.T. -0.01 min
Lab File: BG044936.D
Acq: 24 Mar 2020 18:47

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	28.7	43.1
170	24.4	19.0	28.6

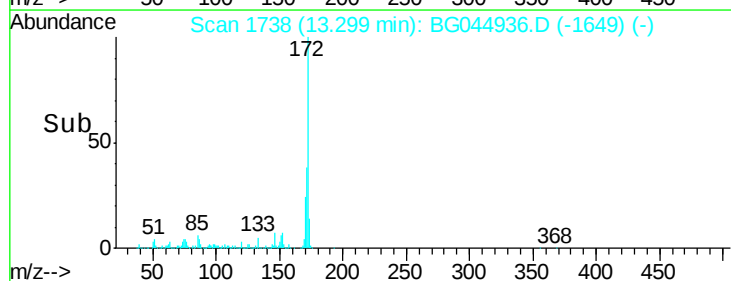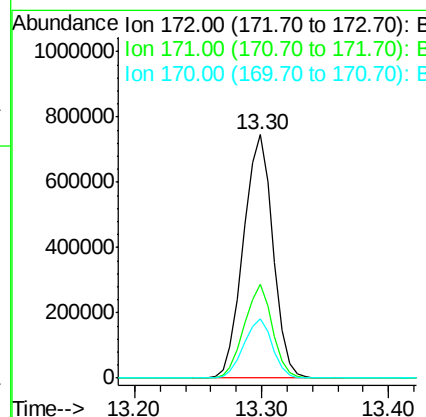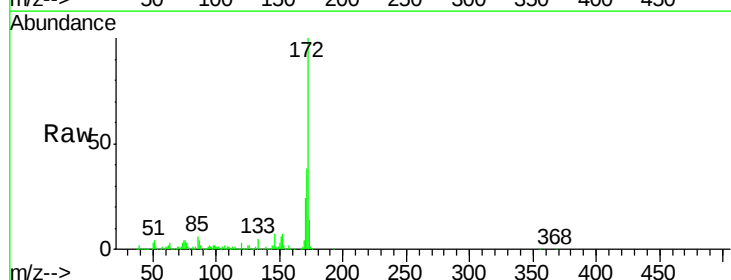

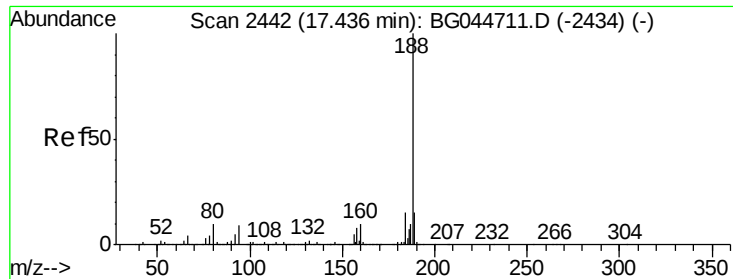

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2439

Delta R.T. -0.01 min

Lab File: BG044936.D

Acq: 24 Mar 2020 18:47

Instrument :

BNA_G

ClientSampleId :

PB127773BL


Tot Ion:188 Resp: 462204

Ion Ratio Lower Upper

188 100

94 8.0 7.3 10.9




80 8.4 8.0 12.0

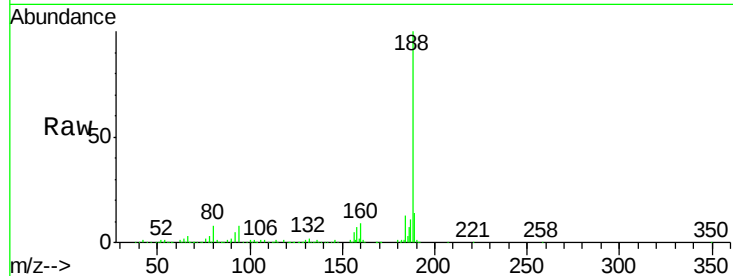

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

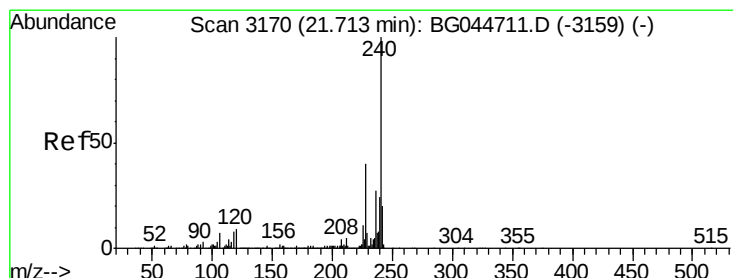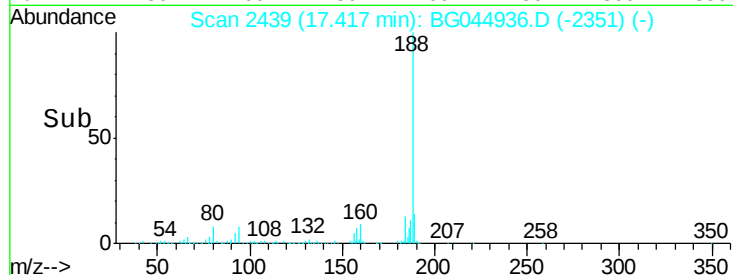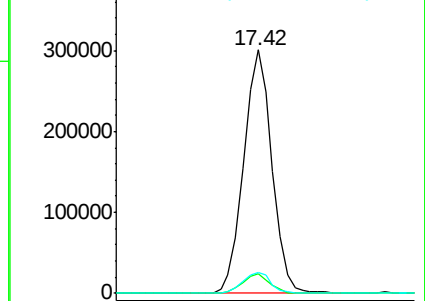

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.68 min Scan# 3165

Delta R.T. -0.02 min

Lab File: BG044936.D

Acq: 24 Mar 2020 18:47


Tgt Ion:240 Resp: 468978

Ion Ratio Lower Upper

240 100

120 8.9 6.7 10.1



236 25.7 21.5 32.3

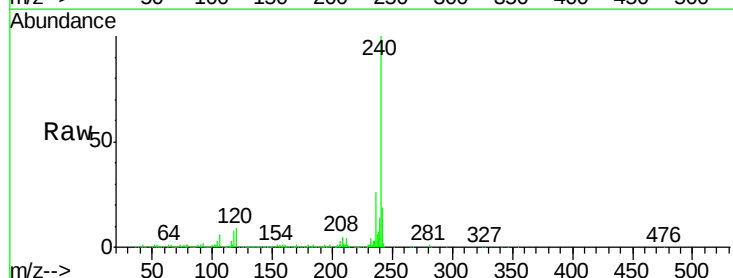


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

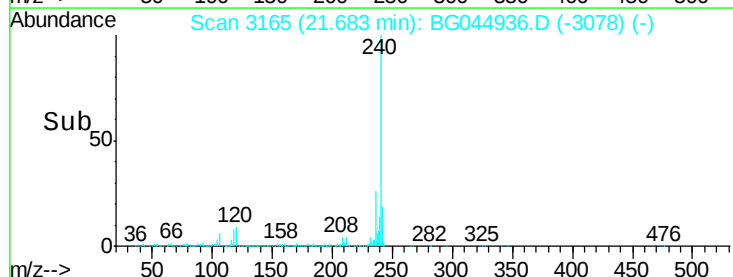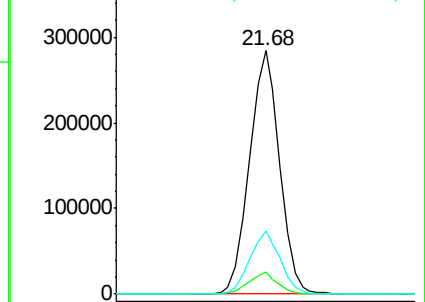

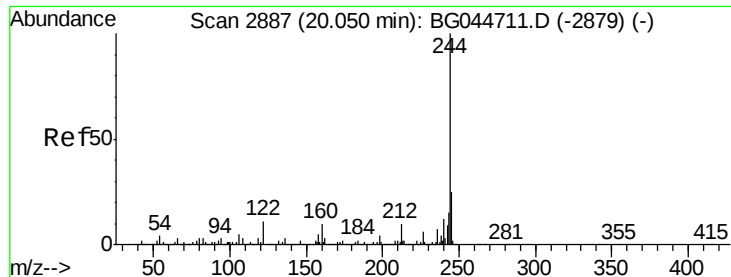

#79

Terphenyl-d14

Concen: 82.512 ng

RT: 20.03 min Scan# 2883

Delta R.T. -0.01 min

Lab File: BG044936.D

Acq: 24 Mar 2020 18:47

Instrument :

BNA_G

ClientSampleId :

PB127773BL


Tot Ion:244 Resp: 2068709

Ion Ratio Lower Upper

244 100

212 9.0 7.7 11.5




122 9.6 8.6 12.8

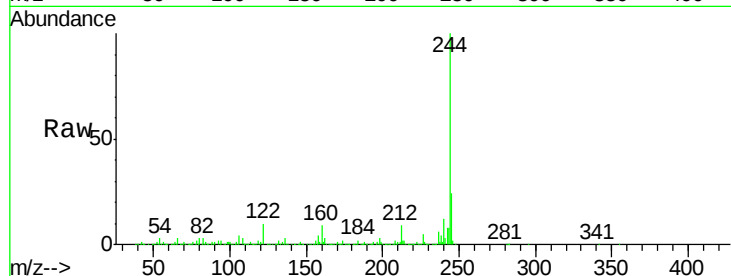

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

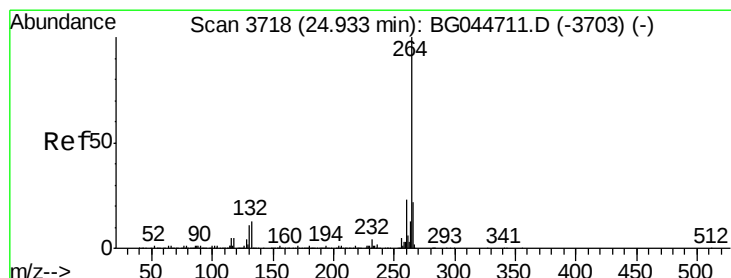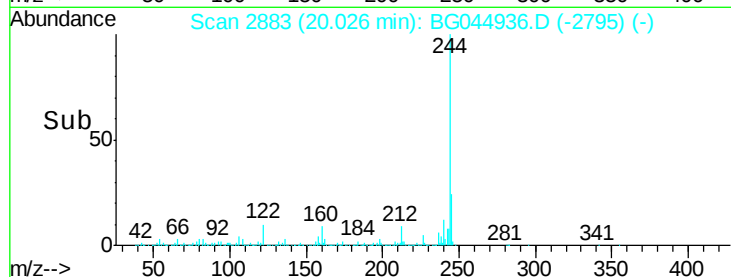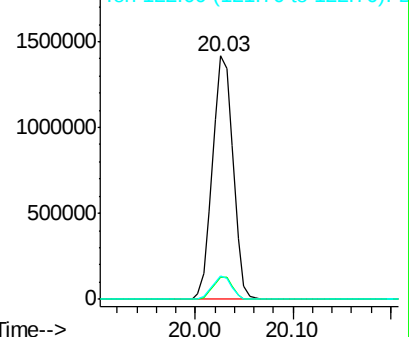

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.88 min Scan# 3710

Delta R.T. -0.02 min

Lab File: BG044936.D

Acq: 24 Mar 2020 18:47


Tgt Ion:264 Resp: 489030

Ion Ratio Lower Upper

264 100

260 22.8 18.1 27.1

265 21.9 17.1 25.7

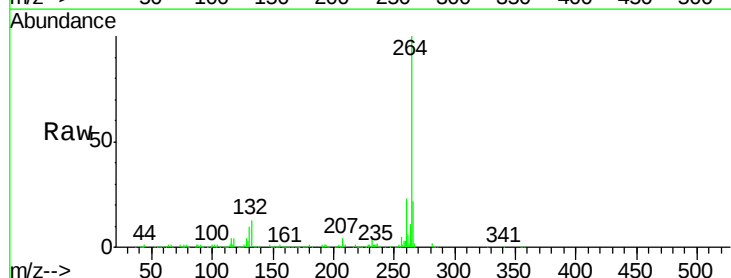

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

