

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032420\
 Data File : BG044936.D
 Acq On : 24 Mar 2020 18:47
 Operator : CG/JU
 Sample : PB127773BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB127773BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	19	rVB5	22171	60565	1.02%	0.251%
2	5.613	423	430	441	rVB	969560	1623609	27.39%	6.737%
3	7.200	692	700	712	rBV	989351	1707786	28.81%	7.086%
4	8.040	836	843	851	rVB	271280	478100	8.07%	1.984%
5	8.369	890	899	908	rBV	1094123	1972980	33.29%	8.187%
6	9.197	1028	1040	1050	rBV	862185	1607157	27.12%	6.669%
7	10.848	1313	1321	1330	rBV	347063	646168	10.90%	2.681%
8	13.299	1730	1738	1750	rBV	2261851	3591377	60.59%	14.902%
9	14.673	1963	1972	1980	rBV2	528158	877413	14.80%	3.641%
10	16.160	2217	2225	2238	rBV	1200977	1948150	32.87%	8.084%
11	17.417	2429	2439	2447	rBV	716531	1115662	18.82%	4.629%
12	20.026	2877	2883	2895	rBV	4209207	5927168	100.00%	24.595%
13	21.683	3158	3165	3172	rBV2	759378	1268860	21.41%	5.265%
14	24.885	3698	3710	3721	rBV2	419931	1274242	21.50%	5.287%


Sum of corrected areas: 24099237

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032420\
Data File : BG044936.D
Acq On : 24 Mar 2020 18:47
Operator : CG/JU
Sample : PB127773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB127773BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

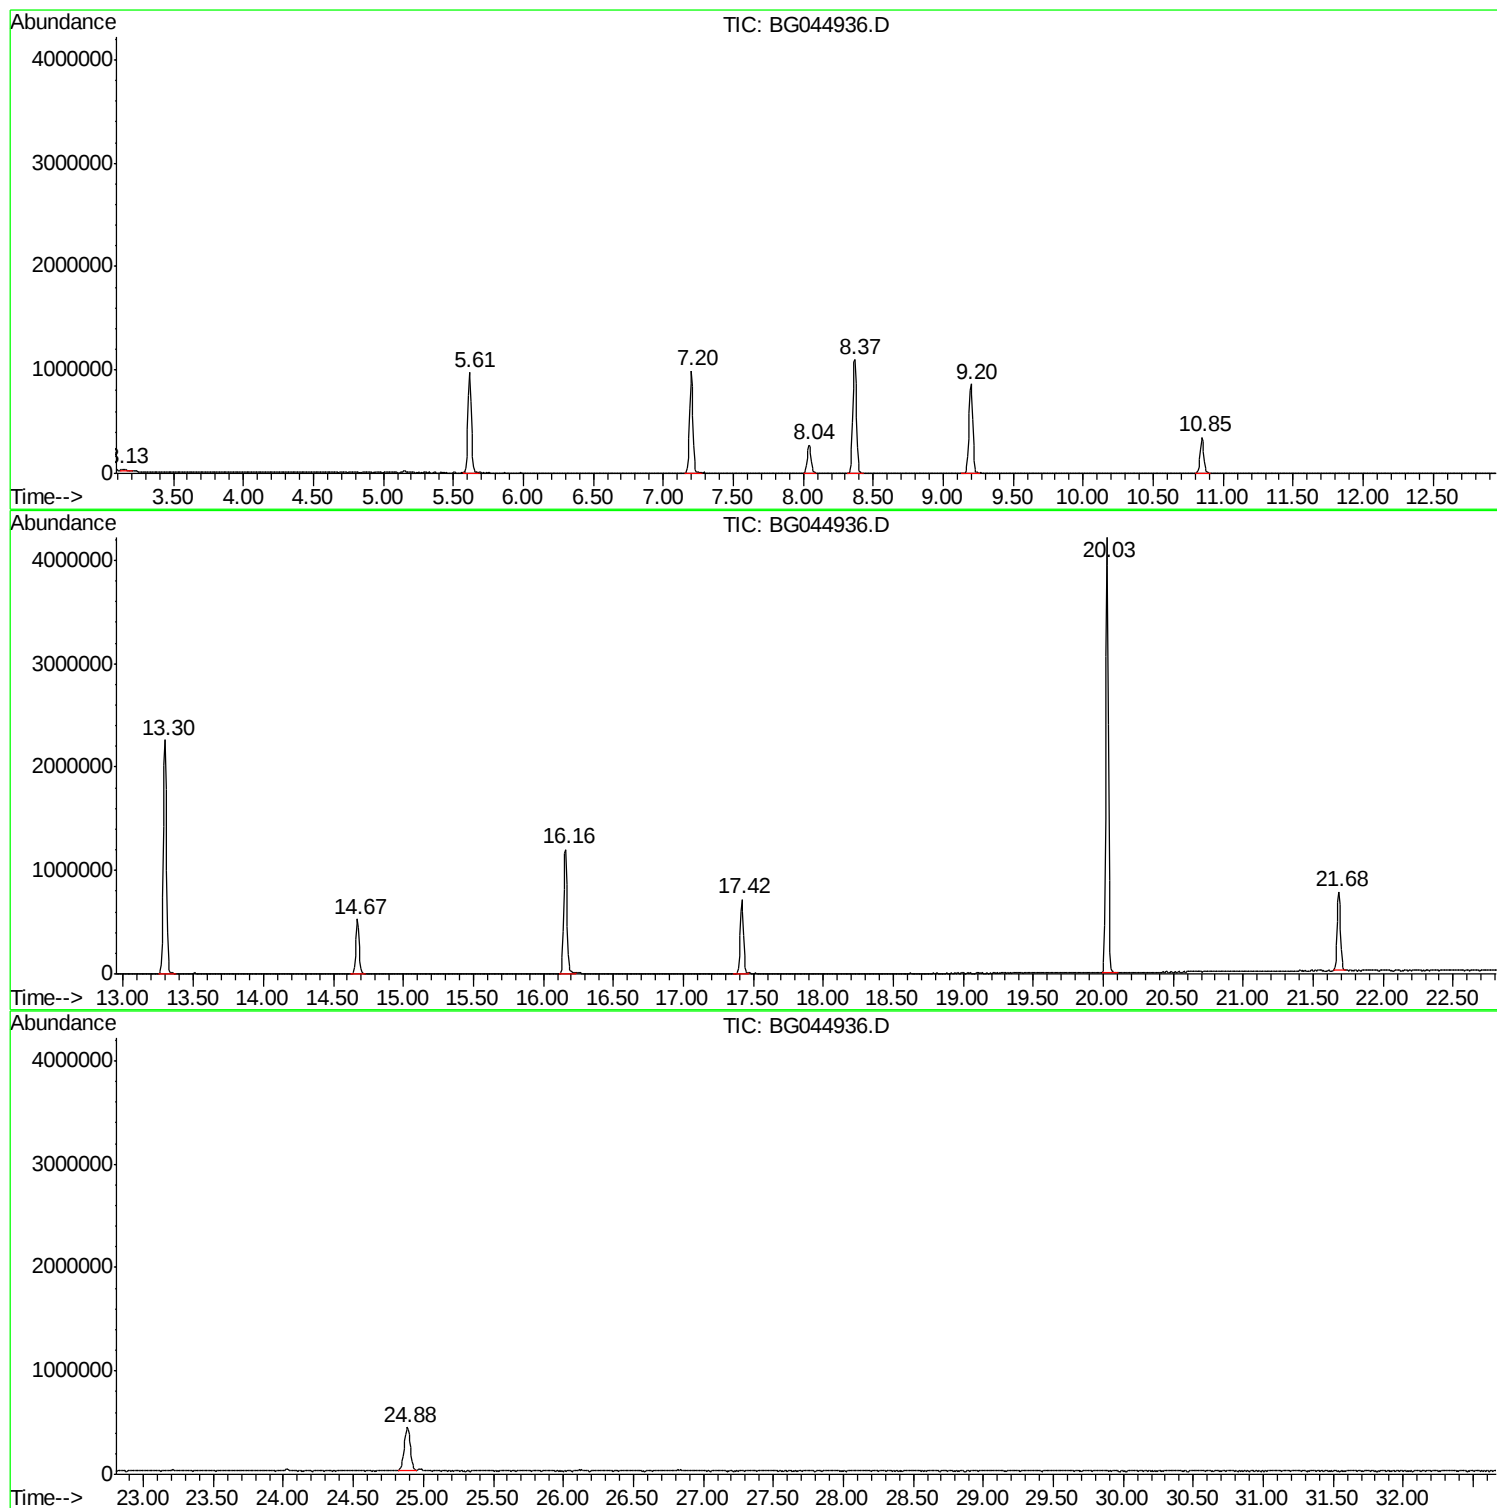

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032420\
Data File : BG044936.D
Acq On : 24 Mar 2020 18:47
Operator : CG/JU
Sample : PB127773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB127773BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032420\
Data File : BG044936.D
Acq On : 24 Mar 2020 18:47
Operator : CG/JU
Sample : PB127773BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB127773BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc