


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG032420\
 Data File : BG044927.D
 Acq On : 24 Mar 2020 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 23 07:18:46 2020

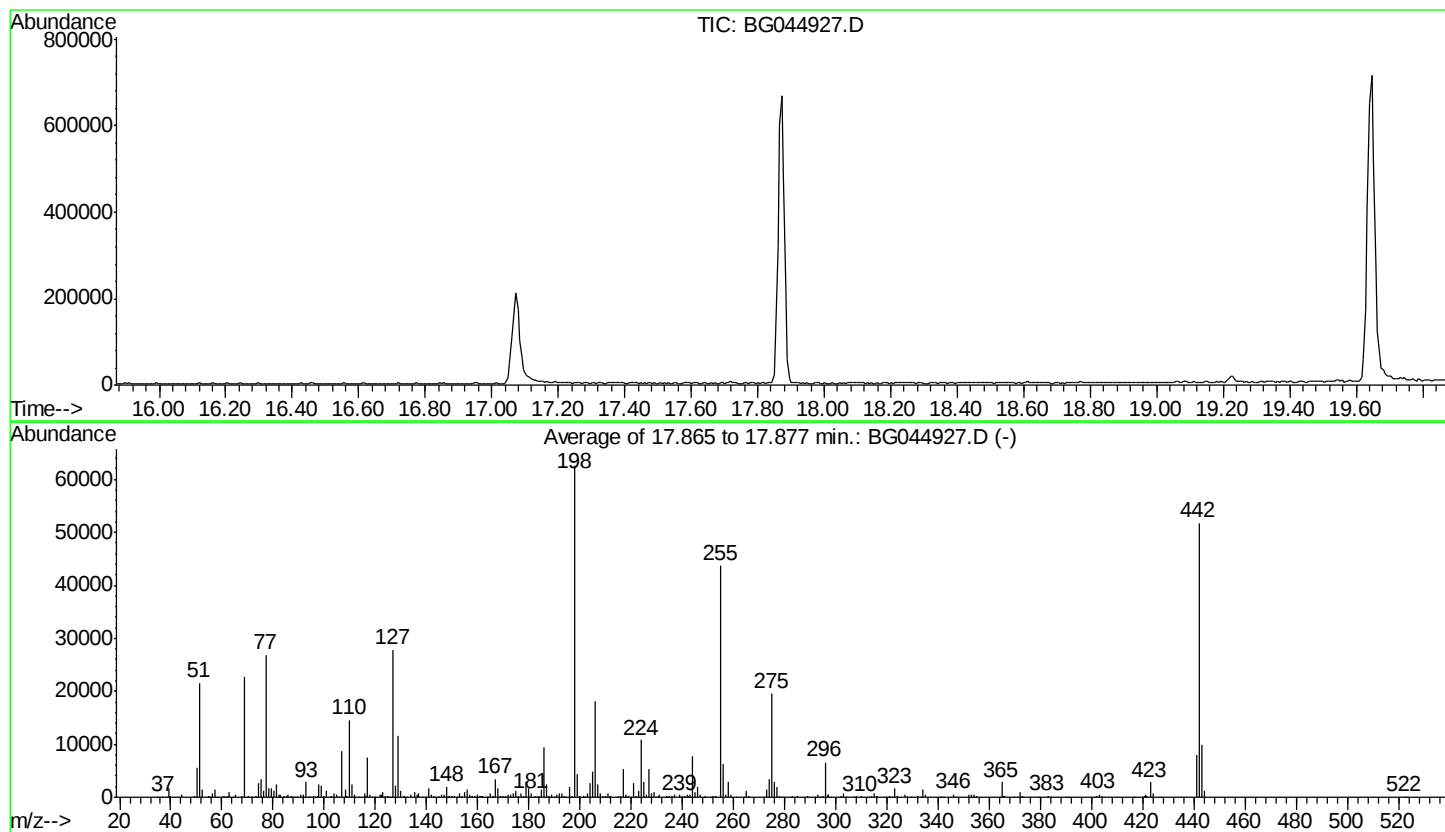

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	21597	PASS
68	69	0.00	2	0.8	189	PASS
69	198	0.00	100	36.1	22613	PASS
70	69	0.00	2	0.7	159	PASS
127	198	10	80	44.5	27856	PASS
197	198	0.00	2	0.3	214	PASS
198	198	100	100	100.0	62605	PASS
199	198	5	9	7.0	4365	PASS
275	198	10	60	31.1	19490	PASS
365	198	1	100	4.5	2847	PASS
441	198	0.01	100	12.9	8070	PASS
442	198	50	100	82.8	51824	PASS
443	442	15	24	19.0	9823	PASS