


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032420\
 Data File : BG044942.D
 Acq On : 24 Mar 2020 22:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 23 07:18:46 2020

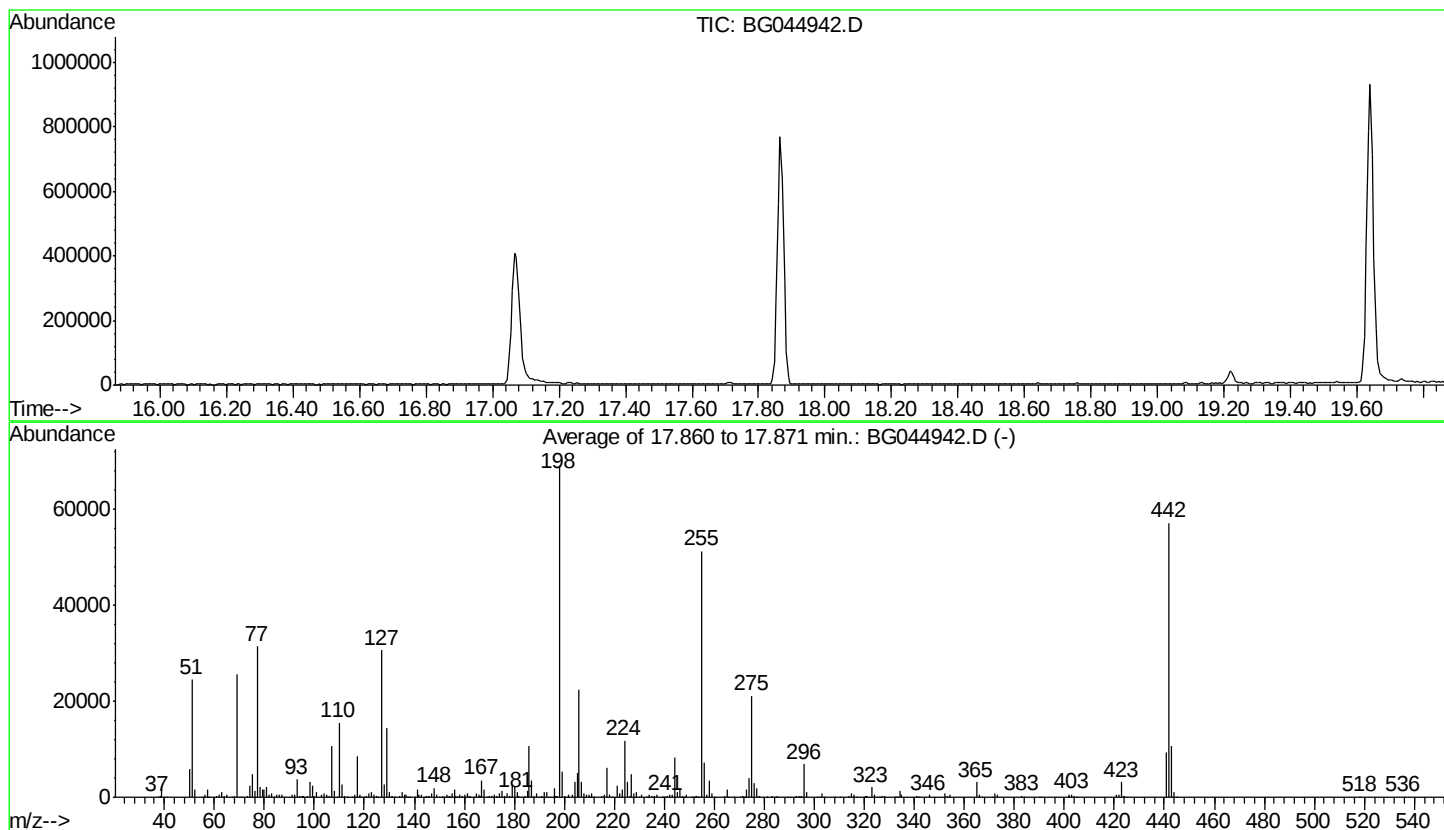

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	24464	PASS
68	69	0.00	2	1.2	300	PASS
69	198	0.00	100	37.2	25672	PASS
70	69	0.00	2	0.3	81	PASS
127	198	10	80	44.4	30664	PASS
197	198	0.00	2	0.4	306	PASS
198	198	100	100	100.0	69088	PASS
199	198	5	9	7.6	5284	PASS
275	198	10	60	30.5	21072	PASS
365	198	1	100	4.5	3093	PASS
441	198	0.01	100	13.7	9466	PASS
442	198	50	100	82.7	57117	PASS
443	442	15	24	18.8	10760	PASS