
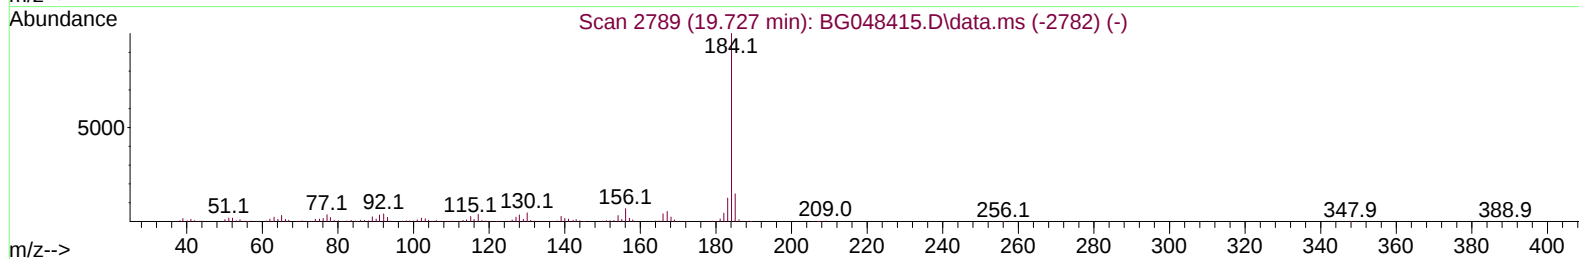
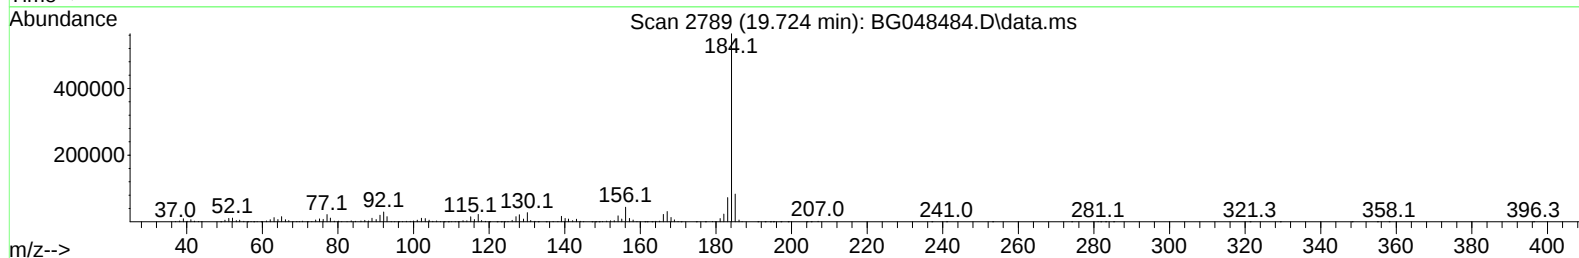


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048484.D
Acq On : 24 Mar 2021 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 02:04:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:36:47 2021
Response via : Initial Calibration

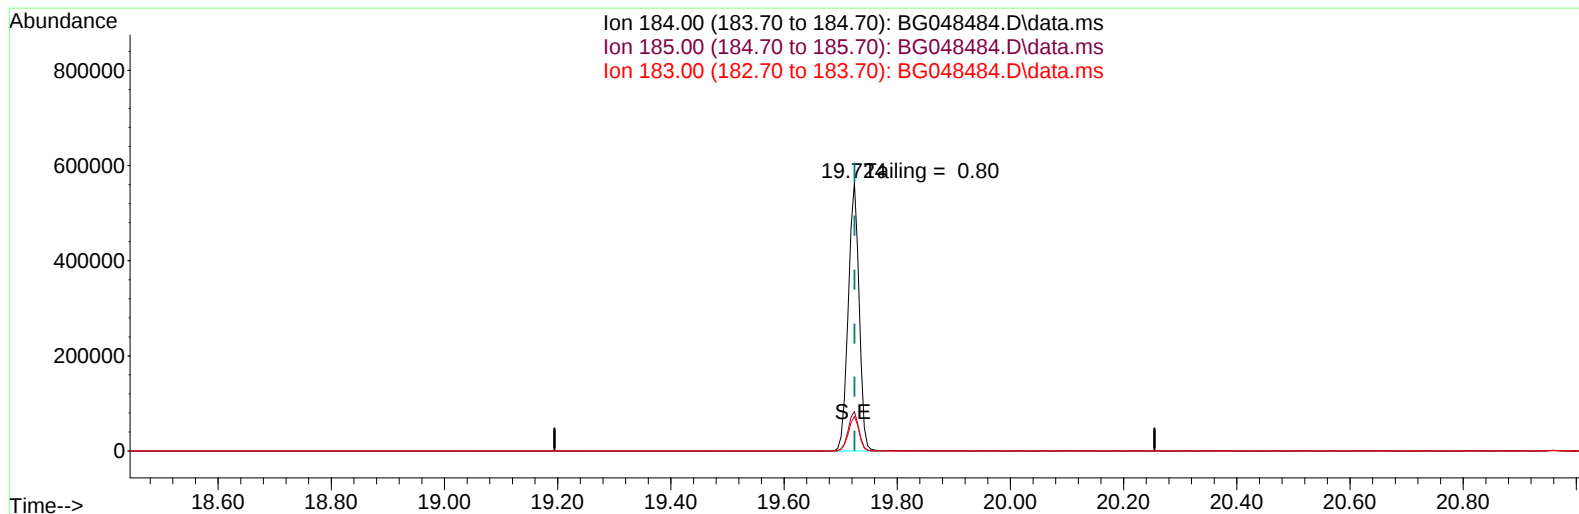




TIC: BG048484.D\data.ms

(77) Benzidine**19.724min (-0.000) 145936.09 ng****response 751896**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	12.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048484.D
Acq On : 24 Mar 2021 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 02:04:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:36:47 2021
Response via : Initial Calibration

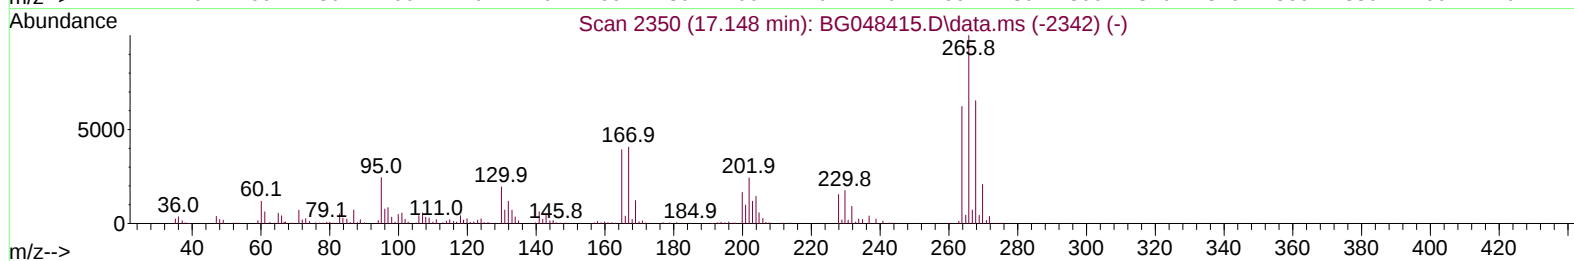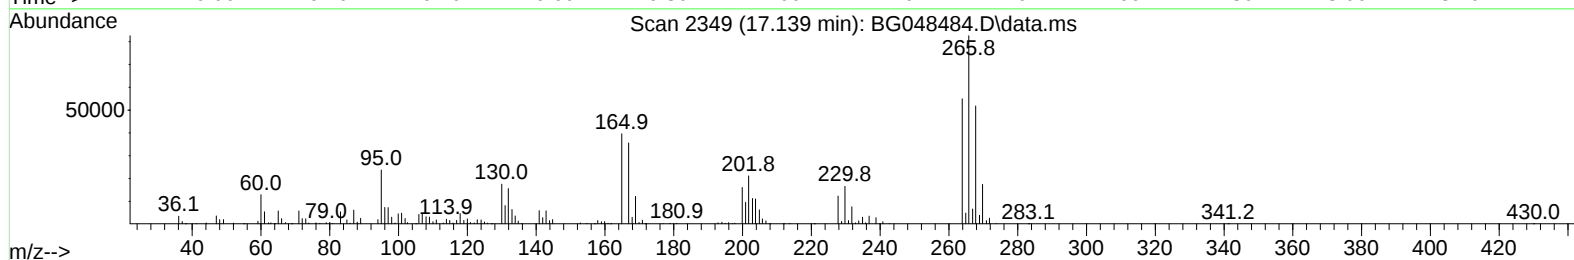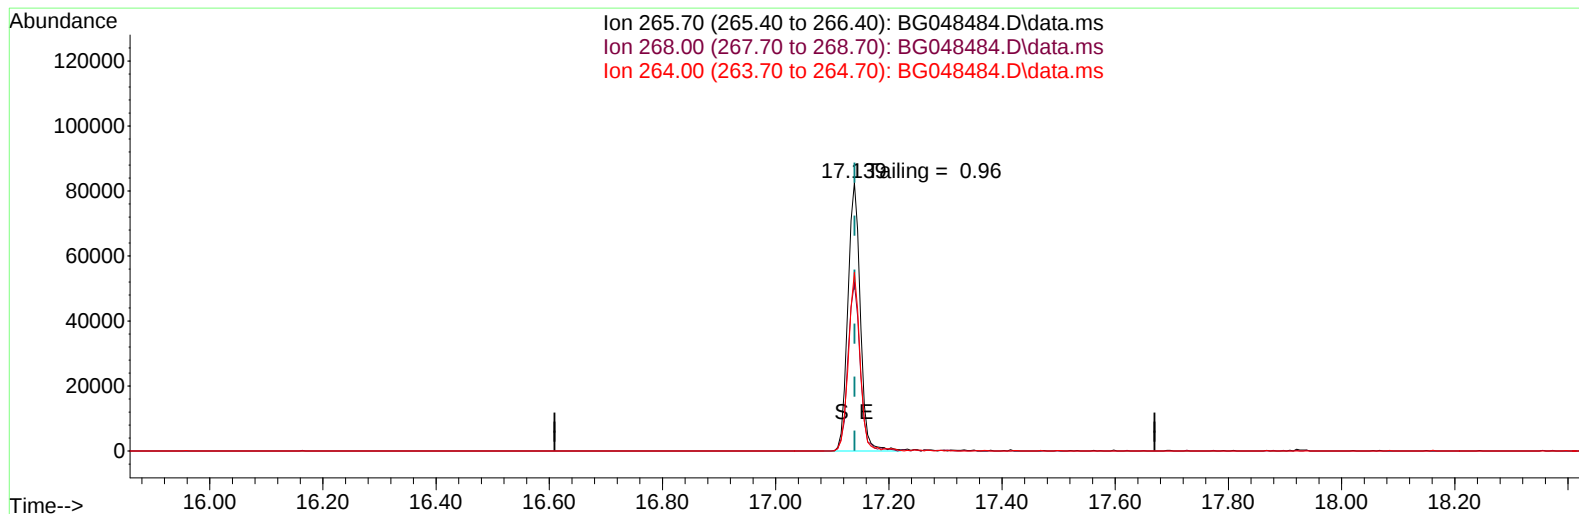

TIC: BG048484.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.000) 15311.74 ng

response 125278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.72
264.00	61.60	66.50
0.00	0.00	0.00