

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
 Data File : BG048488.D
 Acq On : 24 Mar 2021 14:15
 Operator : CG/JU
 Sample : M1718-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.655	387	394	403	rBV	564537	906881	28.16%	4.275%
2	7.253	656	666	678	rBV	590581	1059631	32.91%	4.994%
3	8.099	804	810	817	rBV	208140	352159	10.94%	1.660%
4	9.269	1001	1009	1018	rBV	409216	729312	22.65%	3.438%
5	10.920	1282	1290	1297	rBV	261756	485179	15.07%	2.287%
6	13.364	1698	1706	1713	rBV	1077141	1595915	49.56%	7.522%
7	14.186	1840	1846	1851	rBV	31052	46617	1.45%	0.220%
8	14.745	1933	1941	1947	rBV	448767	695233	21.59%	3.277%
9	15.097	1990	2001	2002	rBV8	20987	49421	1.53%	0.233%
10	15.168	2007	2013	2014	rBV2	20828	34855	1.08%	0.164%
11	15.279	2024	2032	2034	rBV2	100910	233965	7.27%	1.103%
12	15.814	2098	2123	2124	rBV2	301771	1106804	34.37%	5.217%
13	16.231	2172	2194	2198	rBV	1270291	3219903	100.00%	15.177%
14	16.678	2255	2270	2285	rVB2	104261	589832	18.32%	2.780%
15	17.494	2403	2409	2414	rBV	532209	799912	24.84%	3.770%
16	18.158	2511	2522	2534	rBV6	86916	369930	11.49%	1.744%
17	18.370	2553	2558	2565	rBV	156742	226747	7.04%	1.069%
18	19.139	2685	2689	2694	rVB	73326	93950	2.92%	0.443%
19	19.574	2756	2763	2770	rVV2	192970	444886	13.82%	2.097%
20	19.639	2771	2774	2780	rVB6	49255	58354	1.81%	0.275%
21	20.103	2847	2853	2859	rVB	1682073	2224894	69.10%	10.487%
22	20.555	2924	2930	2937	rVB2	230757	438928	13.63%	2.069%
23	20.749	2957	2963	2971	rVB4	92013	225679	7.01%	1.064%
24	21.366	3062	3068	3073	rBV2	118728	254592	7.91%	1.200%
25	21.437	3073	3080	3086	rVV3	404840	986230	30.63%	4.649%
26	21.496	3086	3090	3099	rVV	588881	896368	27.84%	4.225%
27	21.578	3102	3104	3107	rVB2	42075	45382	1.41%	0.214%
28	21.783	3133	3139	3145	rVB	477469	800295	24.85%	3.772%
29	22.465	3249	3255	3261	rVB3	131755	285157	8.86%	1.344%
30	22.606	3276	3279	3283	rBV4	33553	48714	1.51%	0.230%
31	23.329	3398	3402	3408	rVB7	40809	78139	2.43%	0.368%
32	23.675	3453	3461	3470	rVB3	131558	358195	11.12%	1.688%
33	24.010	3516	3518	3534	rVB8	95637	273972	8.51%	1.291%
34	24.163	3542	3544	3553	rVB6	32529	66360	2.06%	0.313%
35	25.115	3697	3706	3720	rVB2	329707	1133680	35.21%	5.343%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048488.D
Acq On : 24 Mar 2021 14:15
Operator : CG/JU
Sample : M1718-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 21216071

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048488.D
Acq On : 24 Mar 2021 14:15
Operator : CG/JU
Sample : M1718-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

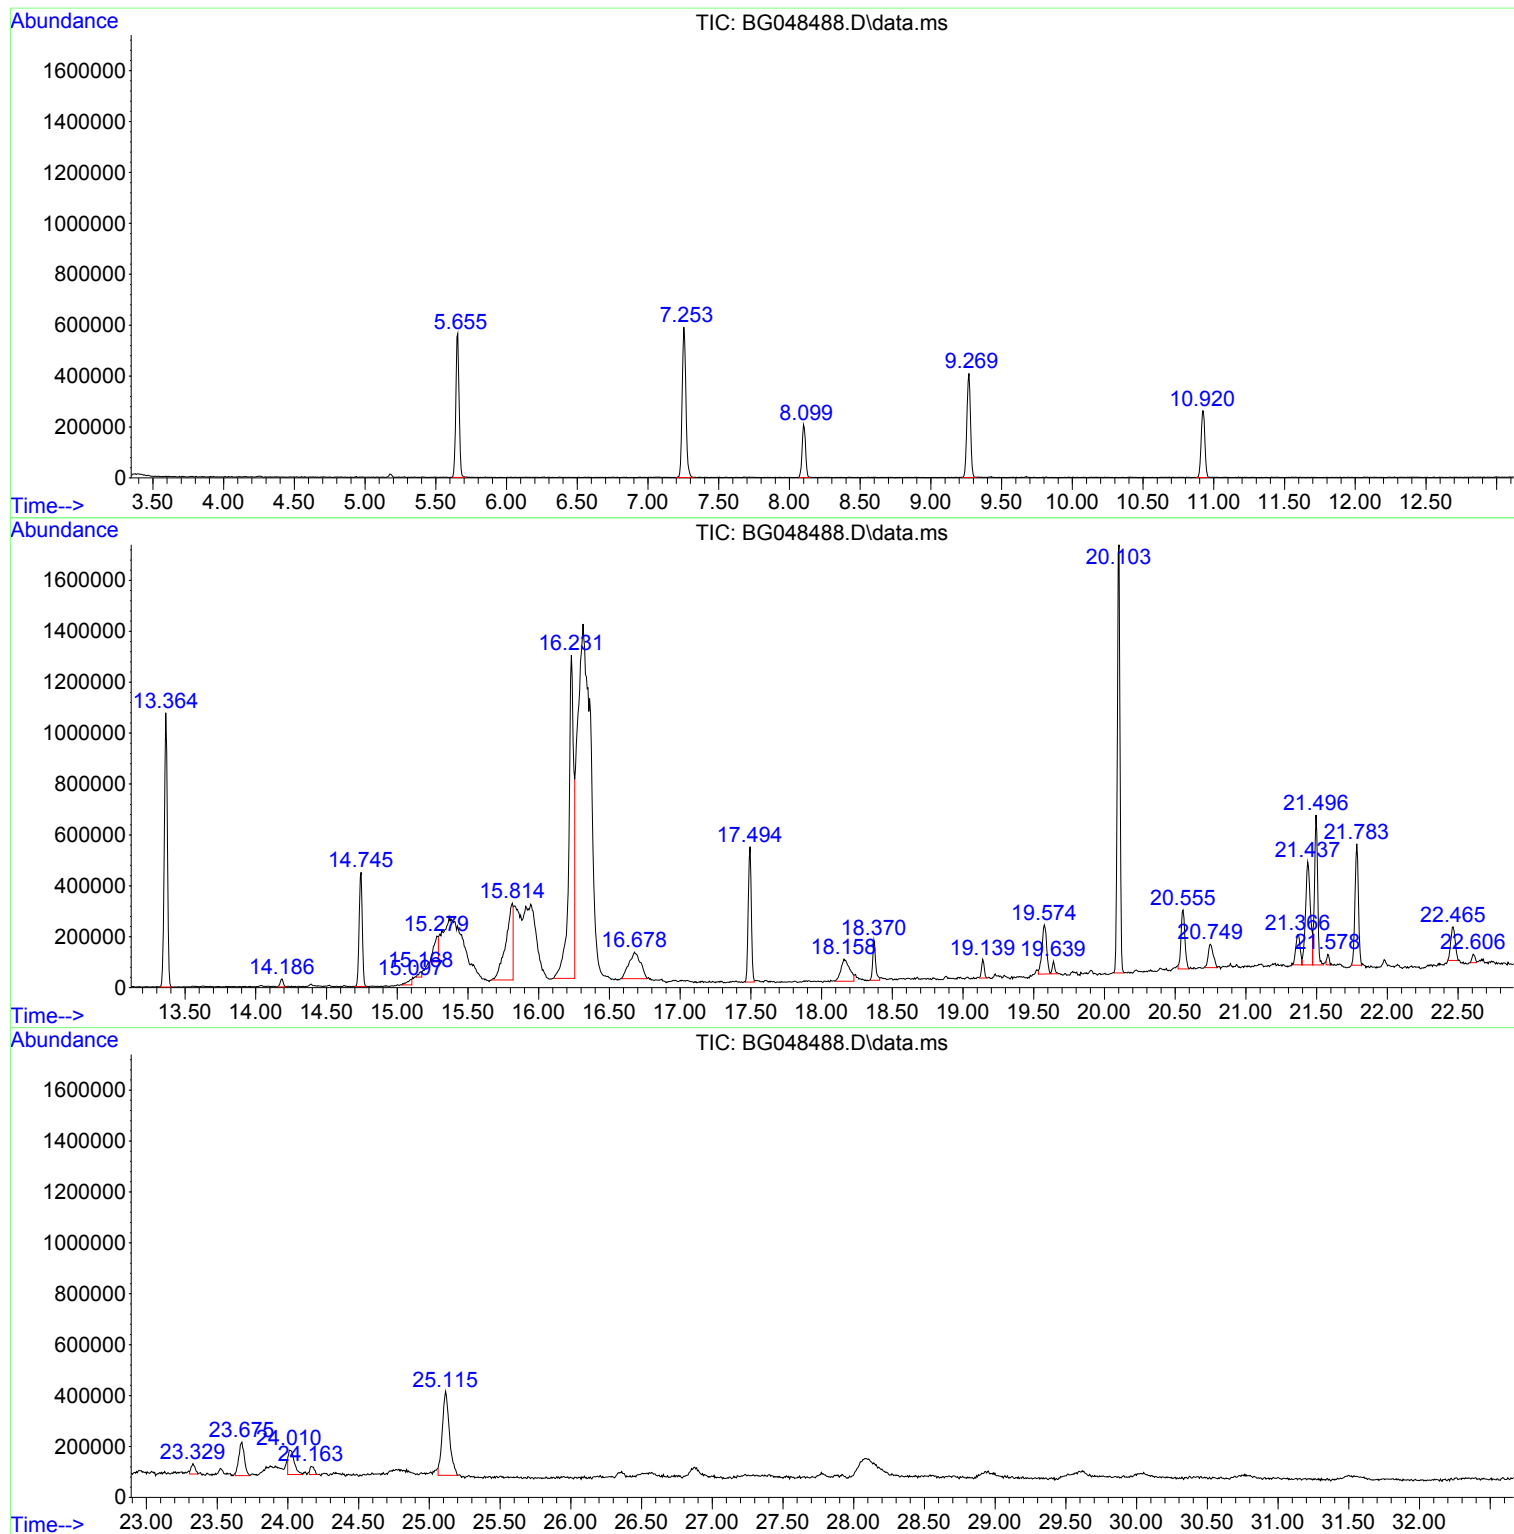

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048488.D
Acq On : 24 Mar 2021 14:15
Operator : CG/JU
Sample : M1718-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048488.D
Acq On : 24 Mar 2021 14:15
Operator : CG/JU
Sample : M1718-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------