
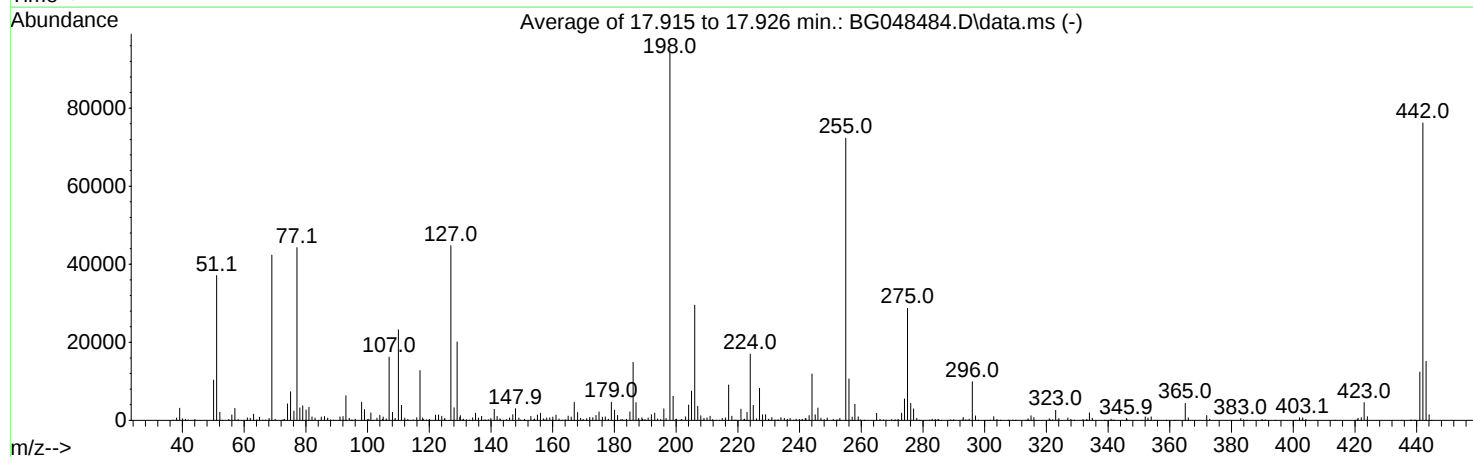


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
 Data File : BG048484.D
 Acq On : 24 Mar 2021 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 24 12:36:47 2021

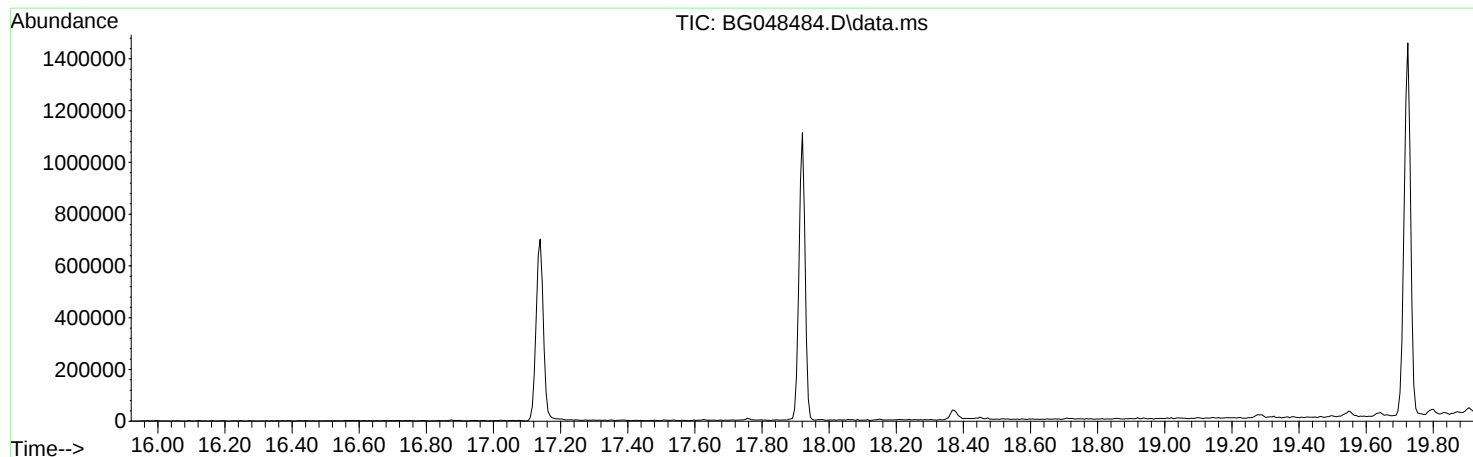




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	37099	PASS
68	69	0.00	2	1.1	476	PASS
69	198	0.00	100	44.9	42364	PASS
70	69	0.00	2	0.7	285	PASS
127	198	10	80	47.5	44757	PASS
197	198	0.00	2	0.5	492	PASS
198	198	100	100	100.0	94261	PASS
199	198	5	9	6.6	6177	PASS
275	198	10	60	30.5	28712	PASS
365	198	1	100	4.6	4359	PASS
441	198	0.01	100	13.2	12397	PASS
442	198	50	100	80.8	76203	PASS
443	442	15	24	19.9	15129	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048484.D
Acq On : 24 Mar 2021 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 25 02:04:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:36:47 2021
Response via : Initial Calibration

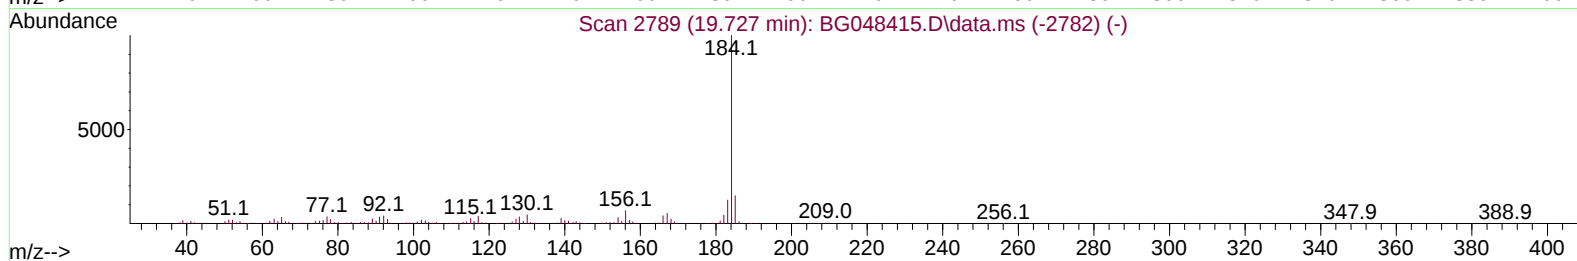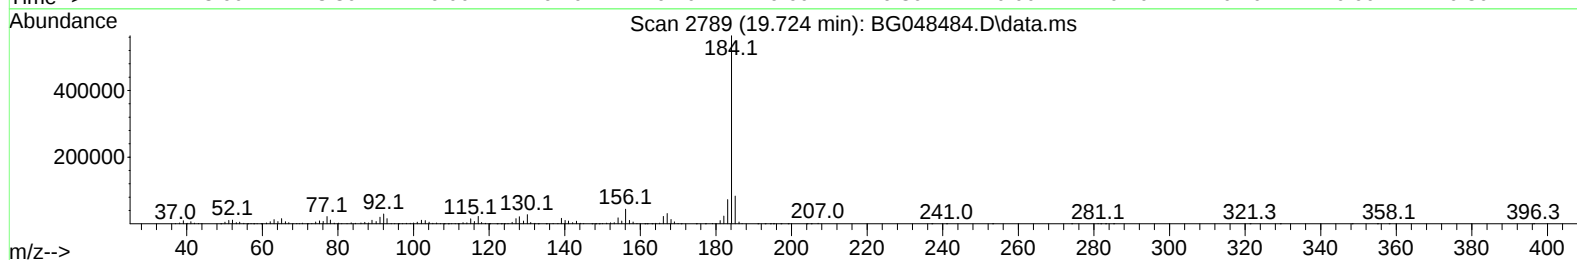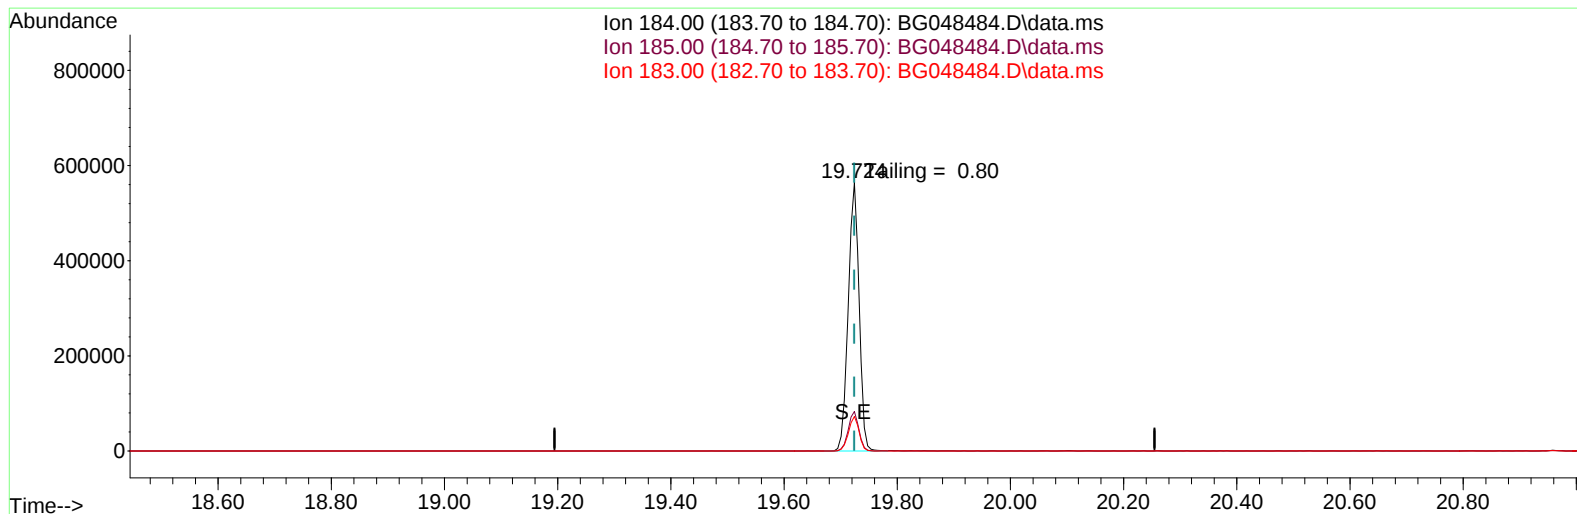

TIC: BG048484.D\data.ms

(77) Benzidine

19.724min (-0.000) 145936.09 ng




response 751896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	12.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032421\
Data File : BG048484.D
Acq On : 24 Mar 2021 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 25 02:04:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:36:47 2021
Response via : Initial Calibration

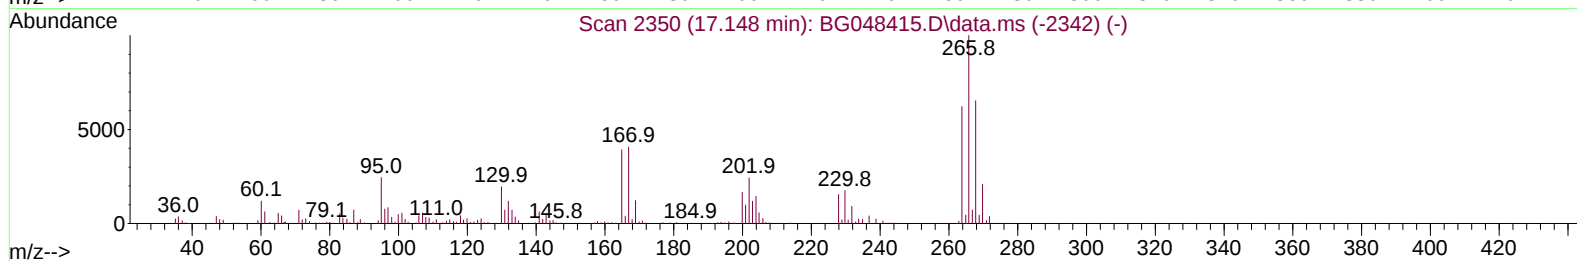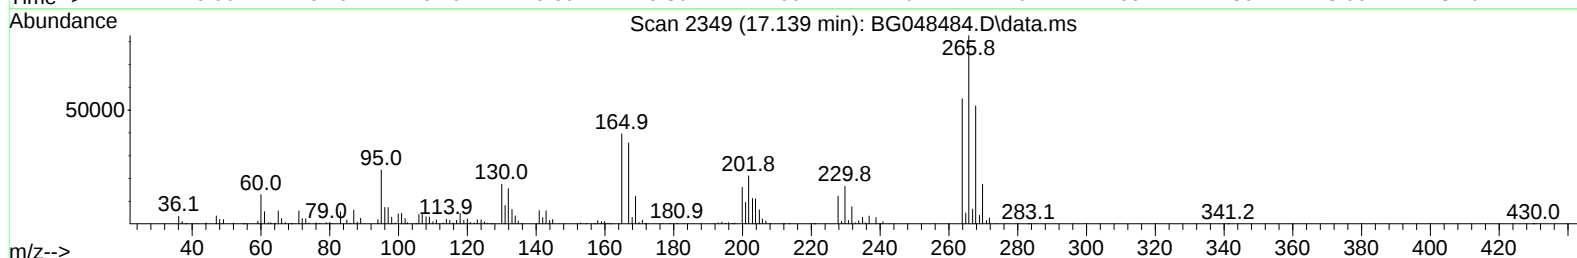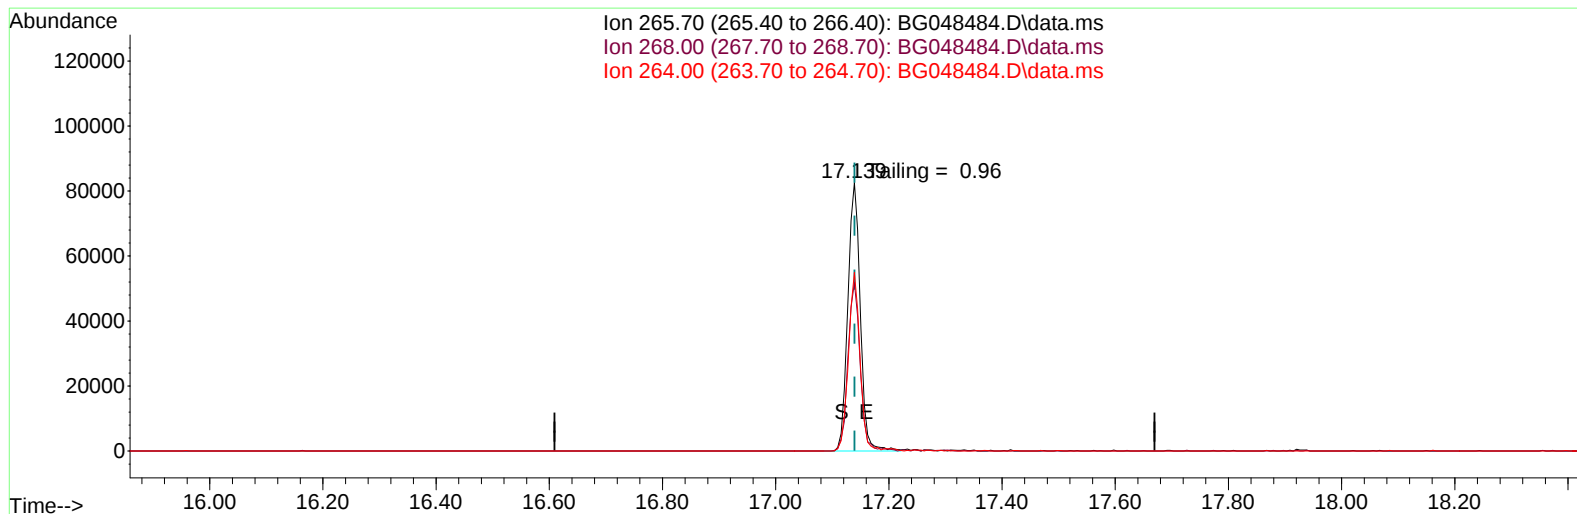

TIC: BG048484.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.000) 15311.74 ng

response 125278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.72
264.00	61.60	66.50
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/24/2021	BNA_G	BG048484.D
Compound Name	Response	Retention Time
DDT	341981	20.958
DDD	1662	20.517
DDE	468	20.018
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2130	344111	0.62