




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052826.D
Acq On : 25 Mar 2022 12:50
Operator : CG/JU
Sample : PB143573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 25 13:50:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

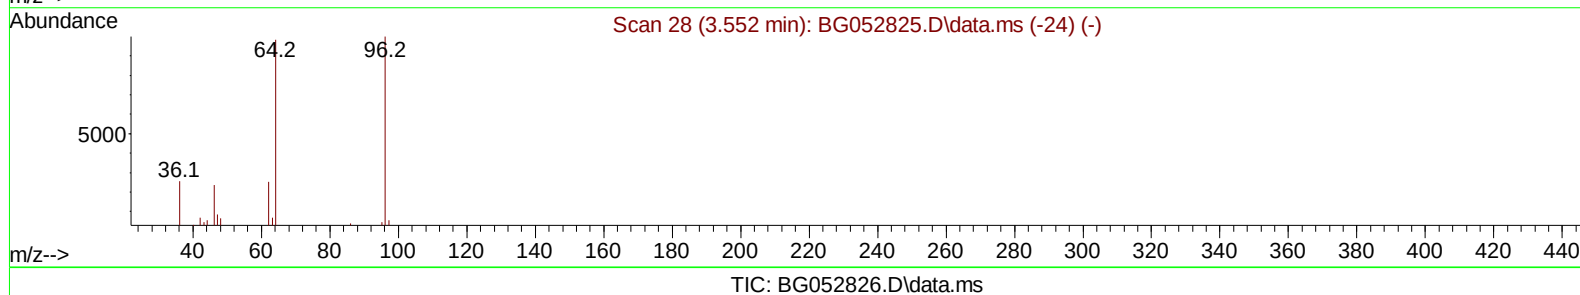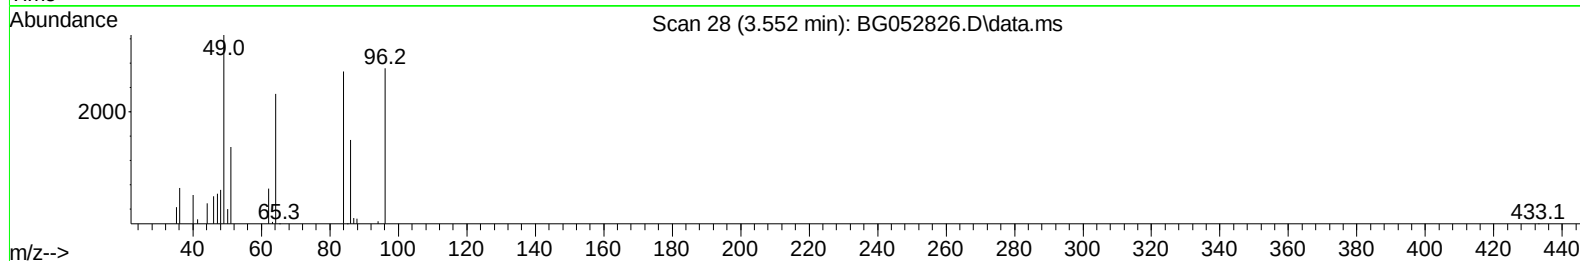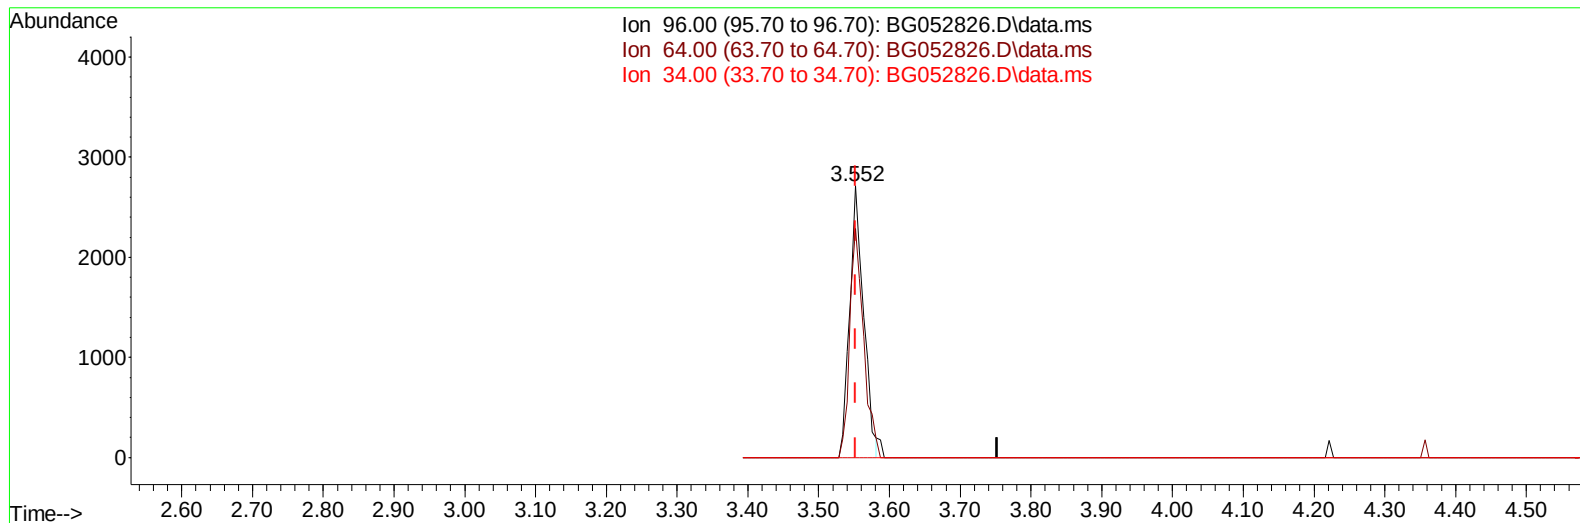**(3) 1,4-Dioxane-d8 (S)**

3.552min (-0.001) 5.98 ng/uL

response 3721

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	84.37
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052826.D
Acq On : 25 Mar 2022 12:50
Operator : CG/JU
Sample : PB143573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 25 13:50:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

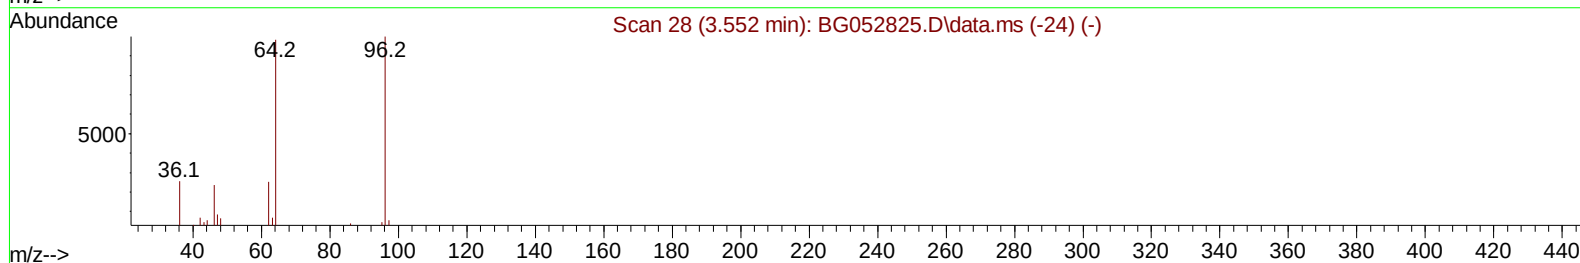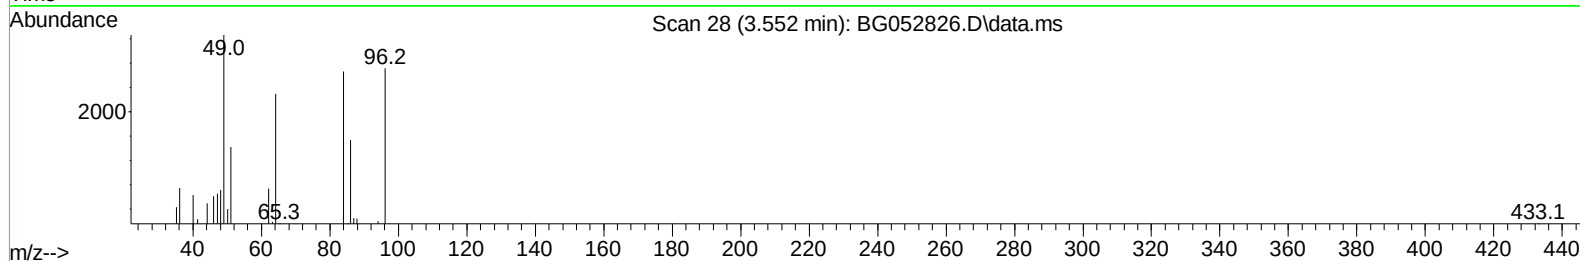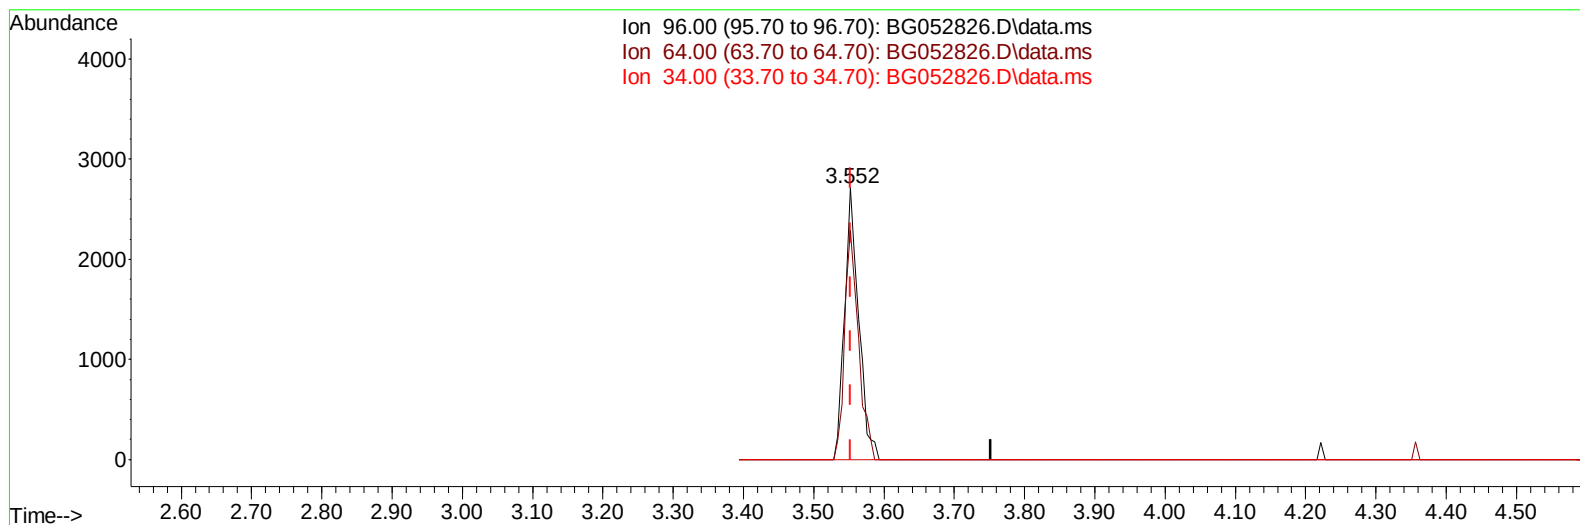

TIC: BG052826.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.552min (-0.001) 6.08 ng/uL m

response 3783

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	84.37
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052826.D
 Acq On : 25 Mar 2022 12:50
 Operator : CG/JU
 Sample : PB143573BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 25 13:50:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.146	152	21974	20.000	ng/ul	0.00
20) Naphthalene-d8	10.954	136	95801	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.760	164	79920	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.504	188	202042	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	221377	20.000	ng/ul	# 0.00
88) Perylene-d12	25.111	264	215082	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.552	96	3783m	6.081	ng/uL	0.00
4) Pyridine-d5	3.969	84	53382	34.372	ng/ul	0.00
7) Phenol-d5	7.288	99	71612	36.386	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	45251	37.645	ng/ul	0.00
11) 2-Chlorophenol-d4	7.670	132	47163	35.292	ng/ul	0.00
15) 4-Methylphenol-d8	8.839	113	53665	37.642	ng/ul	0.00
21) Nitrobenzene-d5	9.303	128	25271	36.645	ng/ul	0.00
24) 2-Nitrophenol-d4	10.025	143	30351	41.727	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.566	165	53537	33.833	ng/ul	0.00
31) 4-Chloroaniline-d4	11.077	131	76844	36.743	ng/ul	0.00
46) Dimethylphthalate-d6	14.161	166	223234	36.358	ng/ul	0.00
49) Acenaphthylene-d8	14.455	160	253825	34.021	ng/ul	0.00
54) 4-Nitrophenol-d4	14.931	143	39434	38.200	ng/ul	0.00
60) Fluorene-d10	15.753	176	191258	35.477	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	35055	34.094	ng/ul	0.00
73) Anthracene-d10	17.603	188	339978	36.136	ng/ul	0.00
81) Pyrene-d10	19.889	212	424205	34.254	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.882	264	402099	36.182	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052826.D
Acq On : 25 Mar 2022 12:50
Operator : CG/JU
Sample : PB143573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 25 13:50:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

