




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052834.D
 Acq On : 25 Mar 2022 18:01
 Operator : CG/JU
 Sample : N2079-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW608

Manual IntegrationsAPPROVED

Quant Time: Mar 26 00:46:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

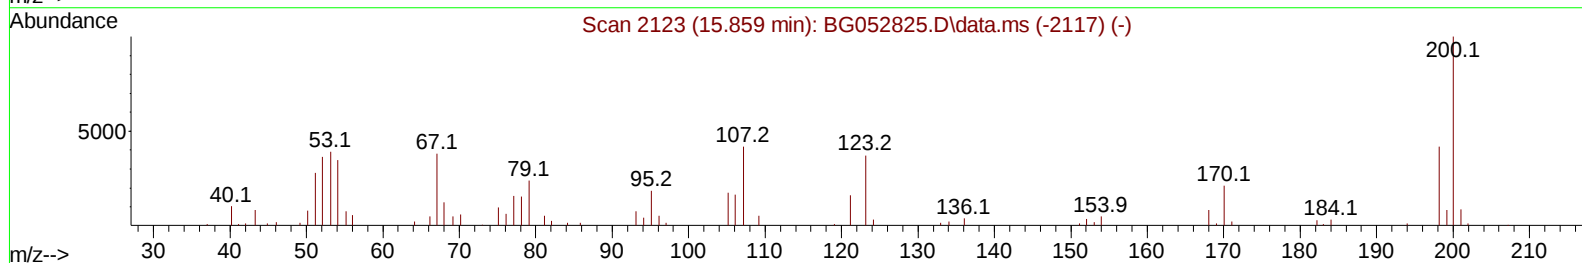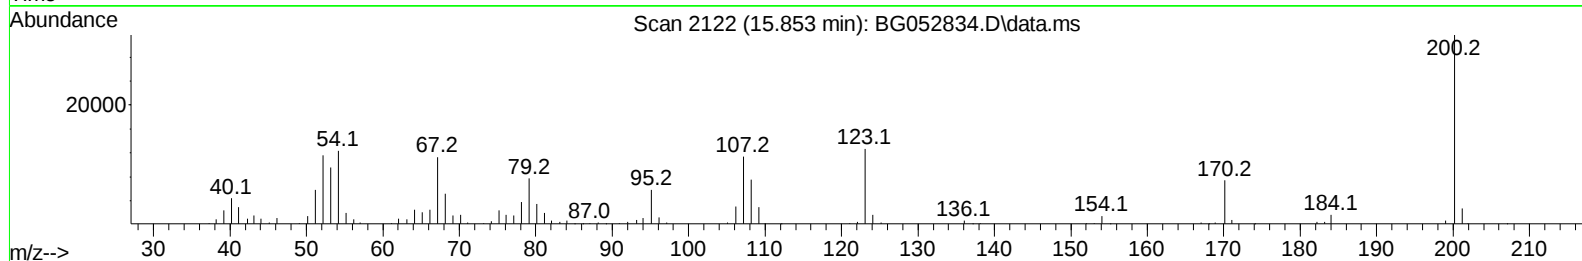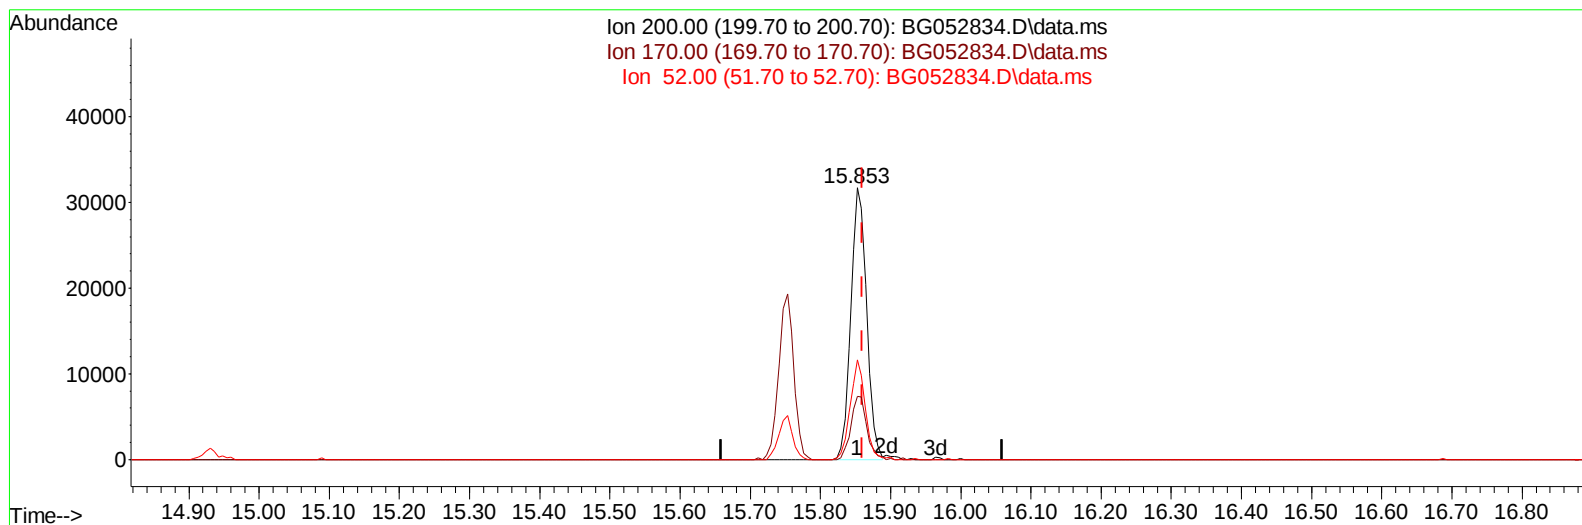

TIC: BG052834.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.853min (-0.007) 37.89 ng/u1

response 49620

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	20.70	23.31
52.00	31.80	36.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052834.D
Acq On : 25 Mar 2022 18:01
Operator : CG/JU
Sample : N2079-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW608

Manual IntegrationsAPPROVED

Quant Time: Mar 26 00:46:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

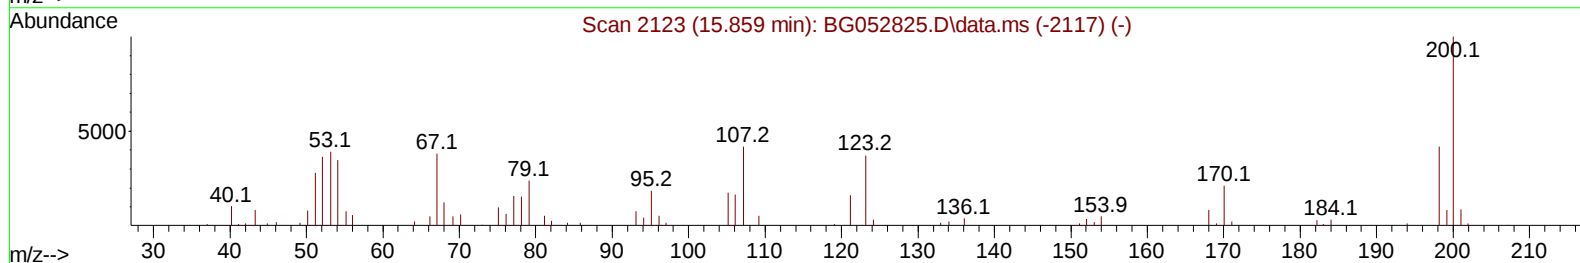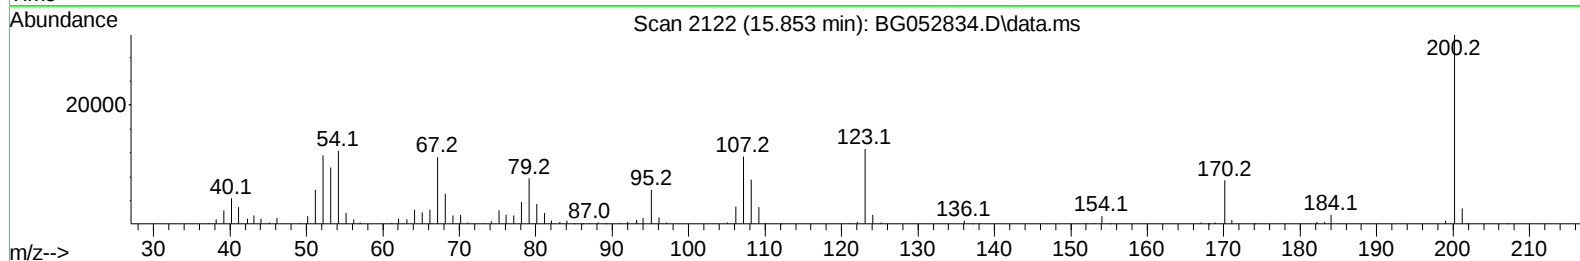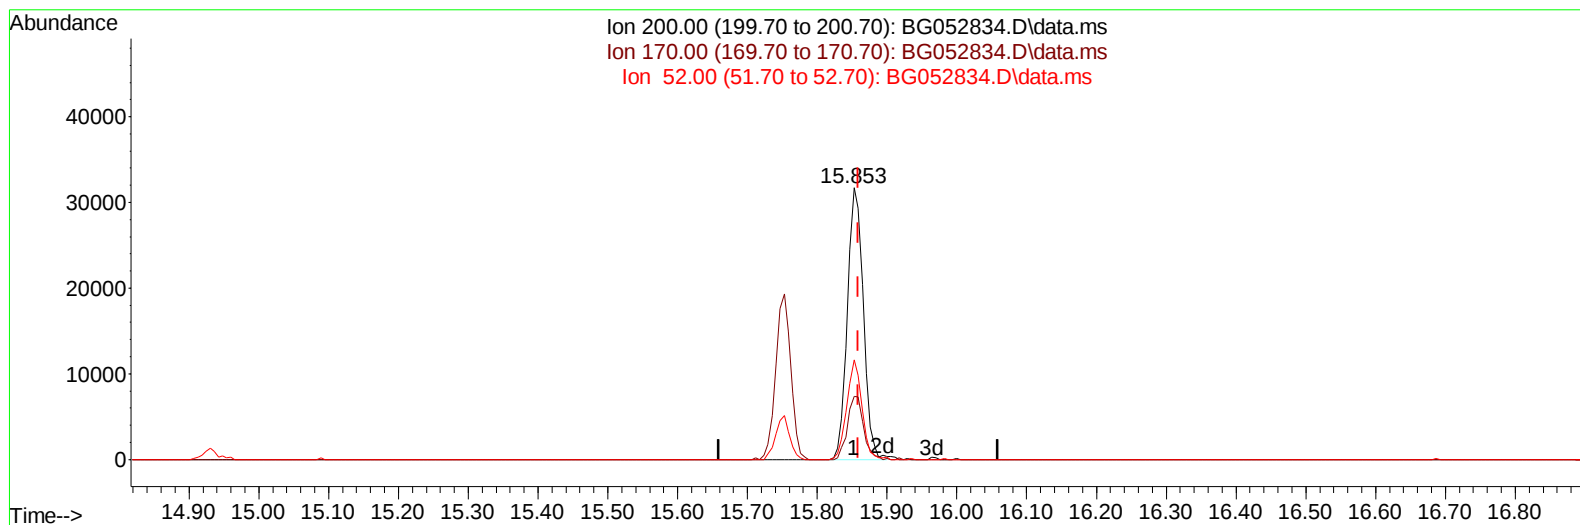

TIC: BG052834.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.853min (-0.007) 38.10 ng/ul m

response 49902

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	20.70	23.31
52.00	31.80	36.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052834.D
 Acq On : 25 Mar 2022 18:01
 Operator : CG/JU
 Sample : N2079-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW608

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 00:46:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	26712	20.000	ng/ul	0.00
20) Naphthalene-d8	10.953	136	128899	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.760	164	102920	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.503	188	257350	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	282804	20.000	ng/ul	0.00
88) Perylene-d12	25.111	264	284347	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.552	96	3521	4.656	ng/uL	0.00
4) Pyridine-d5	3.975	84	14651	7.760	ng/ul	0.00
7) Phenol-d5	7.288	99	18286	7.643	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	55629	38.070	ng/ul	0.00
11) 2-Chlorophenol-d4	7.670	132	45681	28.120	ng/ul	0.00
15) 4-Methylphenol-d8	8.833	113	33366	19.252	ng/ul	0.00
21) Nitrobenzene-d5	9.303	128	33713	36.334	ng/ul	0.00
24) 2-Nitrophenol-d4	10.025	143	36394	37.187	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.566	165	61132	28.713	ng/ul	0.00
31) 4-Chloroaniline-d4	11.077	131	77460	27.527	ng/ul	0.00
46) Dimethylphthalate-d6	14.161	166	272727	34.493	ng/ul	0.00
49) Acenaphthylene-d8	14.455	160	311632	32.435	ng/ul	0.00
54) 4-Nitrophenol-d4	14.936	143	10941	8.230	ng/ul	0.00
60) Fluorene-d10	15.753	176	242264	34.896	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	49902m	38.103	ng/ul	0.00
73) Anthracene-d10	17.603	188	443677	37.023	ng/ul	0.00
81) Pyrene-d10	19.888	212	555167	35.091	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.882	264	555280	37.794	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052834.D
Acq On : 25 Mar 2022 18:01
Operator : CG/JU
Sample : N2079-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW608

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 00:46:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

