




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052843.D
Acq On : 26 Mar 2022 00:30
Operator : CG/JU
Sample : N2079-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z7

Manual IntegrationsAPPROVED

Quant Time: Mar 26 01:21:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

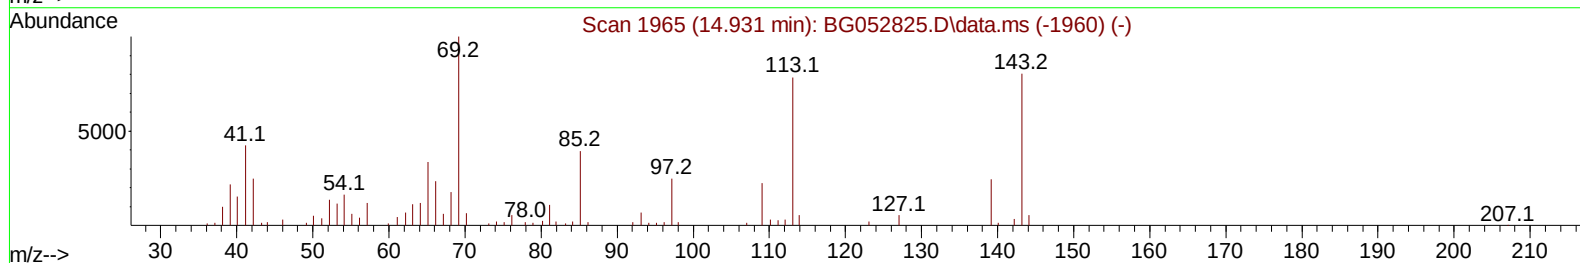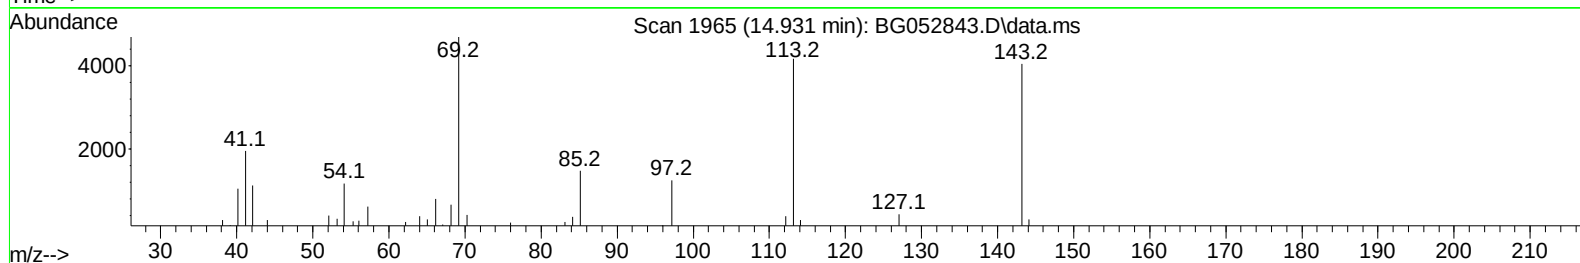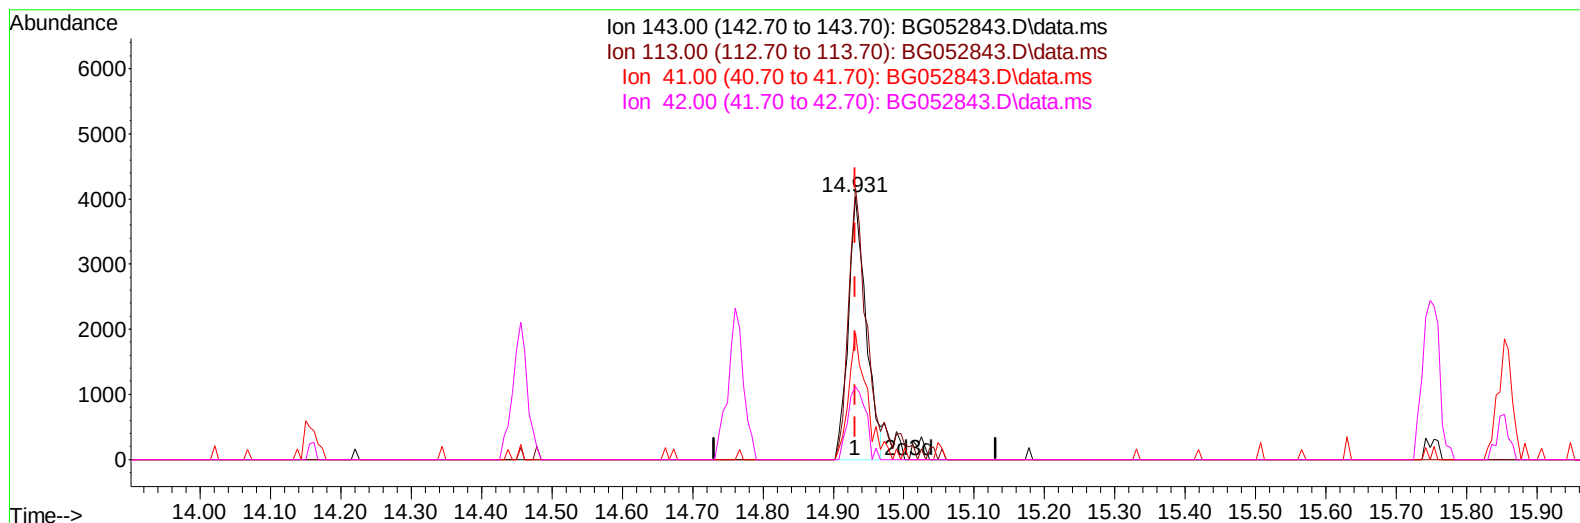

TIC: BG052843.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.931min (+ 0.000) 5.54 ng/ul

response 7055

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	103.32
41.00	47.20	48.20
42.00	29.40	27.71




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052843.D
 Acq On : 26 Mar 2022 00:30
 Operator : CG/JU
 Sample : N2079-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Z7

Manual IntegrationsAPPROVED

Quant Time: Mar 26 01:21:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

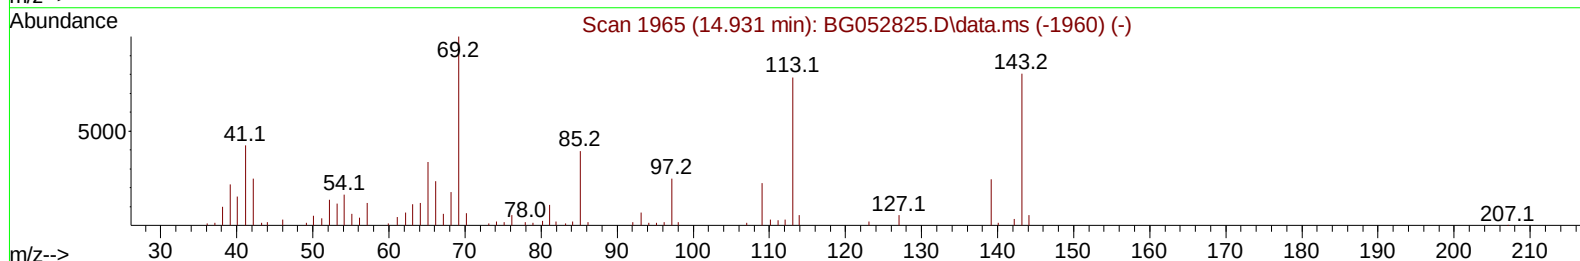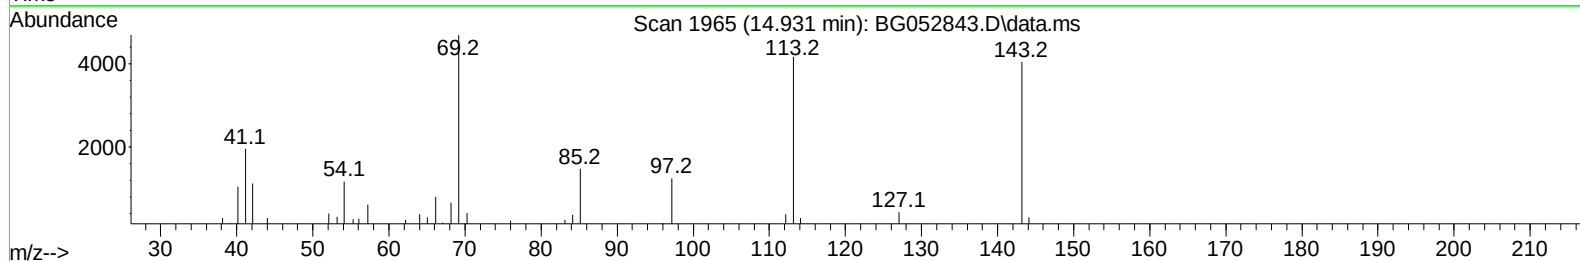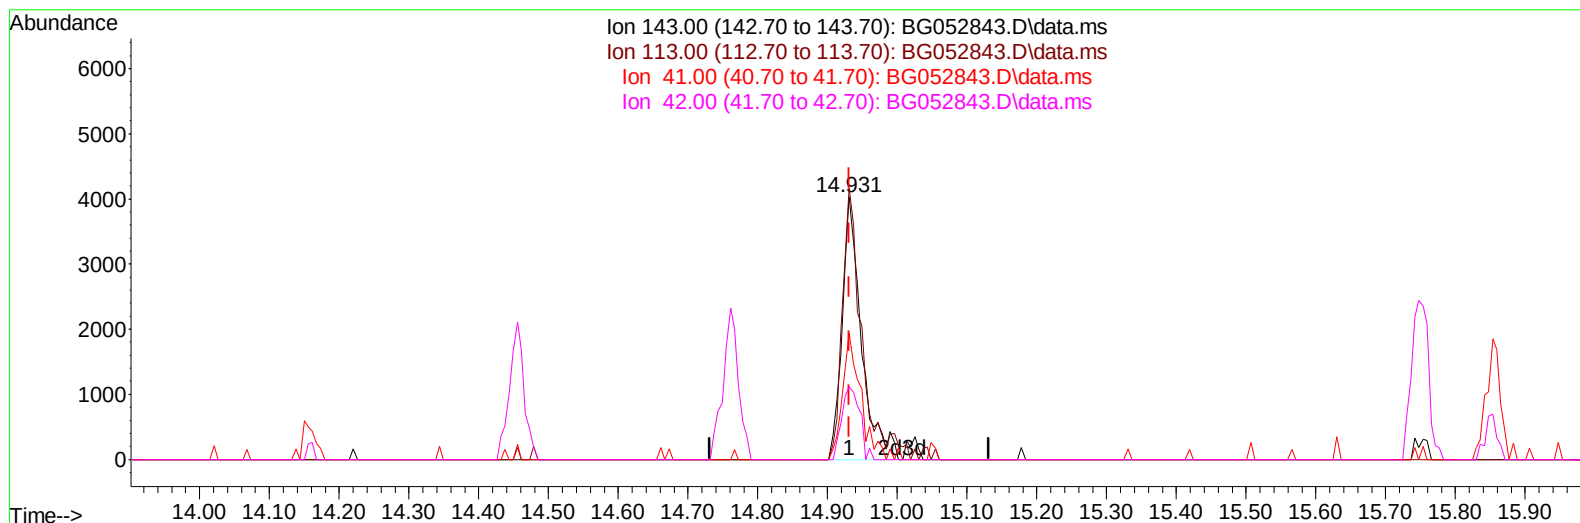

TIC: BG052843.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.931min (+ 0.000) 5.85 ng/ul m

response 7446

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	103.32
41.00	47.20	48.20
42.00	29.40	27.71

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052843.D
 Acq On : 26 Mar 2022 00:30
 Operator : CG/JU
 Sample : N2079-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Z7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 01:21:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.146	152	26092	20.000	ng/ul	0.00
20) Naphthalene-d8	10.954	136	117298	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.761	164	98515	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.504	188	247452	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	280059	20.000	ng/ul	0.00
88) Perylene-d12	25.111	264	278702	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.552	96	3104	4.202	ng/uL	0.00
4) Pyridine-d5	3.975	84	14854	8.055	ng/ul	0.00
7) Phenol-d5	7.283	99	13368	5.720	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.453	67	37942	26.583	ng/ul	0.00
11) 2-Chlorophenol-d4	7.670	132	29768	18.760	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	22453	13.263	ng/ul	0.00
21) Nitrobenzene-d5	9.298	128	20430	24.196	ng/ul	0.00
24) 2-Nitrophenol-d4	10.020	143	24448	27.452	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.566	165	40971	21.147	ng/ul	0.00
31) 4-Chloroaniline-d4	11.078	131	64349	25.130	ng/ul	0.00
46) Dimethylphthalate-d6	14.156	166	185154	24.464	ng/ul	0.00
49) Acenaphthylene-d8	14.455	160	214484	23.322	ng/ul	0.00
54) 4-Nitrophenol-d4	14.931	143	7446m	5.852	ng/ul	0.00
60) Fluorene-d10	15.748	176	169368	25.487	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	32470	25.785	ng/ul	0.00
73) Anthracene-d10	17.604	188	309986	26.902	ng/ul	0.00
81) Pyrene-d10	19.883	212	398240	25.419	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.882	264	387346	26.898	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052843.D
Acq On : 26 Mar 2022 00:30
Operator : CG/JU
Sample : N2079-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 01:21:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

