




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052845.D
Acq On : 26 Mar 2022 1:48
Operator : CG/JU
Sample : N2079-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Y8

Manual IntegrationsAPPROVED

Quant Time: Mar 26 05:02:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

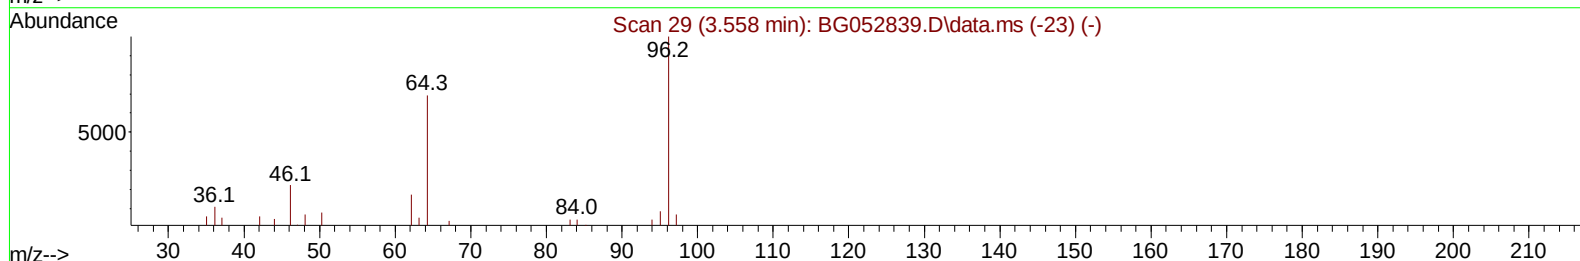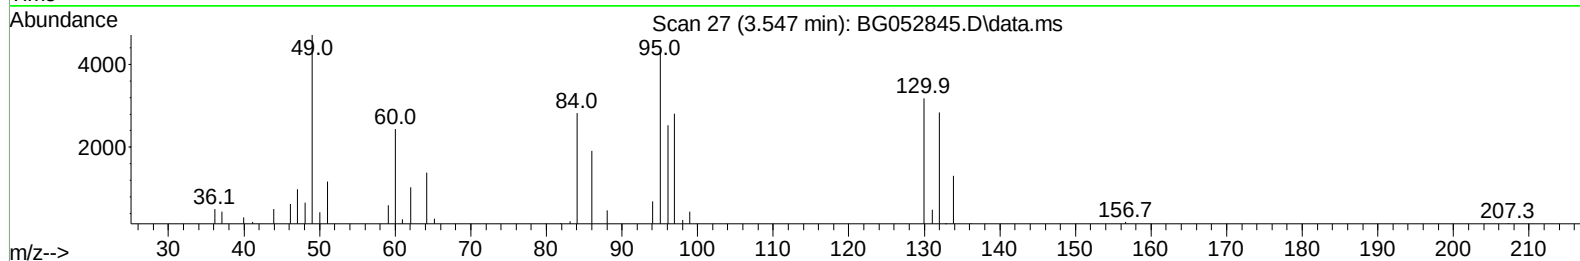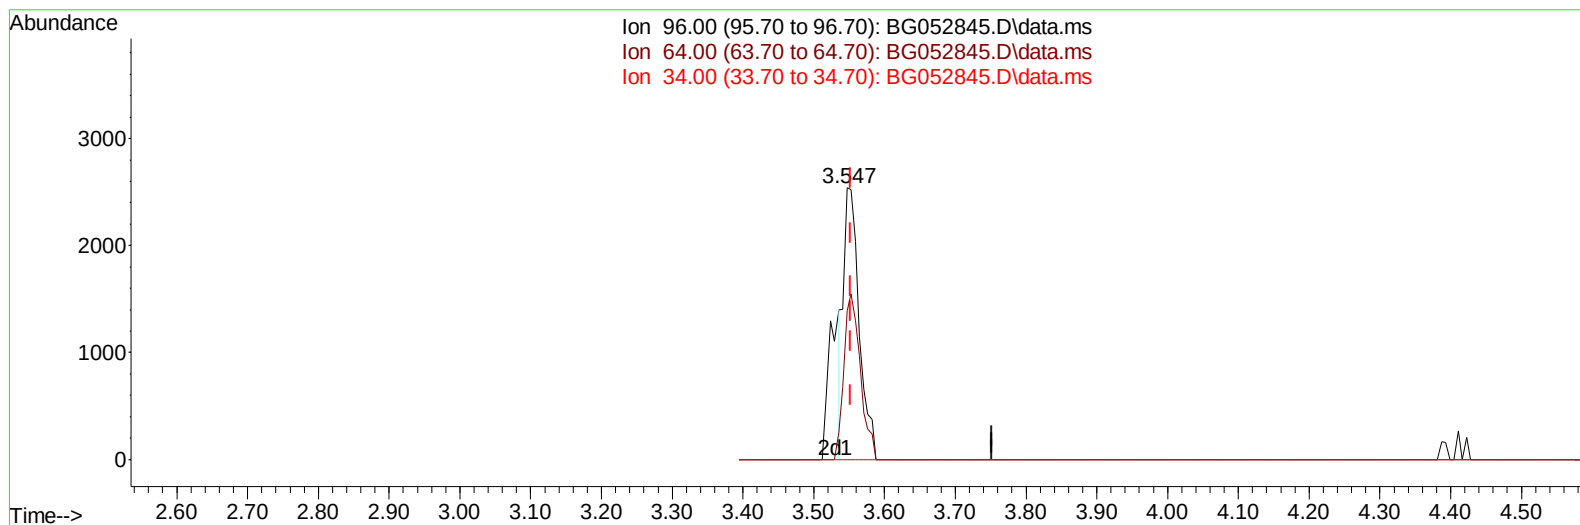

TIC: BG052845.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.547min (-0.005) 4.51 ng/uL

response 3914

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	54.89#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052845.D
Acq On : 26 Mar 2022 1:48
Operator : CG/JU
Sample : N2079-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Y8

Manual IntegrationsAPPROVED

Quant Time: Mar 26 05:02:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

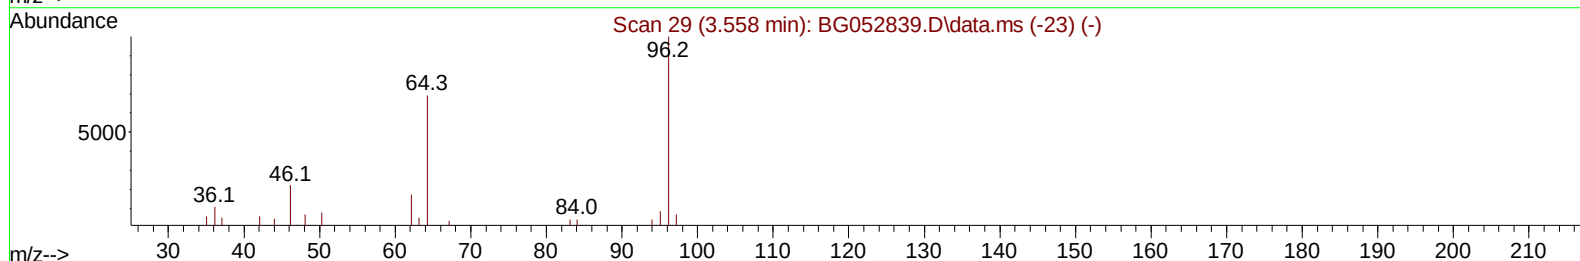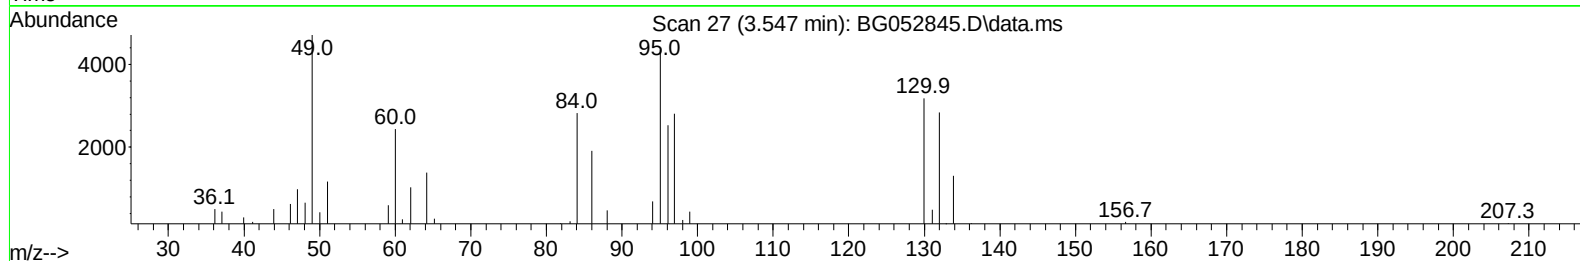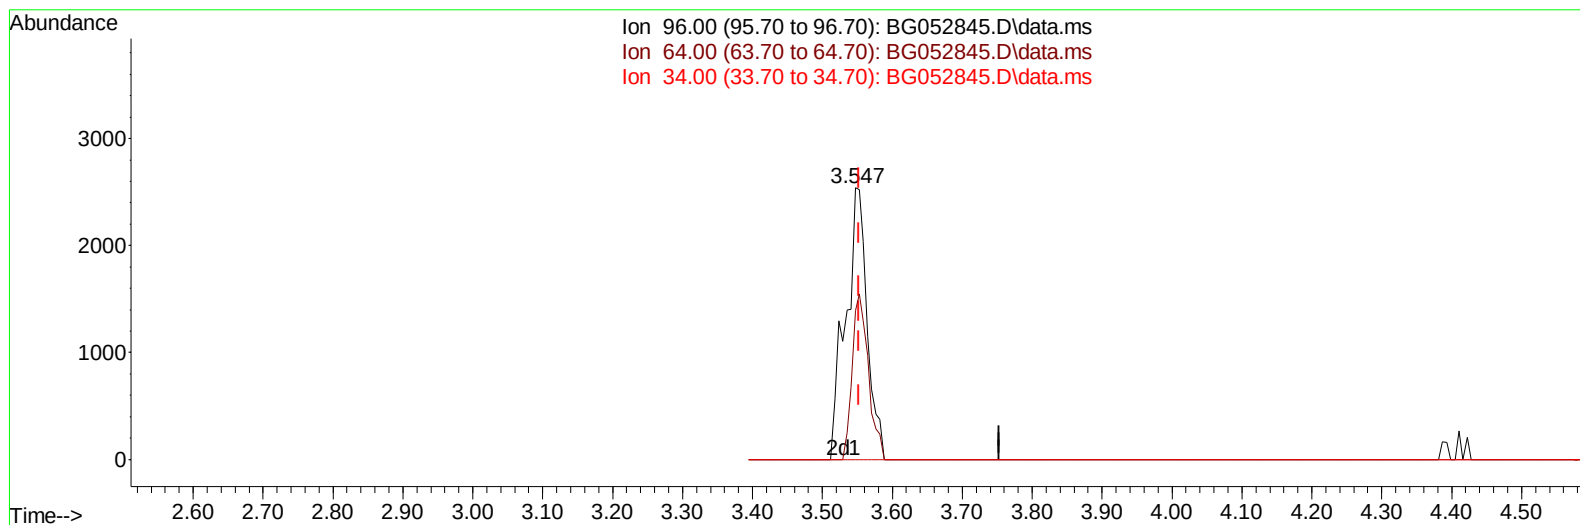

TIC: BG052845.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.547min (-0.005) 6.29 ng/uL m

response 5455

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	54.89#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052845.D
 Acq On : 26 Mar 2022 1:48
 Operator : CG/JU
 Sample : N2079-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Y8

Manual IntegrationsAPPROVED

Quant Time: Mar 26 05:02:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.141	152	30621	20.000	ng/ul	0.00
20) Naphthalene-d8	10.955	136	135102	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.761	164	109726	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.505	188	273112	20.000	ng/ul	0.00
79) Chrysene-d12	21.793	240	304111	20.000	ng/ul	# 0.00
88) Perylene-d12	25.106	264	302493	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	5455m	6.293	ng/uL	0.00
4) Pyridine-d5	3.976	84	17103	7.903	ng/ul	0.00
7) Phenol-d5	7.283	99	21687	7.907	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.459	67	59123	35.296	ng/ul	0.00
11) 2-Chlorophenol-d4	7.671	132	50055	26.879	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	37071	18.660	ng/ul	0.00
21) Nitrobenzene-d5	9.298	128	35490	36.493	ng/ul	0.00
24) 2-Nitrophenol-d4	10.021	143	39478	38.487	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.567	165	69603	31.191	ng/ul	0.00
31) 4-Chloroaniline-d4	11.078	131	93791	31.800	ng/ul	0.00
46) Dimethylphthalate-d6	14.156	166	306580	36.369	ng/ul	0.00
49) Acenaphthylene-d8	14.456	160	349825	34.152	ng/ul	0.00
54) 4-Nitrophenol-d4	14.932	143	12247	8.641	ng/ul	0.00
60) Fluorene-d10	15.754	176	269338	36.389	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.854	200	54822	39.444	ng/ul	0.00
73) Anthracene-d10	17.604	188	466632	36.691	ng/ul	0.00
81) Pyrene-d10	19.884	212	585539	34.418	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.883	264	598967	38.322	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.594	88	3018	2.841	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052845.D
Acq On : 26 Mar 2022 1:48
Operator : CG/JU
Sample : N2079-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Y8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 05:02:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

